




COMPAGNIE GÉNÉRALE DE MÉTROLOGIE

ANNECY

FRANCE

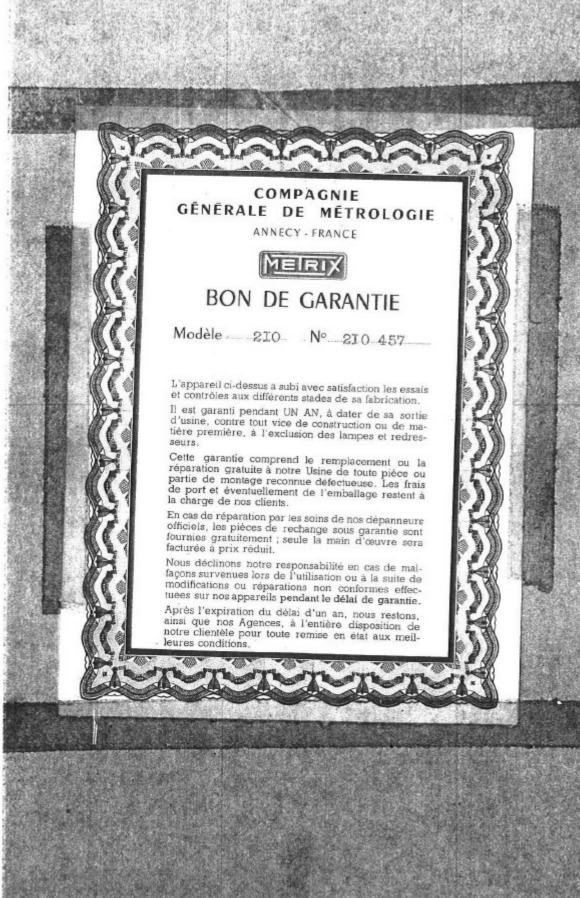

# CONTENTS

		Pa	ges
I -	GENERAL	1	1
II -	DESCRIPTION	1 -	2
III-	WORKING INSTRUCTIONS	2 -	3 - 4
IV -	TECHNICAL CHARACTERISTICS		7
V -	REPLACEABLE PARTS LIST	5 -	6
		1	
		i	

ANNEX: SCHEMATIC DIAGRAM, 210

SCHEMATIC DIAGRAMS, PROBES & FILTER

. . . . .

\* .\*\*

## TELEVISION WOBULATOR Type 210

#### I - GENERAL -

This instrument has been designed for production lines and research on wide band amplifiers such as those used in television and frequency modulation receivers. Its outstanding performance is due to the incorporation of original ideas specially adapted to this new technique.

In particular the range 5 - 220 Mc/s is covered on a single scale without switching. All I.F. stages can therefore be aligned, whatever may be their working frequencies, and so can R.F. and local oscillator stages up to and including 220 Mc/s.

This very wide frequency range is obtained by using the difference in frequency between two oscillators, one being swept about a fixed frequency and the other being unmodulated but variable. Both frequencies are always higher than 220 Mc/s.

A great advantage of this system is that only the wanted frequency can act on the circuit under test, all other frequencies being higher. This result is not possible if the sum of the internal oscillator frequencies is used.

#### Other features are:

Frequency sweeping is obtained by a system of variable permeability. Neither mechanical parts nor electronic tubes are used, this leading to stability and linearity.

The high attenuable output allows the use of any oscilloscope provided with a horizontal amplifier, even if the oscilloscope is not very sensitive or the receiver out of alignment.

#### II - DESCRIPTION -

(See circuit diagram)

A)R.F. group: V2 is an oscillator whose frequency is swept about the fixed frequency of 260 Mc/s. The sweep is obtained by the use of a ferrite core in the oscillator coil. A permanent magnet provides a stable polarizing field which fixes the working point and a coil wound on a stack of A.F. iron stampings provides an alternating field which sweeps the permeability of the ferrite core about the working point. The polarizing field determines the centre frequency and the alternating field, which may be controlled from the front panel, determines the sweep width, 1 to 20 Mc/s in 5 steps.

V 4 is an unmodulated Lecher line oscillator whose frequency is variable from 260 to 480 Mc/s. The line length, hence the frequency, is controlled from the main dial.

V 3 is a mixer to whose grid the outputs of V2 and V4 are fed. The output of V3, which includes the range 5 to 220 Mc/s, is fed to an attenuator whose output impedance is 75 Ohms in all positions.

.../...

## B) Oscilloscope Horizontal sweep .-

Pransformer T 1, which provides the modulation current to the R.F. section, also delivers a voltage whose phase is adjustable with respect to the modulation and which is used the oscilloscope horizontal sweep.

Curves should be taken with the return trace blanked, the R.F. output being suppressed during the return trace.

### C) Power supply -

A normal power supply feeds the oscillators and mixer.

### D) Stray radiation suppression -

The principal screen is that over the R.F. section with filters in all outgoing leads. A second screen is the metal case and front panel with filters in the horizontal sweep output and in the power line.

## III - WORKING INSTRUCTIONS .-

## Overall response curve of a receiver -

Before connecting the power supply make sure that the power supply voltage switch is in the correct position for the power supply in use and that the power supply frequency is 50 - 60 c/s.

Connect the output of the 210 to the input of the receiver under test by means of the unmatched 75 Ohms cable supplied.

Connect the oscilloscope vertical amplifier to the detector load resistance of the receiver.

Connect the oscilloscope horizontal amplifier to binding posts and  $\circ$ 

Set the oscilloscope horizontal amplitude so that the whole of the trace appears on the screen.

Set the TRACE switch to ADJUST.

Set the main dial to the required centre frequency and the SWEEP WIDTH switch to the width required.

The curve may then be made to appear conveniently on the oscilloscope screen by a judicious use of :

the 210 attenuator, the receiver contrast control, and the oscilloscope vertical amplitude control.

The use of these three controls will usually be sufficient to produce a conveniently sized trace without any sign of "noise" or saturation. If, however, the 210 attenuator steps of 10 are too widely spaced the 10 dB coaxial attenuator interposed in the output cable will give intermediate steps.

..../....

-3-

Superpose the forward and return trace curves by means of the ADJUST PHASE control.

Set the trace in the centre of the oscilloscope screen by adjusting the main dial.

If necessary retouch the oscilloscope vertical amplitude control and the phase adjustment.

Set the TRACE switch to RETURN BLANKED to produce a single curve with a base line.

Marker in pass band .-The main dial is engraved in centre frequencies. i.e. the frequency to which the centre of the trace corresponds whenthe phase is correctly set, but generally this is not sufficiently accurate to evaluate frequency and a marker is necessary.

If the output of an unmodulated R.F. generator, the METRIX 936 for instance, is injected into the coaxial MARKER jack a pip appears on the curve traced on the oscilloscope screen. To avoid deforming the curve the marker output should be reduced to the minimum consistent with adequate visibility of the pip, (50 to IOO mV).

If the pip should appear too wide on the curve the pass band of the oscilloscope amplifier should be reduced by connecting a small condenser in parallel with the input. Since the sides of the curve to be observed correspond to relatively long rise times the pip will be redueed in width but the curve will not be deformed.

Remarks .-

Stray radiation by marker.-Under certain conditions when the receiver gain is set to maximum, measurements may be rendered difficult by stray radiation of the swept frequency from the cable connecting the marker generator to the 210.

To avoid this effect disconnect the marker from the 210 and connect an unscreened lead to the marker output.

Bring the open end of this lead near the receiver input.Coupling to the receiver will take place by radiation or stray capacity.

## Use of the coaxial IO dB attenuator .-

The input impedance of certain circuits may be far from the 75 Ohms resistance necessary to match the 210 output cable and, although this may not deform the response curve obtained, the circuit and cable may become sensitive to the approach of the hand. To avoid this state of affairs connect the 10 dB attenuator at the end of the 210 output cable and connect the output of the attenuator to the circuit under test by shortest possible connections.

## Stage by stage measurements.-

Whether the amplifier is stagger tuned or contains over coupled circuits there are times when stage by stage measurements become

necessary. An overall check does not directly reveal which circuit to adjust if the amplifier is out of alignment. Since the circuits of these amplifiers are tuned by extremely small capacities, often stray wiring and interelectrotube capacities, it is impossible to make connections to them without pro-

ducing detuning.

Nevertheless, with the two probes available the 2IO can be used to produce a response curve for un single circuit. The injector probe (see circuit diagram) matches the 2IO output cable and connects to the grid of the tube proceding the circuit under test. The condenser avoids short circuiting any D.O. voltages present whilst the 75 ohms resistance renders the grid circuit. appriodic. The detector probe connects to the plate of the tube following the circuit under test. The condenser blocks any D.C. voltages and the 75 ohms resistance renders this plate circuit aperiodic. By this means the circuit under test is not perturbed and all other tuned circuits are so beavily damped that their response curves cannot disturb the measurement.

#### Use of the filter .-

In a few cases the presence of unwanted frequencies may render an adjustment difficult: this may be so with neutralised R.F. stages or with certain receivers whose image frequency is 260 Me/s (frequency of oscillator V2).

To suppress these unwanted frequencies a low pass filter is available, out-off frequency 230 Mc/s, which is connected in the 210 output cable.

#### Miscellaneous precautions -

Line and frame frequency generators in a television receiver produce high amplitude signals, very rich in harmonics, which may be picked up irectly by the oscilloscope vertical amplifier and its connections.

Where possible it is a good thing to disconnect these generators long as this does not radically change the amplifier B supply voltage.

Another advantage of doing this is that the picture tube high tension isappears and so there is no need for the excessive precautions which therwise are necessary.

IV - TECHNICAL CHARACTERISTICS -Proquency: 5 to 220 Mc/s in one range

ccuracy : That of the marker generator (e.g. METRIX 936)

weep width: 1-2-5-10-20 Mc/s.

inearity: 10 % at sweep width 10 Mc/s.

mplitude modulation : Less than IO % at sweep width IO Mc/s.

owor supply: IIO - I3O - 220 V, 50 - 60 c/s

130 V may be replaced by 160 V ) on demand: 220 V. may be replaced by 240

ower input : 35 VA approx.

ubos usod: 2 x EC 81 - 1 x 6 J 6 - 1 x 6 x 4.


oight : 20 1bs 8 ozs (9,300 Kg)


imensions: 20 x 11 1/2 x 7 5/8 ins.(510 x 295 x 195 mm) overall


# REPLACEABLE PARTS LIST


Symbol	Value	DESCRIPTION	METRIX PART NO
RRRRRRRRRRRRRRRRRRRRRRRRRRRRRRRRRRRRRR	IKR 0,IMQ 70KR 20KR 75KR 10KR 300R	RESISTANCES  + 5 % PE IO MCB  1/2 W. IO %  1/2 W. IO %  1 W. IO %  I W. IO %  I W. IO %  I W. IO %  I/2 W. IO %  I/2 W. IO %  I/2 W. IO %  I/2 W. IO %	
R IO R II R I2 R I3 R I4 R I5 R I6 R I7 R I8 R I9 R 20 R 21 R 22	371 \( \text{371 \text{\alpha}} \) 371 \( \text{\alpha} \) 371 \( \text{\alpha} \) 371 \( \text{\alpha} \) 371 \( \text{\alpha} \) 41 \( \text{\alpha} \) 45,8 \( \text{\alpha} \) 200 \( \text{\alpha} \) 1 \( \text{\alpha} \) 2 \( \text{\alpha} \) 2 \( \text{\alpha} \)	I/4 W. I % I/2 W. I % I/4 W. I %	UE 29
		POTENTIOMETER	
R 2	50 KΩ	ALTER Type VC 45 CONDENSERS	UA 60
123456789112345678911234567	IS µF IS µF IS µF Filter 30.000 pF approx. I µF approx. O,5 µF Filter Filter Filter Filter Filter Filter Filter IS pF I,8 pF Filter IO00 pF 50 pF Filter	Electrolytic 500-550 v Electrolytic 500-550 v Mica Paper 500/I500 V Paper 500/I500 V IO % Paper 500/I500 V Mica Mica Mica Mica Mica Mica Mica Mica	


Symbol	Value	Description	METRIX PART N
		TRANSFORMER	
TI		Power supply	LA 87
		FILTERS	
L Z		Power supply Power supply	LC 46 LC 46
		Oscillo swoop	LC 8I LC 46
L 3 L 4 L 5 L 7		R. F. R. F.	LC 46 LC 46
L 7 L 8		R. F. R. F.	LC 46 LC 46
ь 9		SWEEP WIDTH	LB 27
		SWITCHES	
A B	8	Power supply	KE 70
C		Sweep width Attenuator	KE 93 KE 74
		FUSE	
FI	I.5 A		AA 44
		TUBES	
A 5	6 B X 4 (6 X 4) E C 8I	Rectifier Swopt oscillator	
V 2 V 3 V 4	E C 8I 6 J 6 E C 8I	Mixer Variable oscillator	
	2 0 01	TOT ECOLO OBOLLETOOL	

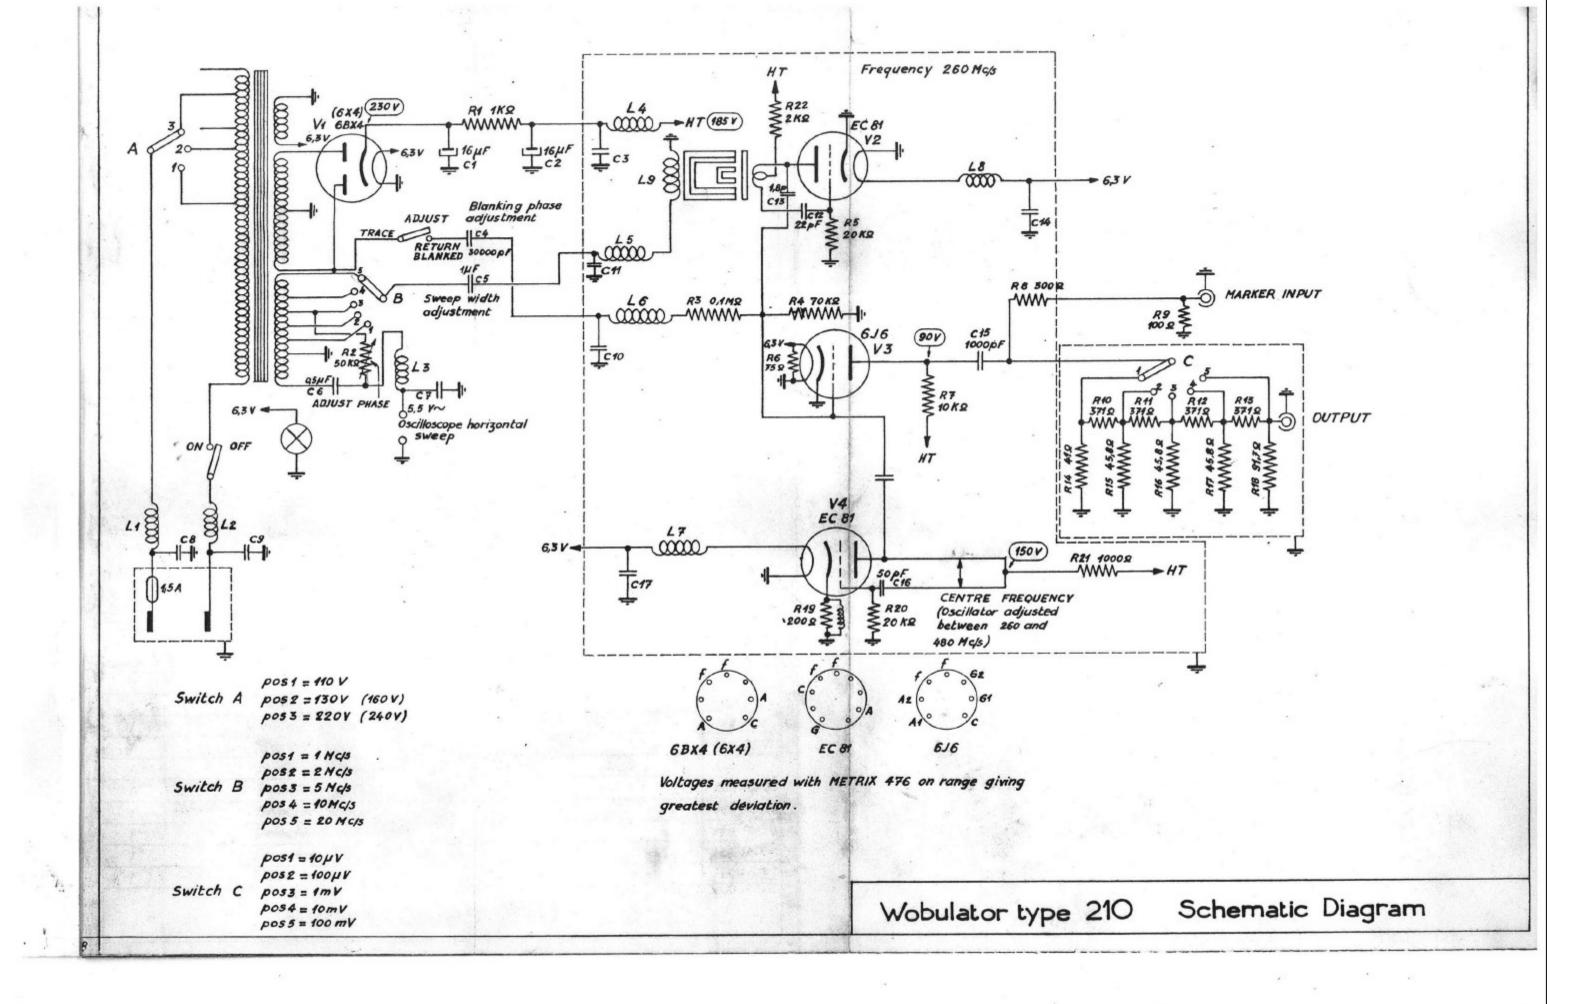










10 dB Attenuator

Low.pass Filler, fo = 230 Mc/s

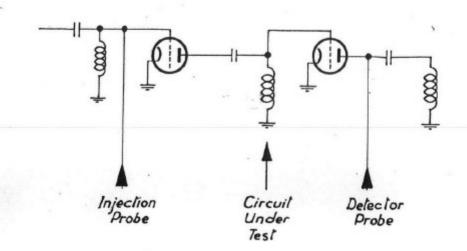

	LIST OF ACCESSORIES		
Quantity	Designation	Melirix Nº	
1	Webulator Type 210		
1	Power cord	AG I	
1	Output cable	HB 73	
1	Morker cable	HB 73	
1.	10 dB attenuator	AA 92	
1	Injection probe	HA 164	
1	Defector probe	HA 165	
1	Delector probe cable	HA 166	
1	Low_pass filler, fo = 230 Mc/s	HA 167	
1	Filler coble	HA 168	

Accessories 210