

KA311


Single Comparator

Features


- Low input bias current : 250nA (Max)
- Low input offset current : 50nA (Max)
- Differential Input Voltage : $\pm 30V$
- Power supply voltage : single 5.0V supply to $\pm 15V$.
- Offset voltage null capability.
- Strobe capability.

Description


The KA311 series is a monolithic, low input current voltage comparator. The device is also designed to operate from dual or single supply voltage.

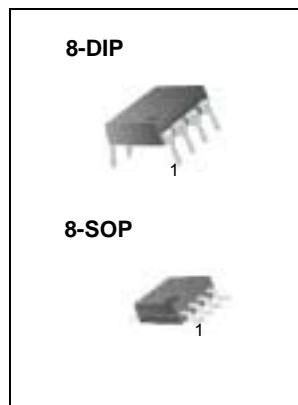

Internal Block Diagram

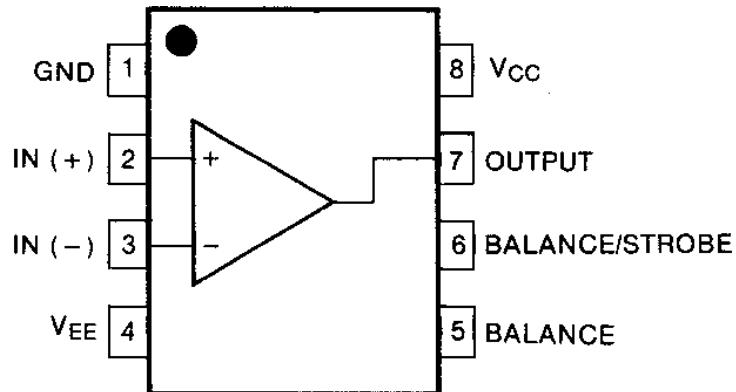

Schematic Diagram

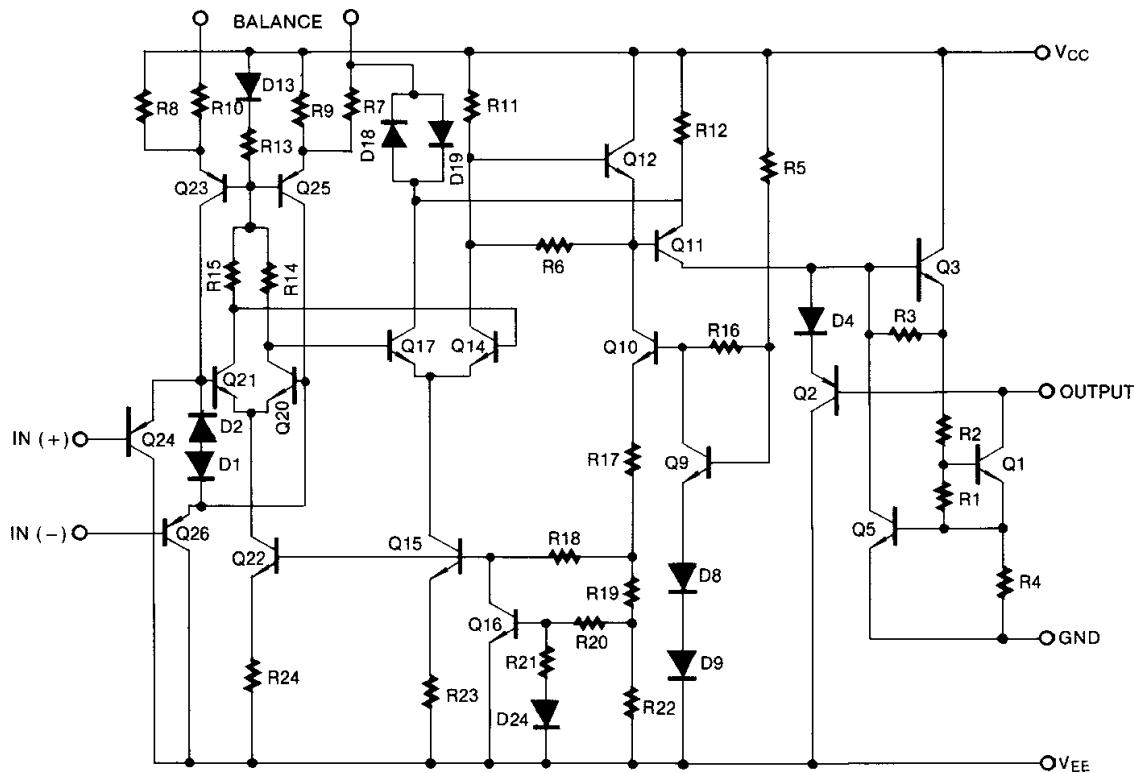

Absolute Maximum Ratings

Parameter	Symbol	Value	Unit
Total Supply Voltage	V _{CC}	36	V
Output to Negative Supply Voltage KA311	V _O - V _{EE}	40	V
Ground to Negative voltage	V _{EE}	-30	V
Differential Input Voltage	V _{I(DIFF)}	30	V
Input Voltage	V _I	±15	V
Output Short Circuit Duration	-	10	sec
Power Dissipation	P _D	500	mW
Operating Temperature Range	T _{OPR}	0 ~ +70	°C
Storage Temperature Range	T _{STG}	- 65 ~ +150	°C

Electrical Characteristics

(VCC = 15V, TA = 25°C, unless otherwise specified)

Parameter	Symbol	Conditions	Min.	Typ.	Max.	Unit	
Input Offset Voltage	VIO	$R_S \leq 50K\Omega$	-	1.0	7.5	mV	
			Note 1	-	-		
Input Offset Current	IIO		-	6	50	nA	
			Note 1	-	-		
Input Bias Current	IBIAS		-	100	250	nA	
			Note 1	-	-		
Voltage Gain	GV	-	40	200	-	V/mV	
Response Time	TRES		Note 2	-	200	-	ns
Saturation Voltage	VSAT	$I_O = 50mA, V_I \leq -10mV$	-	0.75	1.5	V	
		$V_{CC} \geq 4.5V, V_{EE} = 0V$ $I_O = 8mA, V_I \leq -10mV,$	Note 1	-	0.23		
Strobe "ON" Current	ISTR(ON)	-	-	3	-	mA	
Output Leakage Current	ISINK	$I_{STR} = 3mA, V_I \geq 10mV$ $V_O = 15V, V_{CC} = \pm 15V$	-	0.2	50	nA	
Input Voltage Range	VI(R)	Note 1	-14.5 to 13.0	-14.7 to 13.8	-	V	
Positive Supply Current	ICC	-	-	3.0	7.5	mA	
Negative Supply Current	IEE	-	-	-2.2	-5.0	mA	
Strobe Current	ISTR	-	-	3	-	mA	

Notes :

1. $0 \leq T_A \leq +70^\circ C$
2. The response time specified is for a 100mV input step with 5mV over drive.

Typical Performance Characteristics

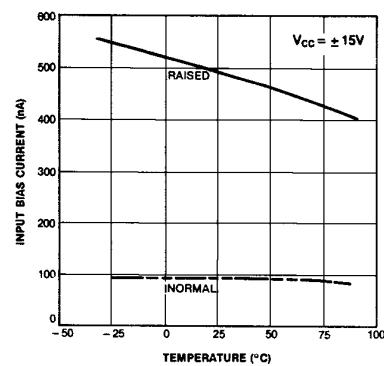


Figure 1. Input Bias Current vs Temperature

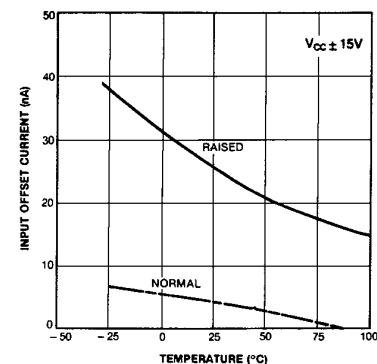


Figure 2. Input Offset Current vs Temperature

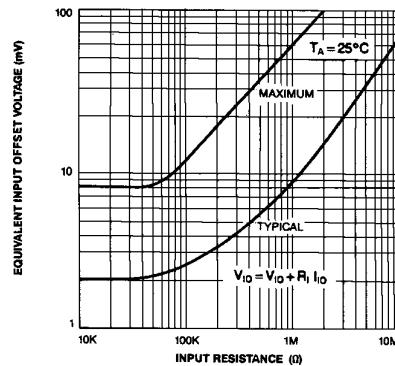


Figure 3. Offset Voltage vs Input Resistance

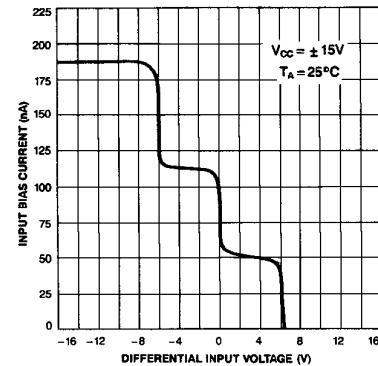


Figure 4. Input Bias Current vs Differential input voltage

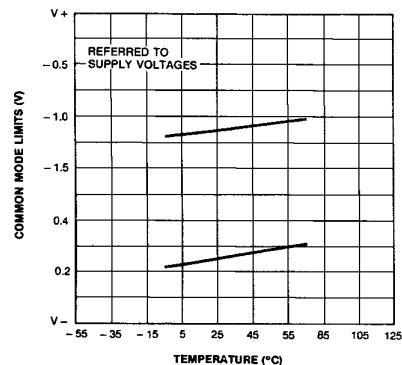


Figure 5. Common Mode Limits vs Temperature

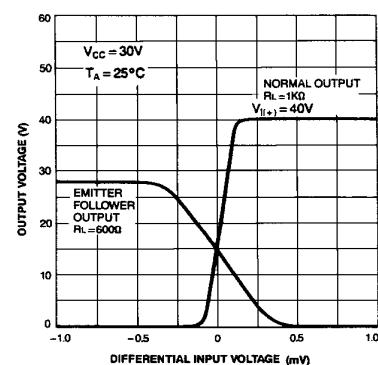


Figure 6. Output Voltage vs Differential input voltage

Typical Performance Characteristics (continued)

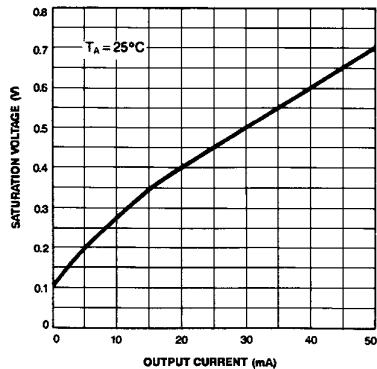


Figure 7. Saturation voltage vs Current

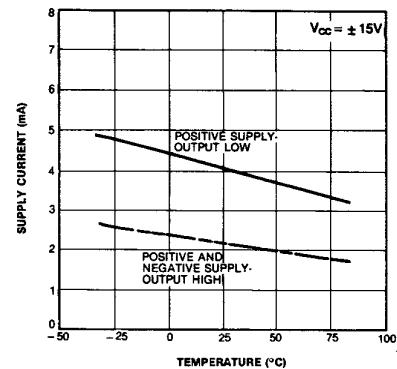


Figure 8. Supply Current vs Temperature

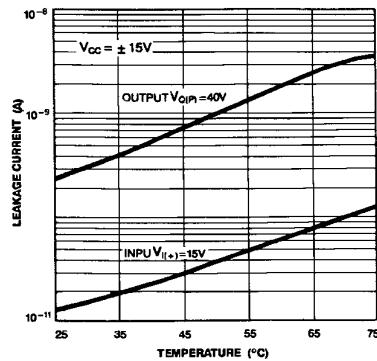


Figure 9. Leakage Current vs Temperature

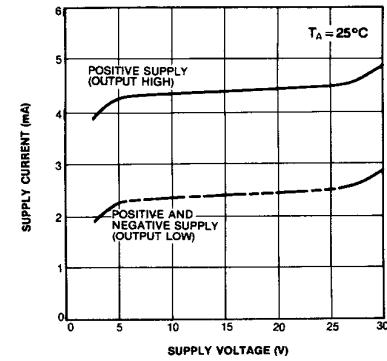


Figure 10. Supply Current vs Supply Voltage

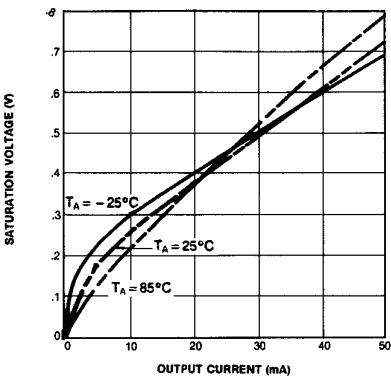


Figure 11. Current Saturation Voltage


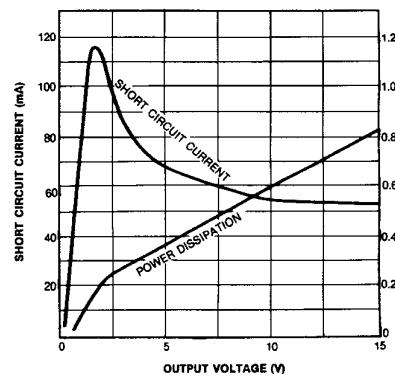


Figure 12. Output Limiting Characteristics


Mechanical Dimensions

Package

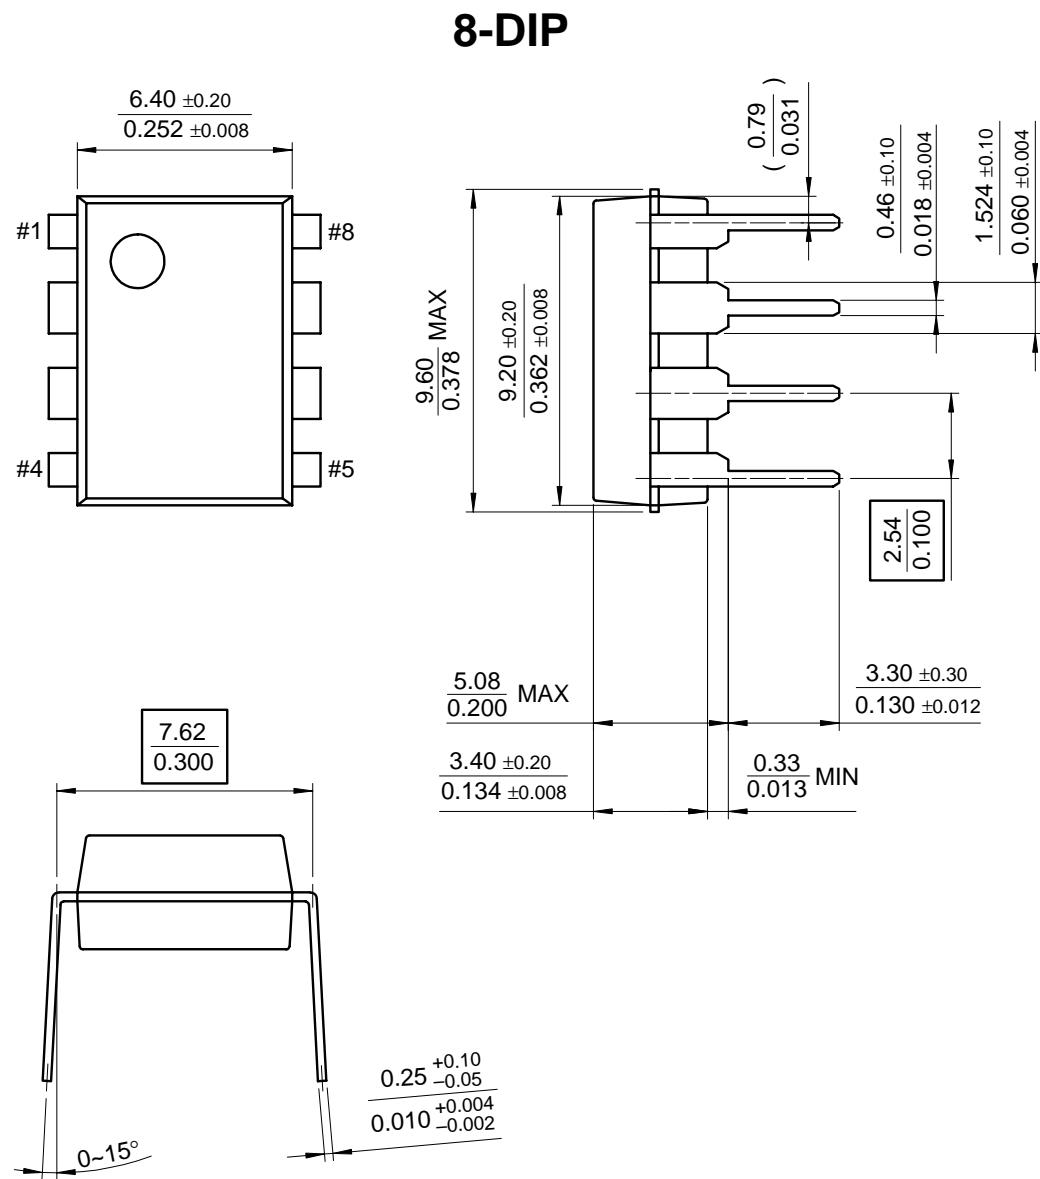

Mechanical Dimensions (Continued)

Package

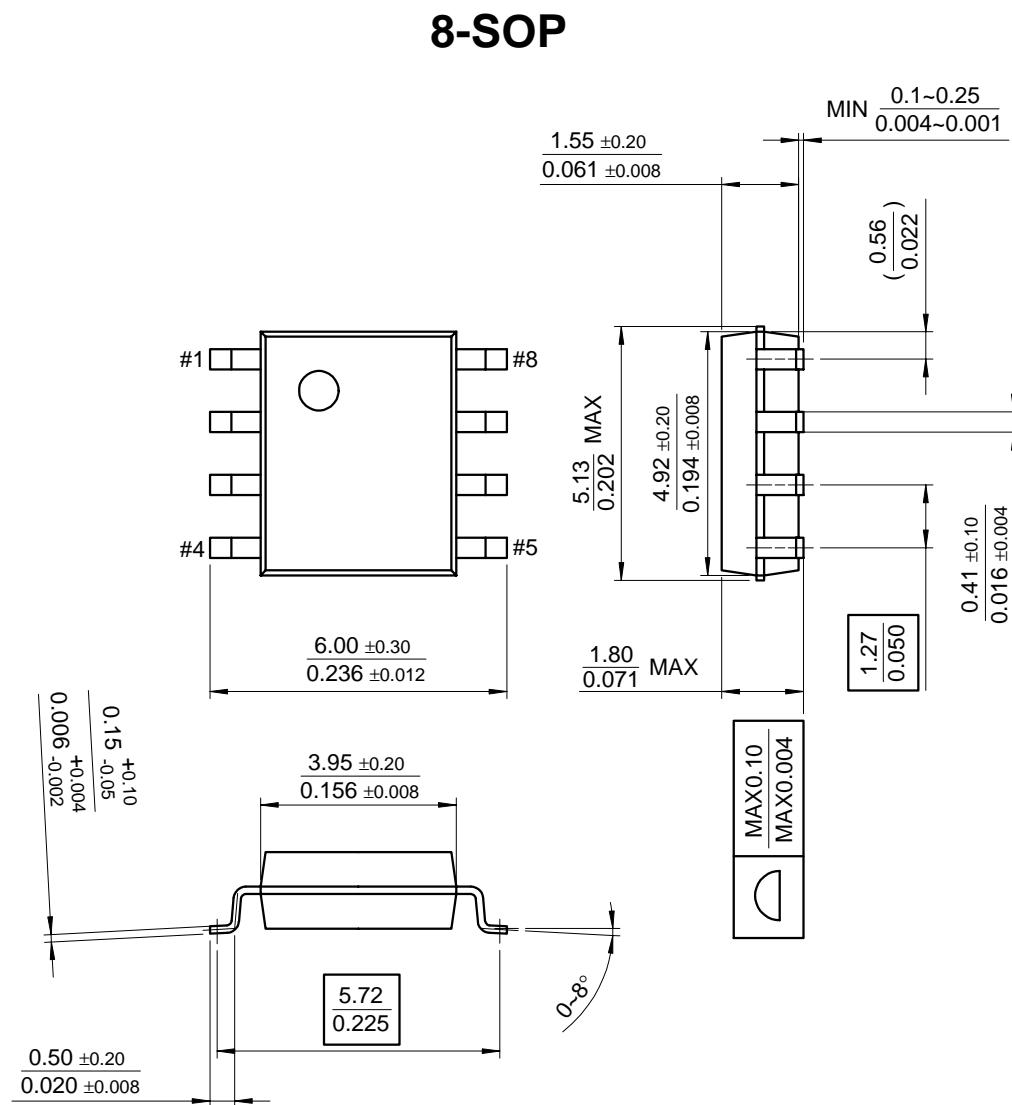

Ordering Information

Product Number	Package	Operating Temperature
KA311	8-DIP	0 ~ +70°C
KA311D	8-SOP	

DISCLAIMER

FAIRCHILD SEMICONDUCTOR RESERVES THE RIGHT TO MAKE CHANGES WITHOUT FURTHER NOTICE TO ANY PRODUCTS HEREIN TO IMPROVE RELIABILITY, FUNCTION OR DESIGN. FAIRCHILD DOES NOT ASSUME ANY LIABILITY ARISING OUT OF THE APPLICATION OR USE OF ANY PRODUCT OR CIRCUIT DESCRIBED HEREIN; NEITHER DOES IT CONVEY ANY LICENSE UNDER ITS PATENT RIGHTS, NOR THE RIGHTS OF OTHERS.

LIFE SUPPORT POLICY

FAIRCHILD'S PRODUCTS ARE NOT AUTHORIZED FOR USE AS CRITICAL COMPONENTS IN LIFE SUPPORT DEVICES OR SYSTEMS WITHOUT THE EXPRESS WRITTEN APPROVAL OF THE PRESIDENT OF FAIRCHILD SEMICONDUCTOR CORPORATION. As used herein:

1. Life support devices or systems are devices or systems which, (a) are intended for surgical implant into the body, or (b) support or sustain life, and (c) whose failure to perform when properly used in accordance with instructions for use provided in the labeling, can be reasonably expected to result in a significant injury of the user.
2. A critical component in any component of a life support device or system whose failure to perform can be reasonably expected to cause the failure of the life support device or system, or to affect its safety or effectiveness.