

Variability is the expression of the fundamental energy of the organism, and is not an irregular accident. Heredity is the expression of the acquired adjustment of the organism to the conditions of its existence. Mutable heredity sounds like a contradiction; so did mutable species a century ago; but it is only as heredity is mutable that evolution is possible.

THE MEASUREMENT OF SMALL GASEOUS PRESSURES.*

PRIOR to the invention of the McLeod vacuum gauge, the measurement of even moderately small gaseous pressures was difficult, and subject to large errors. The introduction of the McLeod gauge, however, early in the seventies, seemed to solve the problem. In its ordinary form, and for most purposes, this beautiful instrument admirably serves the purpose for which it is designed. But when *very* accurate measurements of pressures as small as a few millionths only of atmospheric pressure are desired, its performance is extremely unsatisfactory and vexatious. As is well known, the chief cause of the difficulty is the unequal and variable capillary depression of the two small columns of mercury, whose difference in height indirectly serves as the measure of pressure. Accurate measurement of this capricious difference obviously avails nothing.


Three or four years ago I was engaged in an investigation requiring frequent and simultaneous measurements of slight but different pressures in two large glass globes connected by a capillary tube. For this purpose I constructed and carefully calibrated two large McLeod gauges. The internal diameter of the mercury tubes was about three millimeters, and they were made from contiguous parts of the same glass tube selected for uniformity of bore.

* Read before the American Association for the Advancement of Science, August 12, 1897.

These gauges were often compared by measuring the same vacuum with both, but they rarely gave concordant results. Indeed, it was not uncommon at high exhaustions for one or the other of them to indicate a negative vacuum; that is to say, less than no pressure at all. The case of these two gauges is cited because of the opportunity they afforded for comparison. In prior work I had, like most experimentalists, used but one gauge, and, while always suspicious of its indications, had no means of knowing how large its errors might be.

The phenomenon which I next desired to investigate is the spontaneous evolution of gas from glass and other surfaces in high vacua. For this purpose an accurate and entirely reliable means for measuring very small pressures was necessary, because I could not afford to wait months or years for the evolution of sufficient gas to be detected with certainty by the old gauges. To meet these requirements, I designed, constructed, and learned how to use, the modified form of McLeod gauge, which it is the purpose of this paper to discuss.

The diagram herewith shows the essential parts of my apparatus. The bulb A, of the gauge, is made conical in its upper part to avoid adhesion of gas bubbles when the mercury rises. This bulb holds about eleven pounds of mercury. B and C are the gauge head and comparison tube respectively. They are nearly twenty millimeters inside diameter, and are made from contiguous parts of the same carefully selected tube. D is the usual air trap, and E is a long glass tube, with flexible pure rubber connections to the lower end of the gauge stem and the mercury cistern F. The latter is mounted on a carriage G, which moves vertically on fixed guides. The height of the carriage is adjustable, at the upper end of its range of motion, by means of screw H, thumb-nut I and forked support K. The screw is pivoted to the

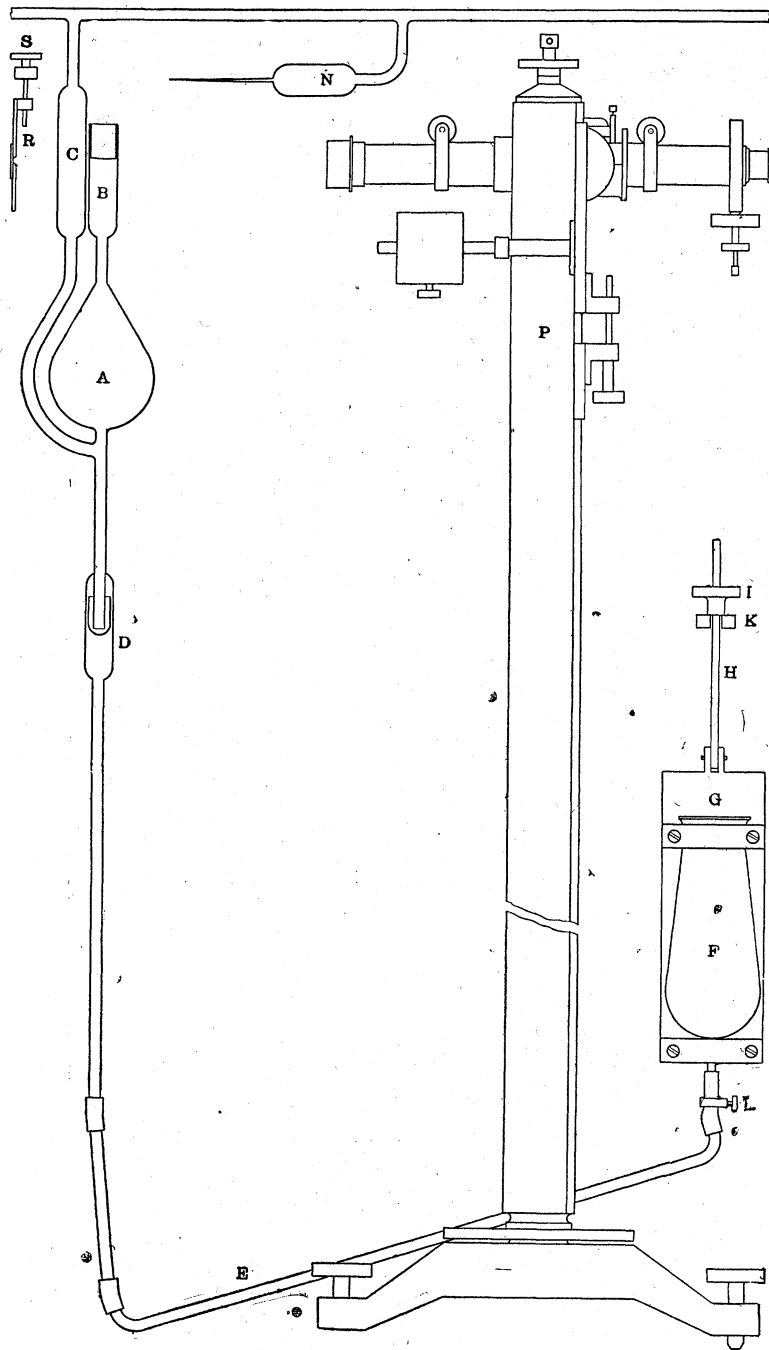

carriage, so that it may swing out of the fork when the carriage is lowered. L is a pinch-cock with screw for regulating the flow of mercury, or stopping it altogether, while pumping out the trap D. N is a bulb containing phosphorus pentoxide, to keep the interior of the gauge and other parts of the apparatus perfectly dry. P is a very elaborate cathetometer for observing the mercury columns in B and C. This beautiful instrument has a revolving column with vertical scale, and vernier with microscope, reading to hundredths of a millimeter. The eye-piece micrometer reads directly to hundredths of a millimeter, and the divisions on the revolving head of the screw are so open, that tenths of divisions are easy and certainly estimated by an experienced eye, thus permitting the micrometer to be read directly to thousandths of a millimeter. Of course the cathetometer is permanently located not as shown, but with the objective of its telescope equally distant from the axes of the tubes B and C, when it is alternately directed to them, and at such a distance that its micrometer readings correspond to a millimeter scale. The whole apparatus is located in a basement room, on a stone floor, whereby vibrations are reduced to a minimum.

The most important part of the gauge is the head B. The purpose of its great diameter is the reduction of capillary depression in its mercury column. But its size necessitates a very close approach of the mercury to its upper end, in order to reduce sufficiently its capacity. Yet the remaining space must be measurable by the cathetometer, with the utmost precision. Hence the glass must not be distorted by heating, and the closed end just over the mercury must be sharply defined. In constructing this part of the apparatus, I selected a piece of heavy tubing which would just slip inside of B, with the least possible clearance. One end of this tube was closed

as squarely as possible by fusion, and then ground with fine emery and a suitable tool, to a convex spherical surface of a long radius. Care was taken to make the center of curvature lie in the axis of the tube, and the ground surface was left unpolished to facilitate observation. A suitable length of the closed end of the tube was then cut off, slipped into B, and both tubes were fused together at their open ends, as shown.

For calibrating the head B, a ground glass stopper with a capillary duct was fitted to its neck, before the latter was sealed to the bulb A. The head was then filled with mercury by boiling, thus completely filling the small space between its wall and the cap. After cooling, the stopper was inserted to expel all excess of mercury, and the whole weighed. Next the head was emptied, and the mercury in the annular space distilled out. Again the head was very nearly filled with mercury, without allowing any to get into the annular space, and weighed as before; and the space between the top of the mercury and the convex end of the head was very carefully measured by the cathetometer. This process of weighing and measuring was repeated several times, with less mercury each time. Thus the capacity of a vertical millimeter of the head was ascertained, as well as the capacity that would remain, if the top of the meniscus of mercury just touched the convex end of the gauge, above it. Finally the neck was sealed to the bulb A, and the capacity of head, neck and bulb combined was found by weighing them empty, and again filled with mercury.

For lighting the top of each mercury column, a narrow horizontal slit in an opaque screen, R is used. The slit is covered with a strip of ground glass and obliquely illuminated by an electric lamp. The screen and slit are vertically adjusted by a thumb-screw S. The heat of the lamp is prevented from reaching the mercury col-

umns and head B, by a thick screen. This is very necessary.

In order to get the best results from the apparatus, many precautions are necessary. After filling A and B with mercury, time must be allowed for the compressed gas to cool. The effect of changing barometric pressure is nearly eliminated by so regulating the quantity of mercury in F, that its surface is in the small tube at the bottom of the cistern, when the gauge is properly filled. Its area is then very small, as compared with that in B and C. The height of the meniscus in both tubes is easily adjusted sensibly equal, by a little manipulation. I *always* raise the mercury above the point at which readings are to be taken, and then lower it, so as to read on a falling meniscus. This is highly important.

Some trouble was occasionally experienced at first, from electro-static induction between the mercury in B, and the glass above it. This was shown by distortion of the miniscus when it was brought very near the glass. The difficulty was partially, but not wholly remedied by putting mercury in the outside open end of the gauge head, and connecting it by a flexible conductor with the mercury in the cistern F. A complete remedy was effected by moistening the inside of the gauge head with a dilute solution of phosphorus pentoxide. This became completely dried by the anhydrous phosphorus pentoxide in N, but was, of course, not dehydrated, and hence always remains conducting, and dissipates the static charge.

Large pressures, up to a thousand millionths or more, are readily measured with this apparatus, by finding with the cathetometer the distance between the mercury in B, and the end of the head above it; from this is quickly calculated the necessary multiplier for the number of millimeters difference in height between the columns B and C, also measured by the

cathetometer, in order to express the result in millionths. For very small pressures, the micrometer wires are set at such a distance apart as to give a convenient constant (usually 2), and the column in B is adjusted this distance away from the glass, careful allowance being made for the thickness of the wires. Then the micrometer is used for repeated measurements of the difference in height of the mercury in B and C. The disturbing effect of *bias* is entirely eliminated by giving the micrometer screw a partial turn after each reading. Thus the next measurement is made without any knowledge of its difference from the preceding one, until the eye is removed from the telescope.

In my early experience with the apparatus, unusually careful measurements of very small pressures were often made, to determine how far its indications might be relied upon. In this connection I quote as follows from my notes, under date of February 20, 1895, concerning the last one of a series of pressure determinations: "Following is the last reading in detail, showing the extreme accuracy of these measurements:

.432 M.	.438 M.	.441 M.
.441 "	.4335 "	.429 "
.4335 "	.4275 "	.4305 "
.426 "	.450 "	.435 "
.4335 "	.4425 "	.432 "
.4395 "	.432 "	.4185 "
.4305 "	.435 "	.435 "
.441 "	.432 "	.453 "
.435 "	.4215 "	.4425 "
.435 "	.4245 "	.438 "
Means4347 "	.43365 "
		.43545 "

"Mean of all the readings, .4346 M.

"Readjusted zero point of micrometer before each reading of each set. Partially emptied gauge and readjusted capillary depression before each set of readings. The first series has no known source of error. The second and third series were made during wind squall, and surface of mercury was often tremulous. In the

third series, capillary depression was perceptibly though very slightly unequal, in direction to make readings too high."

In the above quotation 'M' means millionths of atmospheric pressure. The calculated probable error of the thirty readings taken together, is only ninety-two hundredths of a unit in the third decimal place; that is to say, less than a thousandth part of a millionth of atmospheric pressure. The probable error of the three mean results, considered as single readings, is only eleven hundredths of a unit in the third decimal place of millionths. The net result may be expressed as follows, in terms of atmospheric pressure: Considered as thirty measurements:

$$0.000\ 000\ 434\ 60 \pm 0.000\ 000\ 000\ 92.$$

Considered as three measurements:

$$0.000\ 000\ 434\ 60 \pm 0.000\ 000\ 000\ 11.$$

Here we have the measurement of a total quantity of less than half a millionth of atmospheric pressure, with a probable error of only about a fifth of one per cent. of the quantity measured.

To show how small is the effect of variable capillary depression in the large mercury columns, the following measurements were made July 25, 1897. No correction was made of accidental capillary differences, but the columns were always observed with a falling meniscus. The zero of the micrometer was freshly adjusted for each reading, and before each of the six sets of readings the mercury was lowered and then readjusted to the proper height in the gauge head.

	M.	M.	M.	M.	M.	M.
	2.210	2.203	2.209	2.198	2.198	2.202
	.204	.195	.202	.203	.204	.198
	.209	.198	.204	.208	.200	.196
	.203	.204	.210	.200	.196	.208
	.203	.192	.202	.198	.196	.203
Means	2.2058	2.1984	2.2054	2.2014	2.1988	2.2014

Calculating the probable errors we have:

Six mean readings.....2.20187 M. ± 0.00073 M.

All readings.....2.20187 " ± 0.00059 "

The effect of not equalizing the capillary depression is very apparent when these results are compared with the earlier ones quoted. But on account of increased skillfulness of observation, due to long experience, the individual readings of each set are more uniform than before; so that the net result is better.

In this example, we have the measurement of about two millionths of atmospheric pressure, with a probable error of only one part in three thousand, of the quantity measured.

From the foregoing, we may safely conclude that with the apparatus described, small gaseous pressures may be easily measured, with a probable error of less than a thousandth part of a millionth of atmospheric pressure.

CHARLES F. BRUSH.

CLEVELAND, O.

SOME THOUGHTS CONCERNING THE TEACHING OF CHEMISTRY.

IN the preface to a short set of 'Notes Upon Qualitative Analysis,' recently published, I made use of the expression: "There is small doubt that, were it not for the expense of printing, every teacher of chemistry would use a text-book made by himself with either pen or scissors."

In a review of the little book which afterwards appeared in one of the foreign journals, the critic referred to the above sentence, with the added remark: 'Sad, indeed, if true!' He who wrote the criticism is a distinguished chemist, for otherwise his opinions could not find place in so eminent a journal; but the thought crosses me: Is he a teacher? There is a tremendous difference between the specialist who never enters the class-room and the trained instructor who but rarely leaves it.

A man may rank in the highest grade as a scientist, and yet be nothing of a teacher; he may be skillful to the last degree in map-