


ZEISS

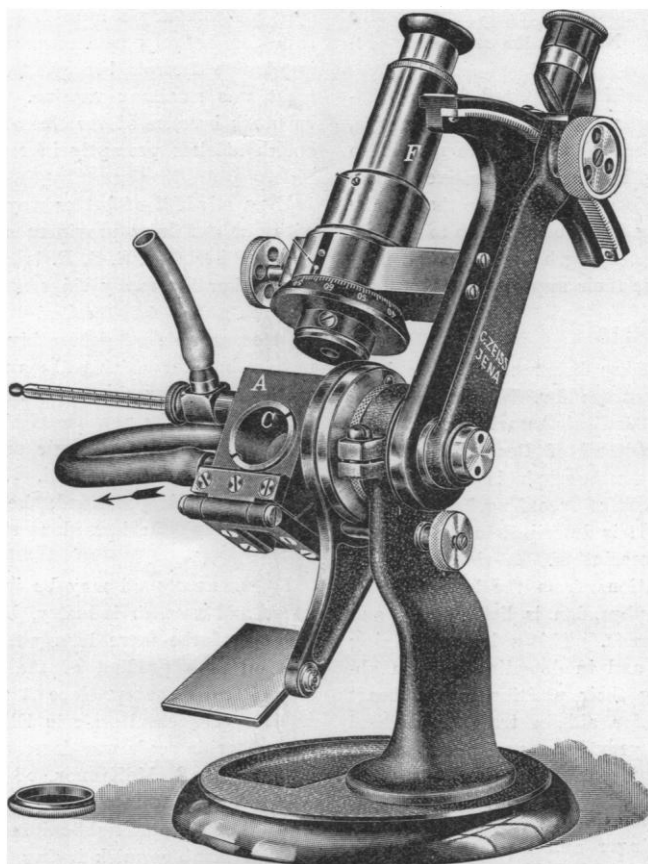

ABBE REFRACTOMETER

For determining the refractive indices and mean dispersions of liquid, plastic and solid substances.

The refractive index is read off a graduated sector without any calculation whatever. The mean dispersion of the substance under examination is calculated from readings furnished by the graduated drum of the compensator.

Range $n_D = 1.3$ to $n_D = 1.7$ accurate to within about two units of the 4th decimal. With heatable prisms.

Complete in case with thermometer and dispersion table.

Price \$278.52 f. o. b. N. Y.

CARL ZEISS, INC.

485 Fifth Avenue
NEW YORK

728 So. Hill Street
LOS ANGELES

