

SCIENCE

NEW SERIES
VOL. 94, No. 2433

FRIDAY, AUGUST 15, 1941

SUBSCRIPTION, \$6.00
SINGLE COPIES, .15



$\frac{1}{5}$ th the Width of a Human Hair

Instruments which play so important a part in national defense call for precision manufacturing methods which Bausch & Lomb have developed over years of producing fine optical instruments. Here, in air-conditioned rooms, deft operators accurately space and

engrave lines only $\frac{1}{5}$ th as wide as a human hair on binocular "mil" scales.

BAUSCH & LOMB
OPTICAL CO. • ROCHESTER, NEW YORK
ESTABLISHED 1853

AN AMERICAN SCIENTIFIC INSTITUTION PRODUCING OPTICAL GLASS AND INSTRUMENTS
FOR NATIONAL DEFENSE, EDUCATION, RESEARCH, INDUSTRY AND EYESIGHT CORRECTION

Science: published weekly by The Science Press, Lancaster, Pa.

Entered as second-class matter July 18, 1923, at the Post Office at Lancaster, Pa., under the Act of March 3, 1879.

New

WEBER Temperature Measurement and Control

This new text for college students presents an experimental study of the methods of temperature measurement. Theoretical principles necessary for a clear understanding and intelligent use of these methods are included.

Contents: Expansion Thermometry; Heat Transfer; Thermoelectricity; Thermoelectric Thermometry; Radiation; Radiation Pyrometry; Resistance Thermometry; Recording Pyrometry; Temperature Control; Calorimetry; Thermal Analysis; Elementary Thermodynamics; Special Methods of Temperature Measurement; Extreme Temperatures; International Temperature Scale.

By Robert L. Weber, Ph.D.,
Pennsylvania State College
Ready This Summer

THE BLAKISTON COMPANY
PHILADELPHIA

The Foundations of Science

By H. POINCARÉ

Pp. xi + 553.

Containing the authorized English translation by George Bruce Halsted of "Science and Hypothesis," "The Value of Science" and "Science and Method," with a special preface by Poincaré, and an introduction by Josiah Royce. *Price, postpaid, \$5.00.*

THE SCIENCE PRESS
Grand Central Terminal New York, N. Y.



Stokes Automatic Water Stills are now available in new and improved laboratory models, with capacities from ½ gal. to 100 gals. per hour, to produce exceptionally pure distilled water for the most exacting research and scientific purpose.

These stills are fully described and illustrated in a complete 24-page catalog just published. Method of operation is shown, comparative costs for electric, steam and gas heating, typical analysis of water produced, description of automatic start-stop and flush controls and other valuable information for users of distilled water are contained. Write.

F. J. STOKES MACHINE COMPANY
5958 Tabor Road Olney P. O. Philadelphia, Pa.



STRANGE MALADY

The Story of Allergy

BY WARREN T. VAUGHAN

In this book one of the most common maladies to which human beings are subject is discussed for laymen by a man who is as distinguished for his literary style as for his eminence as a scientist. It is a book that is as interesting as it is valuable.

"A book as easy to read and understand as a primer, and as interesting as a novel." *Science News Letter.*

"An informative and fascinating work in nontechnical terms." *Nashville Tennessean.*

"Few have been the occasions for this reviewer to find in a book written for nontechnical readers such a completely scientific, lucid and charming exposition of a subject." *The Saturday Review of Literature.*

This is the second nontechnical book published for the American Association for the Advancement of Science by Doubleday, Doran and Company. Price to members of the Association \$2.50; to others, \$3.00.

American Association
for the Advancement of Science
Smithsonian Institution Building,
Washington, D. C.

PURE AMINO ACIDS


● In connection with the greatly increasing number of studies of nutritional problems, investigators have recognized the need for pure chemicals as the individual constituents of basic diets, to eliminate difficulties caused by the introduction of unknown factors. The rapid progress of recent years in the isolation, identification, and synthesis of the vitamins, especially those of the B complex, has fulfilled part of this need, but there remains the problem of the supply of pure amino acids in the required quantities.

The successful activities of Merck & Co. Inc. in furthering research and development of the vitamins, particularly those of the water-soluble group, has led the Company to engage in the commercial production of pure amino acids.

The following pure amino acids are now available at prices calculated to permit investigation of their nutritional significance:

Aminoacetic Acid
(Glycocoll, Glycine)
Beta-Alanine
*dl-Alpha-Alanine
d-Cysteine Hydrochloride
l-Cystine
dl-Glutamic Acid Monohydrate
d-Histidine Monohydrochloride
*l-Hydroxyproline
dl-Isoleucine
dl-Leucine
*d-Lysine Monohydrochloride
dl-Lysine Monohydrochloride
*dl-Methionine
dl-Norleucine
dl-Phenylalanine
*l-Proline
dl-Serine
*dl-Threonine
*l-Tryptophane
dl-Valine

*Available in restricted quantities.

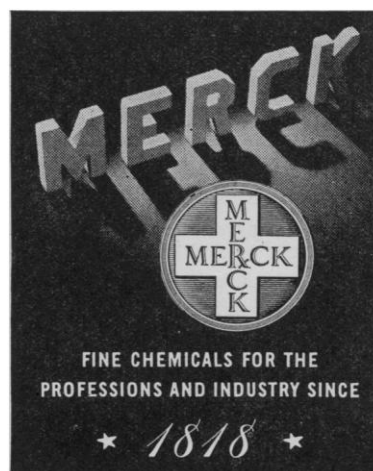

MERCK & CO. Inc. *Manufacturing Chemists* RAHWAY, N.J.

Save Time and Material by Cutting

GLASS .. QUARTZ .. METALS .. STONE .. CERAMICS .. FIBRE .. PLASTICS .. BAKELITE .. ETC.

*with
the*




Bonded-Abrasive-Wheel

WET CUTTING-OFF MACHINE

True, clean cuts are made with this machine by means of a 12-in. diameter bonded abrasive wheel (either 0.04 or 0.06 in. thick). It produces a cut that is smooth surfaced, thus eliminating burring and other finishing operations that are often necessary where other cutting-off means are employed. Cuts of any angle can be made.

Speedy operation, low upkeep cost, and the materials saved by virtue of the thin cutting wheel, make this machine an important economy factor well worthy of your investigation.

Fully Described in Bulletin A-2094

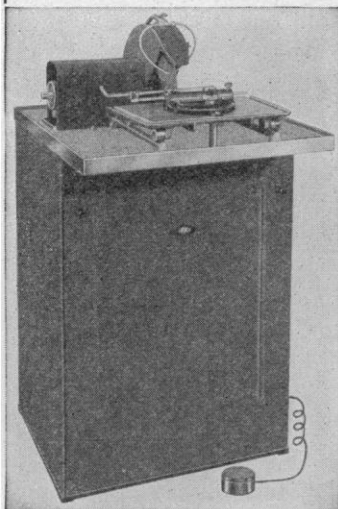

AMERICAN INSTRUMENT CO.

8010 GEORGIA AVENUE • SILVER SPRING, MARYLAND

Constant
temperature uniformity
for safe
incubation



No. 554
Incubator

The Castle Precision Incubator operates with a constancy of $\pm 1/5^\circ$ C. and a uniformity of $\pm 7/8^\circ$ C., under full load conditions, far in excess of the recommended tolerance of $\pm 1^\circ$ C., recommended by the American Public Health Association.

Less variation throughout the chamber is shown by the Castle because heat is transmitted by interior radiation, rather than by convection. One thermometer will suffice for accurate temperature measurements.

Thousands of calories of reserve heat, provided by twenty-two gallons of warm water, accurately controlled, compensate quickly for any heat loss caused by opening of door. Changes in room temperature, if below operating range, do not affect temperatures inside incubator.

Castle Precision Incubator No. 554, illustrated, is recommended for milk analysis by the agar plate method. Other models in varying capacities for various bacteriological applications are available. Write—

WILMOT CASTLE CO.

1212 UNIVERSITY AVENUE

ROCHESTER, N. Y.

VITAMIN-FREE CASEIN SMACO

IN VITAMIN EXPERIMENTATION the type of dietary protein employed may well be the most important factor. When Vitamin-Free Casein SMACO is the protein in the deficiency diet, uniform and consistent depletion of test animals occurs well within the required time interval specified by the U.S.P. or other standard test methods. Recent work suggests the suitability of Vitamin-Free Casein SMACO for vitamin K¹ and biotin² assay and experimental procedures in chicks.

Vitamin-Free Casein SMACO is prepared in our laboratories by a special extraction process which insures a completely vitamin-free product. Each package bears a control number that identifies the protocols showing rigid biological assay, control of uniformity and freedom from complicating vitamin factors.

Vitamin-Free Casein SMACO has found widespread acceptance in university, pharmaceutical and industrial laboratories. We therefore invite you to try this reliable source of protein in your next biological investigation.


Write for the booklet "Special Products for Nutritional Research" for additional information on Vitamin-Free Casein SMACO, prepared diets for U.S.P. assays, crystalline vitamins and other biochemicals of nutritional interest.

1. ANSBACHER, S.: *Proc. Soc. Exp. Biol. & Med.*, 46:421:1941.
2. ANSBACHER, S., and LANDY, M. (In Press).

RESEARCH LABORATORIES
S. M. A. Corporation
CHAGRIN FALLS, OHIO



For the Physiological Laboratory
ELECTRODES WITH UNIVERSAL ADJUSTING ARM

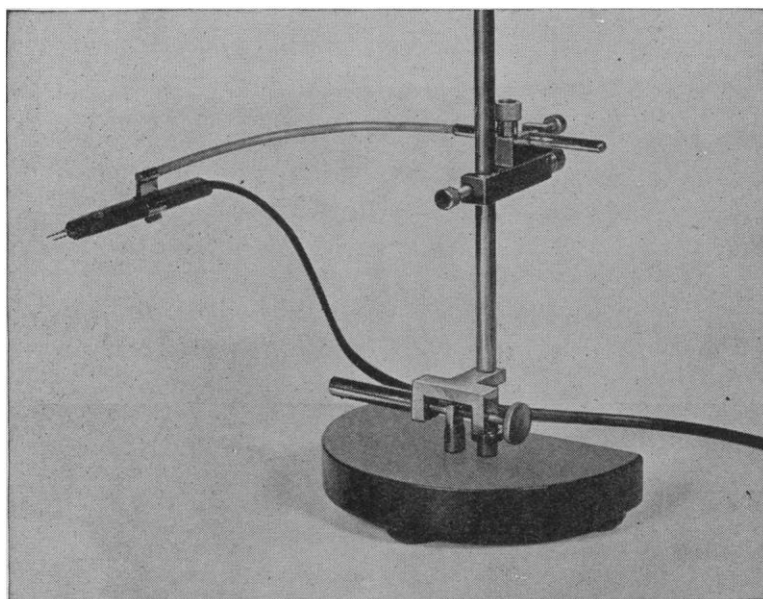

Flexible Electrode Holder with adjustments—one-fourth the actual size.

Electrodes. Detachable silver or platinum tips, quickly interchangeable. Handle and cord strongly and durably coupled.

Electrode Holder. A lead flexing arm supports the electrodes in a removable screw-clip. A binding screw fixes the arm within a tubular mounting-rod by slide adjustment. By this means the flexible lead wire can be promptly shortened or renewed.

Adjusting Clamp. Slow motion governed by a knurled head—swivel action by a set-screw.

Stand with Adjusting Screw. Rotation of post through 45° by an adjustment head operating on the semicircular base.

Each of these devices may be obtained separately. Write for the price list and catalogue of Physiological Apparatus

The HARVARD APPARATUS COMPANY, Incorporated

Dover, Massachusetts

SCIENCE

VOL. 94

FRIDAY, AUGUST 15, 1941

No. 2433

The American Association for the Advancement of Science:

- Preliminary Announcement of the Fifth Chicago Meeting:* DR. F. R. MOULTON 147
- Colloids in Astronomy and Meteorology:* JEROME ALEXANDER 151

Obituary:

- James W. Glover:* PROFESSOR LOUIS C. KARPINSKI 156

Scientific Events:

- The Federal Department of Health of Brazil; Grants of the Geological Society of America; The Annual Report of the Director of Field Museum of Natural History; U. S. Civil Service Examinations* 157

Scientific Notes and News 159

Discussion:

- The Cultivation of Cotton by Pueblo Indians of New Mexico:* PROFESSOR LESLIE A. WHITE. *The Preservation of Natural Areas Exemplifying Vegetation Types:* DR. I. T. HAIG. *Man's Biological Outlook:* GERRIT S. MILLER, JR. *The Law of Urban Concentration:* DR. ALFRED J. LOTKA, PROFESSOR E. L. THORNDIKE 162

Scientific Books:

- Endocrinology:* PROFESSOR C. N. H. LONG. *The Theory of Newtonian Attraction:* PROFESSOR G. C. EVANS 164

Societies and Meetings:

- The American Association of Botanical Gardens and Arboretums:* DR. DONALD WYMAN 166

Special Articles:

- Role of p-aminobenzoic Acid and Inositol in Lactation:* PROFESSOR BARNETT SURE. *Hearing in the Rat at High Frequencies:* JAMES GOULD and DR. CLIFFORD MORGAN. *The Germination of Maize Pollen:* DR. R. A. BAIR and DR. W. E. LOOMIS 167

Scientific Apparatus and Laboratory Methods:

- The Daily Removal of Formalin from Preserved Biological Specimens Used in Class Work:* W. B. FORT, H. C. WILSON and H. G. GOLDBERG. *A Simple Method for Removing the Plungers of "Frozen" Glass Syringes:* DR. AUGUSTA B. MCCOORD 169

Science News 8

SCIENCE: A Weekly Journal devoted to the Advancement of Science, edited by J. MCKEEN CATTELL and published every Friday by

THE SCIENCE PRESS

Lancaster, Pa. Garrison, N. Y.
New York City: Grand Central Terminal
Annual Subscription, \$6.00 Single Copies, 15 Cts.

SCIENCE is the official organ of the American Association for the Advancement of Science. Information regarding membership in the Association may be secured from the office of the permanent secretary in the Smithsonian Institution Building, Washington, D. C.

THE AMERICAN ASSOCIATION FOR THE ADVANCEMENT OF SCIENCE

PRELIMINARY ANNOUNCEMENT OF THE FIFTH CHICAGO MEETING

By Dr. F. R. MOULTON

PERMANENT SECRETARY

FROM September 22 to September 27, inclusive, the association will join with The University of Chicago in celebrating the fiftieth anniversary of its founding. The university has organized a program of addresses by distinguished scientists and scholars and an extensive series of symposia in the fields of the natural sciences and the humanities under the general title "New Frontiers in Education and Research." Outlines of the programs of these addresses and symposia were published in the July 4 issue of SCIENCE, pages 20-22.

This is the fifth meeting of the association in Chicago. The earlier meetings were held in 1868, 1908,

1920 and 1933, the latest in connection with the Century of Progress Exposition organized in celebration of a century of progress through science. The theme of the exposition was proposed by Dr. Michael I. Pupin, president of the association in 1925.

Persons attending the meeting in Chicago may arrange for convenient living accommodations in the Residence Halls of the university by writing the Director of the Fiftieth Anniversary Celebration for reservations. It is suggested that those desiring rooms on the university campus write promptly (not later than August 25) for reservations because the number that will be available is limited. Each applicant

immersed in it within 3 to 5 minutes. The largest specimens required the greatest length of time.

However, because of the acidity of the formalin resulting from the presence of formic acid, sulfur dioxide gas, SO_2 , was liberated from the NaHSO_3 solution in such quantities as to nullify its usefulness in a classroom procedure. It appeared that this source of SO_2 could be eliminated simply by reducing the H ion concentration of the reactant solution. This was accomplished by buffering the solution with Na_2SO_3 .

We may now detail the essential points in the preparation and use of the sulfite-bisulfite solution:

(1) The deformalinizing solution contains 5.7 per cent. (by weight) of NaHSO_3 and 3.8 per cent. (by weight) of Na_2SO_3 dissolved in tap water. A deviation of 1 to 5 per cent. from the above figures would probably introduce no serious failure of the solution to function properly. It is our experience that 20–30 liters of the solution will last a full semester in the daily removal of formalin from any specimens in use in a zoology class of 35 students. To prepare 20 liters of solution dissolve 1260 grams of NaHSO_3 and 840 grams of Na_2SO_3 in tap water.

(2) Specimens removed from their formalin bath are given a brief preliminary rinsing under the tap, and then immersed in the sulfite-bisulfite solution from 3 to 5 minutes. As many specimens as can be conveniently handled may be deformalinized simultaneously. Following a final quick rinse, the specimens are free of formalin odor and ready for dissection. Large specimens or those which may have been injected with various formalin mixtures may require subsequent short immersions as dissection proceeds.

(3) Failure of the solution after repeated usage to remove the formalin promptly may require the addition of more NaHSO_3 just short of the point where SO_2 gas is evolved. Evidence of SO_2 arising during the routine employment of the solution calls for the addition of small amounts of the Na_2SO_3 . There is a considerable variation in the actual amounts of NaHSO_3 and of Na_2SO_3 in the technical grade of these chemicals. This should be kept in mind and the amount of one or the other reagent increased as may be necessary to give a satisfactory solution. A pH determination of the solution gives a reasonably easy method of ascertaining if it has been properly prepared. The solution of the concentration specified has a pH of about 6.4. One containing insufficient Na_2SO_3 and which may therefore evolve sulfur dioxide, will have a lower pH. One containing an excess of Na_2SO_3 will have a higher pH.

(4) Although certain specimens, frogs for example, may be stored for several weeks in the reactant solution without impairing their dissecting qualities, others such as the dogfish become soft after 5 to 6 days and

unsuitable for dissection. In other words, the solution is not a substitute for formalin. After the removal of the formalin, the specimen may be kept in any other satisfactory preservative, or returned to formalin.

(5) The solution should be kept in common glazed earthenware laboratory crocks, as it will slowly attack metal containers.

W. B. FORT
H. C. WILSON
H. G. GOLDBERG

HERZL JUNIOR COLLEGE,
CHICAGO

A SIMPLE METHOD FOR REMOVING THE PLUNGERS OF "FROZEN" GLASS SYRINGES

THE method of removing the plungers of "frozen" glass syringes suggested by Goff in *SCIENCE*, Vol. 93, page 602, was of much interest to us. While we make no claim whatever to originality, we feel justified in calling attention to the method of removing the plungers of "frozen" glass syringes used in our laboratory, because of its simplicity and usefulness, and because many persons are unfamiliar with it.

All that is required is a syringe with a plunger of lesser diameter than the plunger of the "frozen" syringe, and equipped with a short hypodermic needle. We often use a 1 cc Yale tuberculin syringe. The needle passes through a small bit of rubber, such as a piece of a wide rubber band which acts as a gasket. The tuberculin syringe is filled with water, and the needle inserted into the outlet of the "frozen" syringe, the piece of rubber making an airtight seal. Water is then forced from the tuberculin syringe into the "frozen" syringe, until the plunger of the latter is free. It may be necessary to fill the tuberculin syringe with water a number of times, but the method almost never fails.

AUGUSTA B. McCOORD
UNIVERSITY OF ROCHESTER SCHOOL OF
MEDICINE AND DENTISTRY

BOOKS RECEIVED

- DRAKE, N. L., Editor. *Organic Syntheses*, Vol. 21. Pp. v + 120. Wiley. \$1.75.
FERRAR, W. L. *Algebra; A Text-book of Determinants, Matrices and Algebraic Forms*. Pp. vi + 202. Oxford University Press.
GERARD, RALPH W. *The Body Functions*. Pp. xiii + 289. 90 figures. Wiley. \$1.75.
HOLMES, HARRY N. *General Chemistry*. Fourth edition, revised. Pp. viii + 720. 198 figures. Macmillan. \$3.75.
MACY, RALPH W. and HAROLD H. SHEPARD. *Butterflies; A Handbook of the Butterflies of the United States, Complete for the Region North of the Potomac and Ohio Rivers and East of the Dakotas*. Pp. vii + 247. Illustrated. University of Minnesota Press. \$3.50.
Rockefeller Foundation. *Annual Report, 1940*. Pp. 473. The Foundation, New York.

"WRATTEN LIGHT FILTERS"

A Book of Data on Wratten Filters

THERE ARE more than 100 filters in the series of Wratten light filters. They are designed for use in general monochrome and color still photography, cinematography, and special scientific fields—including astronomy, photometry, spectroscopy.

Each Wratten Filter is made to meet a rigid standard, and is supplied in the form most convenient for its application.



The purpose of the book, *Wratten Light Filters*, is to facilitate selection of filters by providing complete spectrophotometric data concerning them.


The 88-page Sixteenth Edition of this publication gives transmission curves and tables for all filters, as well as notes on the use of filters for special purposes. It is available at dealers in photographic supplies.

EASTMAN KODAK COMPANY

Research Laboratories

Rochester, N. Y.

Glass Fractionating Diffusion Pumps

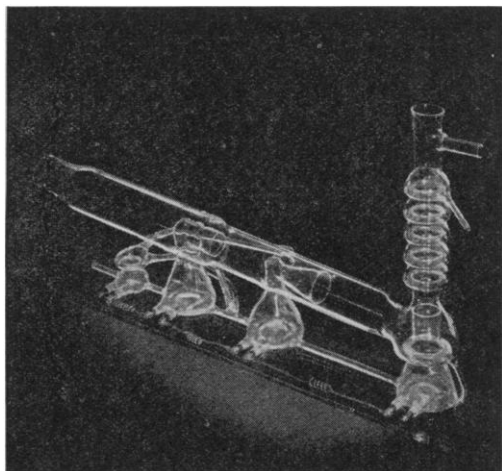

Glass Three-stage Fractionating Pump,
Type GF-25A (air-cooled)

There are now available five types of Distillation Products' glass diffusion pumps, providing ultimate vacua of, respectively: 1×10^{-3} mm., 1×10^{-5} mm., 5×10^{-6} mm., 5×10^{-7} mm., 5×10^{-8} mm. Neither liquid air nor a real cold trap is required for effective performance. The pumping fluid is continuously purified during operation, through fractionation.

These units are important to industry, to provide economical exhaustion of glass systems. They are important to laboratories, to meet the exacting requirements of research. Complete specifications will be furnished promptly upon request.

Inquiries are also invited for information about Distillation Products' glass and metal booster pumps, glass-metal and metal high-vacuum diffusion pumps, pumping fluids, vacuum greases, vacuum gauges, cyclic molecular stills, glass-fabrication service.



DISTILLATION PRODUCTS, INC.

Jointly owned by EASTMAN KODAK COMPANY and GENERAL MILLS, INC.

ROCHESTER, N. Y.