

SCIENTIFIC APPARATUS AND LABORATORY METHODS

A METHOD OF OPENING LYOPHILE TUBES

THE difficulty of conveniently and cleanly breaking open vacuum-sealed tubes of dried material led to the development of the following method of preparing, sealing and opening tubes having a diameter of 1.5 cm. The method is undoubtedly applicable to tubes of other dimensions.


The material to be dried is placed in a sterile Pyrex test-tube, 15 cm by 1.5 cm (A), and the cotton plug is pushed about one inch into the tube. The tube is then heated and constricted about 7 cm from the bottom (B). Using a spot flame, a small cup is blown about 2 cm below the constriction (C), and the tube is then attached to the lyophile apparatus. After the material has been thoroughly dried, the tube is sealed at the constriction and the tip is dipped in sealing-wax to prevent entrance of air if scoring of the sealed tip should occur.

When it is desired to open the tube, a spot flame (gas-oxygen) is applied opposite the cup (D) and the vacuum causes atmospheric pressure to force an inverted bubble into the lumen of the tube. The size of this bubble is controlled by rotating the flame. When a suitable diameter has been obtained, the flame is directed toward the point where the break is desired. With proper direction of the flame, the bubble elongates and finally breaks toward the cup (E). The flame is then removed, and a sterile cotton plug is inserted into the "funnel" (F). This procedure for opening the tube requires about ten seconds.

Theoretically, the air which rushes into the tube through the break is sterile, since, at that time, the walls of the funnel are very hot and the flame is still in place. To test this, the following trials were run.

Five tubes, each containing a small agar slant, were treated by this procedure and, after opening, were plugged with cotton and placed in an incubator at 37.5° C. No growth had occurred at the end of one week. Five tubes containing a suspension of a rapidly growing bacillus, and two tubes containing a suspension of *Mycobacterium tuberculosis avium* were all lyophilized and opened as above. Sterile distilled water was pipetted through the funnels into the tubes and the dried material resuspended. The tubes were then tilted horizontally so that the suspension flowed into the cups, and a loop of material was removed from each tube and streaked on agar slants. Growth without contamination occurred on all slants. Two series of ten tubes each, one containing anti-bovine-brucellosis-serum and the other containing anti-swine-brucellosis-serum, both antisera being of known titer, were lyophilized and sealed. Half of the tubes in each series were opened by the regular method of scoring

and breaking, and the other half were opened by the method herein described. Upon determining the agglutination titers of the redissolved material, no difference was noted among the various samples.

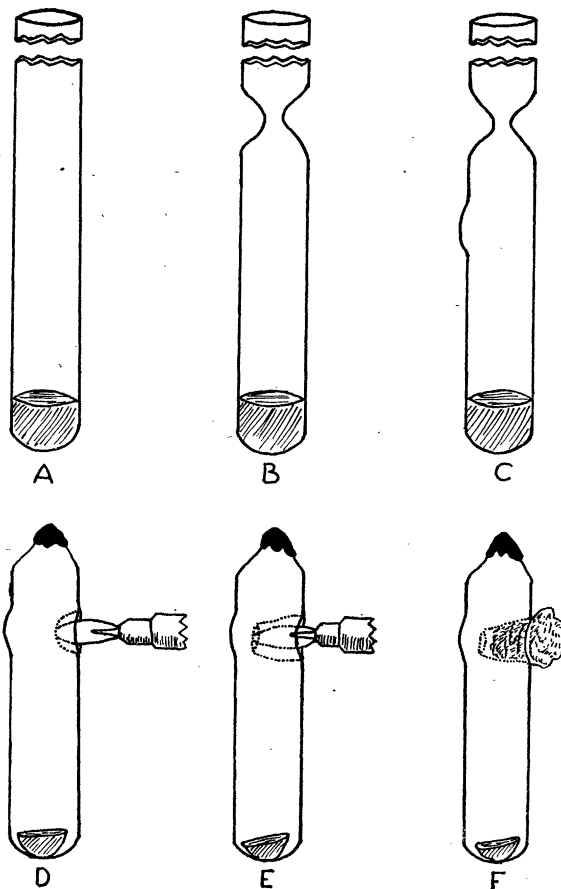

A noticeable advantage is the fact that the cotton plug is protected by the glass walls of the funnel, and only unusual handling will cause the fluid in the tube to come in contact with the cotton.

A. APPLEBY

ANIMAL DISEASE STATION
BUREAU OF ANIMAL INDUSTRY,
AGRICULTURAL RESEARCH ADMINISTRATION

BOOKS RECEIVED

- DAVSON HUGH and JAMES FREDERIC DANIELLI. *The Permeability of Natural Membranes*. Illustrated. Pp. x + 361. Cambridge University Press. \$4.75.
- HARNED, HERBERT S. and BENTON B. OWEN. *The Physical Chemistry of Electrolytic Solutions*. Illustrated. Pp. xi + 611. Reinhold Publishing Corporation. \$10.00.
- JENKINS, GLENN L. and WALTER H. HARTUNG. *The Chemistry of Organic Medicinal Products*. Illustrated. Pp. vi + 675. John Wiley and Sons. \$6.50.
- MATHER, K. *Statistical Analysis in Biology*. Illustrated. Pp. 247. Interscience Publishers, Inc. \$4.50.