## Now available


Adenosine Triphosphate (ATP); Amygdalin; Amylase; Animal Lecithin; Ascorbic Acid Oxidase; Bacitracin; Animal Lecithin; Ascorbic Acid Oxidase; Bacitracin; BAL; Biotin, cryst.; Caffeic Acil; Carotene, cryst.; Catalase; Cellulase Chlorogenic Acid; Chorionic Gonadotropin; Circulatory Hormone; Colchicine; Cytidylic Acid; Cytochrome C; Dehydroascorbic Acid; Diacetonamine; Dihydroxyacetone; Dihydroxyphenylalanine (DOPA); Dipyridyl; Edestin; Emulsin; Erythritol; N-Ethylpiperidine; Fibroin; Folic Acid; Galacturonic Acid; Gentisic Acid; Girard Reagents P and T; Gliadin; Glucose Pentaacetate; Glucuronic Acid; Glyceraldehyde; Glyceric Acid; Heparin; Hordenine; Hyaluronidase; Hydrindene; 2-Hydroxyadipaldehyde; Humulon; Indan; Isoascorbic Acid; Isopropylhyde; Humulon; Indan; Isoascorbic Acid; Isopropylarterenol; Kojic Acid; Kynurenic Acid; Lanthionine; Lipase; Lysozyme; Lyxose; Malononitrile; Maltase; Melezitose; Mesobilirubinogen; Muscle Adenylic Acid; Myanesin; p-Nitrophenylphosphate; Nucleoprotein; Melezitose; Mesobilirubinogen; Muscle Adenylic Acid; Myanesin; p-Nitrophenylphosphate; Nucleoprotein; Orcinol; Pancreatin; Pantothenyl Alcohol; Penicilinase; Peroxidase; Phenazine; Phenylpyruvic Acid; Phloridzin; Phosphorylase; Piperin; Porphyrindine; Protamines; Protoporphyrin; Pyridoxal; Pyridoxamine; Pyrocatechuic Acid; Pyruvic Aldehyde; Ribonuclease; Saccharic Acid; Salmine; Serine Phosphoric Acid; Spermidine; Spermine; Thioacetic Acid; Thiocytosine; Thyroxine; Trigonelline; Triphenyltetrazolium Chloride; Tripyridyl; Trypsinogen; Tyrosinase; Tyrothricin; Tripyridyl; Trypsinogen; Tyrosinase; Tyroth Urease; Uricase; Uridine; Vitellin; Xanthosine. Tyrothricin:

Ask us for others!

DELTA CHEMICAL WORKS



## When Accuracy is Important

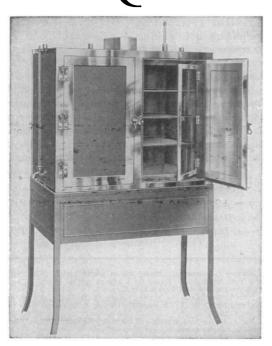

THE CASTLE PRECISION INCUBATOR is designed and built to give you the precise accuracy that is essential in bacteriological work. Construction is of monel metal for lifetime use.

Independent laboratory tests proved these two important facts:

UNIFORMITY: ± 1/4°C. Never as much as a degree variation between top and bottom of chamber even when loaded.

CONSTANT TEMPERATURE: ± 1/2° to 1/4°C. Never more than a fraction of a degree variation at the thermometer . . . despite room temperature fluctuations from 10° to 35°C.

For full details write: Wilmot Castle Co., 1212 University Ave., Rochester 7, N. Y.

Castle Bacteriological Apparatus\_\_\_\_