



SCIENCE

16 October 1959

AMERICAN ASSOCIATION FOR THE ADVANCEMENT OF SCIENCE

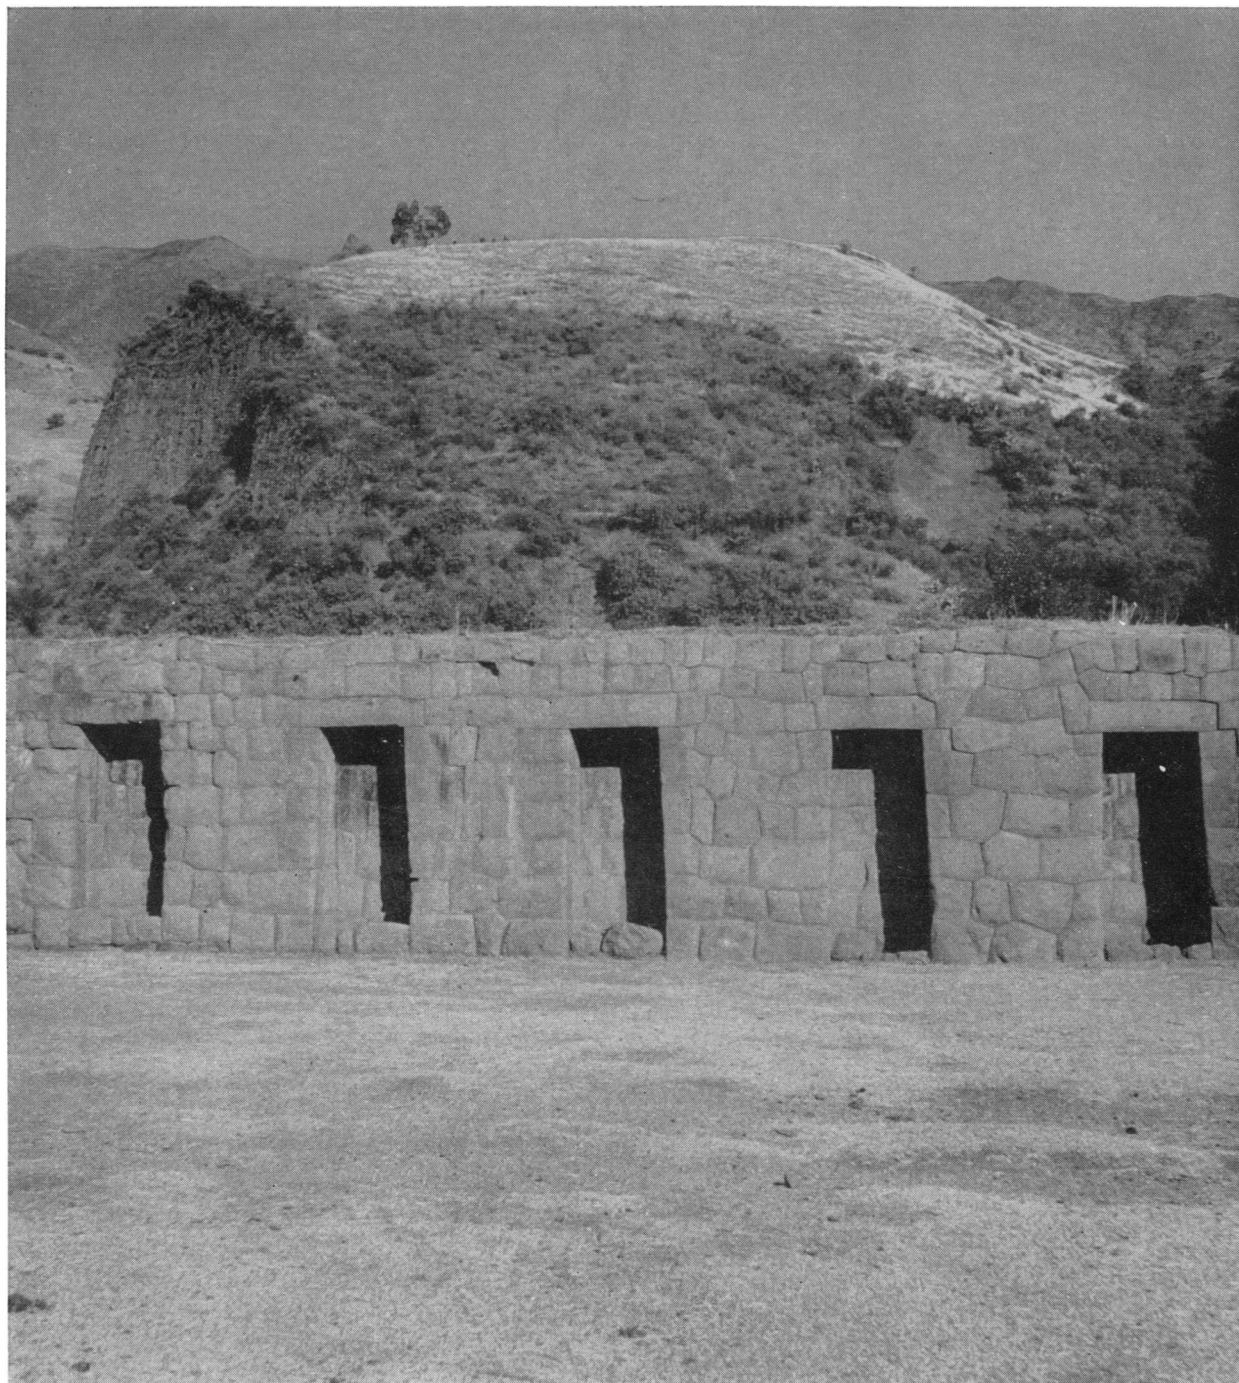

*photomicrography
combining
LEITZ quality
with
unlimited versatility*

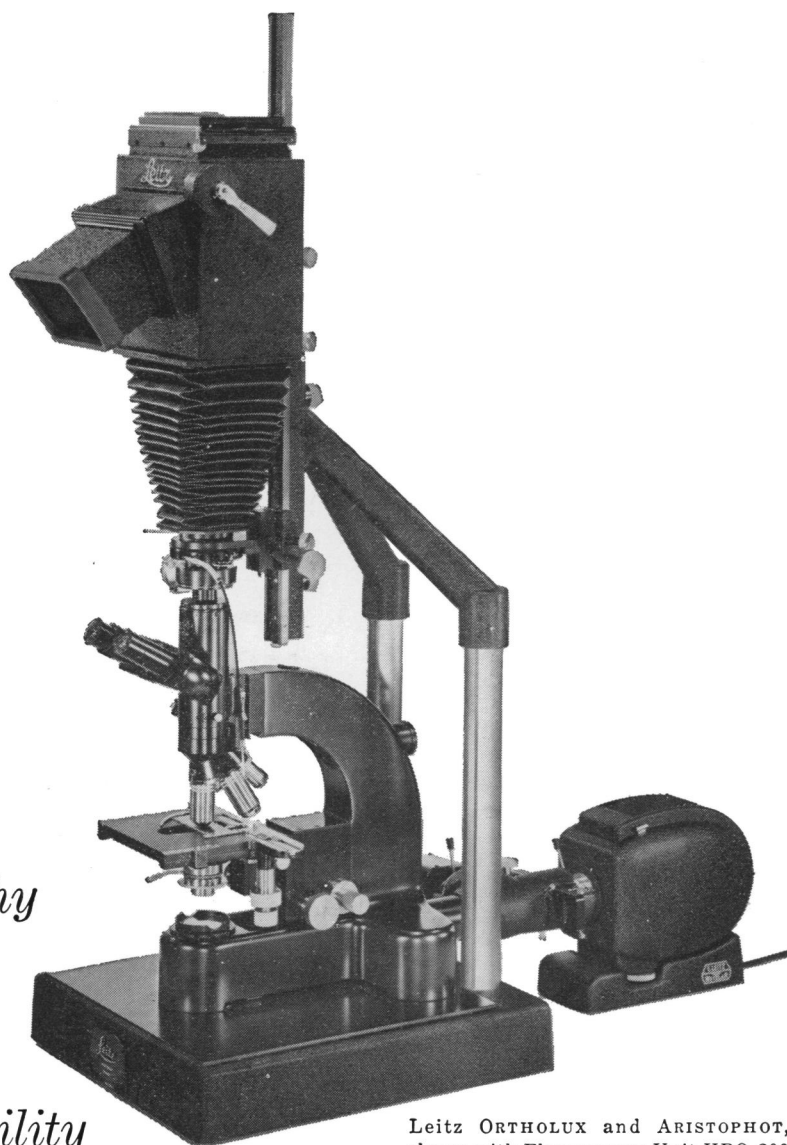

Leitz ORTHOLUX and ARISTOPHOT,
shown with Fluorescence Unit HBO-200

ORTHOLUX *Microscope* *with* **ARISTOPHOT II**

Here are precision Leitz instruments perfectly matched for exacting photomicrography. They are simple to operate, yet capable of infinite variations to fit all your photomicrographic requirements.

With the Leitz ORTHOLUX with ARISTOPHOT, image sharpness is limited only by the resolution of the film you are using. Only air separates the optical system from the film. There is no loss of image sharpness because of mirrors or other devices.

Film size is not restricted: 35mm Leica, $3\frac{1}{4} \times 4\frac{1}{4}$, 4×5 , or Polaroid. Your choice of illumination, too, is virtually unlimited: transmitted or incident light, dark field, polarized or phase contrast.

With the ARISTOPHOT detached, the Leitz ORTHOLUX fulfills the most critical requirements for a research microscope. The ARISTOPHOT II may be used separately for gross photography or macrophotography.

Write for illustrated brochure, Dept. 294 SC-10.

Leitz

E. LEITZ, INC., 468 FOURTH AVENUE, NEW YORK 16, N. Y.
Distributors of the world-famous products of
Ernst Leitz G. m. b. H., Wetzlar, Germany—Ernst Leitz Canada Ltd.
LENSES • CAMERAS • MICROSCOPES • BINOCULARS

Editorial	After 20 Years—Technicians or Scholars?	945
Articles	Reactions of Grafts against Their Hosts: <i>R. E. Billingham</i>	947
	Transplantation immunity works both ways—hosts destroy grafts and grafts may harm hosts.	
	Automatic Linkage of Vital Records: <i>H. B. Newcombe</i> et al.	954
	Computers can be used to extract “follow-up” statistics of families from files of routine records.	
	Genetics and the Hierarchy of Biological Sciences: <i>S. Wright</i>	959
	Genetics is binding biology at all levels, from macromolecule to species, into a unified discipline.	
Science in the News	Science Enters the Political Arena; Lunik III Flight to Moon Underscores United States-Soviet Positions in Space Competition	966
Book Reviews	<i>The Incas of Pedro Cieza de León</i> , reviewed by <i>G. R. Willey</i> ; other reviews	973
Reports	Measurement of Human Heart Rate during Usual Activity: <i>D. A. Rowley, S. Glagov, P. Stoner</i>	976
	Vitamin-A Content of the Frog Eye during Light and Dark Adaptation: <i>R. Hubbard</i> and <i>A. D. Colman</i>	977
	North-South Asymmetry of the Earth's Figure: <i>S. W. Carey; J. A. O'Keefe</i>	978
	Instatement of Stuttering in Normally Fluent Individuals through Operant Procedures: <i>B. Flanagan, I. Goldiamond, N. H. Azrin</i>	979
	Effects on Palate Development of Mechanical Interference with the Fetal Environment: <i>B. E. Walker</i>	981
	Long-Term Effects of Tenotomy on Spinal Monosynaptic Response in the Cat: <i>R. Beranek</i> and <i>P. Hnik</i>	981
Departments	Forthcoming Events; New Products	984
Cover	The remains of the “speaking river” tambo, one of the royal stations on the Royal Road of the Incas between Cuzco and Quito. Called “Rimac-tampu” in Incan times, this was the way-stop before the “Speaking Apurimac River.” From <i>The Incas of Pedro Cieza de León</i> , reviewed by Gordon R. Willey on page 973. [Courtesy University of Oklahoma Press]	



THE HUMAN FACTOR in today's technology

Scientists have long been preoccupied with the technological problems of Man and the Machine. The increasingly complex nature of advanced systems has created an urgent need to enhance man's contribution to effective systems performance. The complicated nature of this relationship requires the skills of psychologists, social scientists, mathematicians, and engineers.

At Ramo-Wooldridge, human engineering, personnel selection, individual and system training, display design, and communications are successfully integrated into systems design and development by the technique of large-scale simulation.

Simulated inputs enable scientists to observe a system as it operates in a controlled environment and make possible the collection of data on performance, training, human engineering, maintenance, and logistics and support. Scientists and engineers use this data to assure the design, production, and delivery of a unified system capable of high performance and reliability.

Expanding programs at Ramo-Wooldridge in the broad areas of electronic systems technology, computers, and data processing have created outstanding opportunities for scientists and engineers. *For further information concerning these opportunities write to Mr. D. L. Pyke.*



RAMO-WOOLDRIDGE

P. O. BOX 90534, AIRPORT STATION • LOS ANGELES 45, CALIFORNIA

a division of **Thompson Ramo Wooldridge Inc.**



Precision . . .
Convenience . . .
Simplicity . . .


For Counting Tritium And Carbon-14



Model 314X

Automatic

Where considerable counting is done, the Model 314X Tri-Carb Spectrometer has proved invaluable in saving overall time and in utilizing laboratory personnel to better advantage. Completely automatic, it handles up to 100 samples and permanently records all data on paper tape. It can be operated around the clock without attendance.

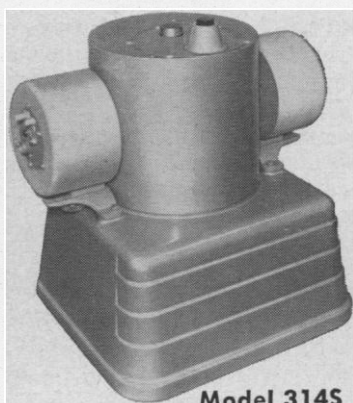

Model 314S


Semi-Automatic

For laboratories that anticipate increased counting in the foreseeable future, Model 314S provides efficient handling of present requirements, plus easy conversion to fully automatic operation at moderate cost. This can be done at any time simply by adding the 100-sample turntable, digital printer and the transistorized automatic control cabinet.

Manual

Model 314 is for laboratories not anticipating increased counting in the near future. Even this model, however, can be converted to fully automatic operation, if and when required. This is done by replacing the manual with the automatic sample chamber and shield and by adding the digital printer and transistorized automatic control cabinet.

All three models offer *all* the advantages of the Tri-Carb Liquid Scintillation Method for counting alpha- and beta-emitting isotopes: *sensitivity, versatility, simplicity of operation and ease of sample preparation.*

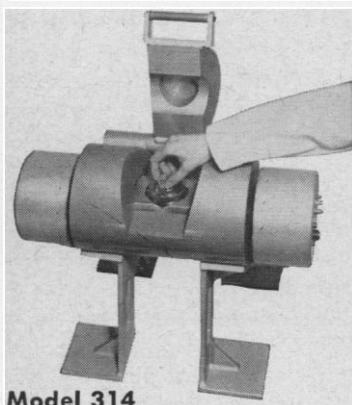

Model 314



For detailed information on the Tri-Carb Liquid Scintillation Method and specifications on Tri-Carb Spectrometers request latest bulletin.

Packard Instrument Company, Inc.

P.O. BOX 428-A • LA GRANGE, ILLINOIS