

J. Robert Willson, professor and chairman of the department of obstetrics and gynecology at Temple University, has been named chairman of the obstetrics and gynecology department in the University of Michigan medical school.

Gertrude Rand Ferree, retired research associate in ophthalmology at the Knapp Foundation of the Columbia University College of Physicians and Surgeons, has been awarded the Gold Medal of the Illuminating Engineering Society. She is the first woman to receive the organization's highest honor.

Recent Deaths

William S. Chepil, 59; agronomy professor, University of Kansas, 6 September.

Mintin A. Chrysler, 91; research professor emeritus of botany, Rutgers University, 16 August.

Walter Cook, 64; dean of the college of education, University of Minnesota; 9 September.

Virginia Griffing, 46; chemistry professor, Catholic University, Washington, D.C.; 5 September.

Arthur Warren Hixson, 83; professor emeritus of chemical engineering, Columbia University; 8 August.

Donald S. King, 74; former professor of thoracic medicine, Harvard University; 30 August.

Walter S. Loewe, 79; research professor emeritus of pharmacology, University of Utah medical college; 24 August.

Sisir Kumar Mitra, 72; India's National Research Professor of Physics; 13 August.

Stephen Rothman, 68; professor emeritus of medicine, University of Chicago, 31 August.


Charles Seymour, 78; retired president of Yale University; 11 August.

Erratum: In the report "Relative dating of Arlington Springs Man," by K. P. Oakley [*Science* 141, 1172 (20 Sept. 1963)], the value 10.4 in the line for Midland, Texas, in column 2 of Table 1 should have been 7.7.

Erratum: Several errors occurred in the announcement of awards for the Jane Coffin Childs Fund on page 894, 6 September. The announcement should have read:

The Jane Coffin Childs memorial fund for medical research is offering grants-in-aid and postdoctoral fellowships in the fundamental aspects of neoplastic growth. The awards are open to foreign as well as to U.S. citizens. Application deadlines for grants: 1 November, 1 March, and 1 September; for fellowships: 1 October (L. E. Lee, Jr., Childs Memorial Fund, 333 Cedar Street, New Haven 11, Conn.)

Now You Can Read Chloride Concentration Directly In Milliequivalents . . . with the

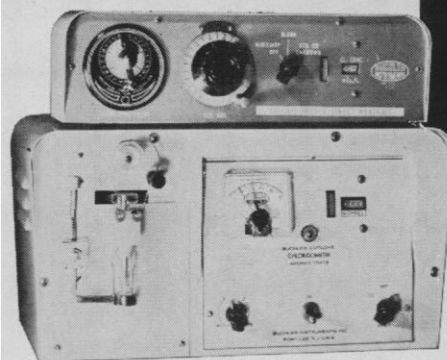

**Buchler
DIRECT
READER
ATTACHMENT**

**for the COTLOVE
CHLORIDOMETER®
AUTOMATIC TITRATOR**

If it has an end point, the CHLORIDOMETER will find it more quickly, accurately, automatically . . . in 6 steps and in less than 60 seconds!

DIVERSIFIED FOR ALL CHLORIDE TITRATION APPLICATIONS

The DIRECT READER speeds output! Automatically subtracts the reagent blank times and presents the net titration time in milliequivalents per liter on a digital register. Does not diminish the reliability and accuracy of the original automatic titrator. Variation with 0.1 ml. samples $\pm 0.05\%$. Easily attached to ANY Cotlove automatic chloride titrator. Installed free of charge at factory, with only shipping costs to pay.

SEND TODAY FOR COMPLETE DESCRIPTION

Direct Reader — Bulletin S 4-2050

Chloridometer — Bulletin S 4-2000


LABORATORY APPARATUS



PRECISION INSTRUMENTS

BUCHLER INSTRUMENTS, INC.

1327 16th Street, Fort Lee, New Jersey
Phone 201-945-1188 or call N.Y.C. direct LO 3-7844

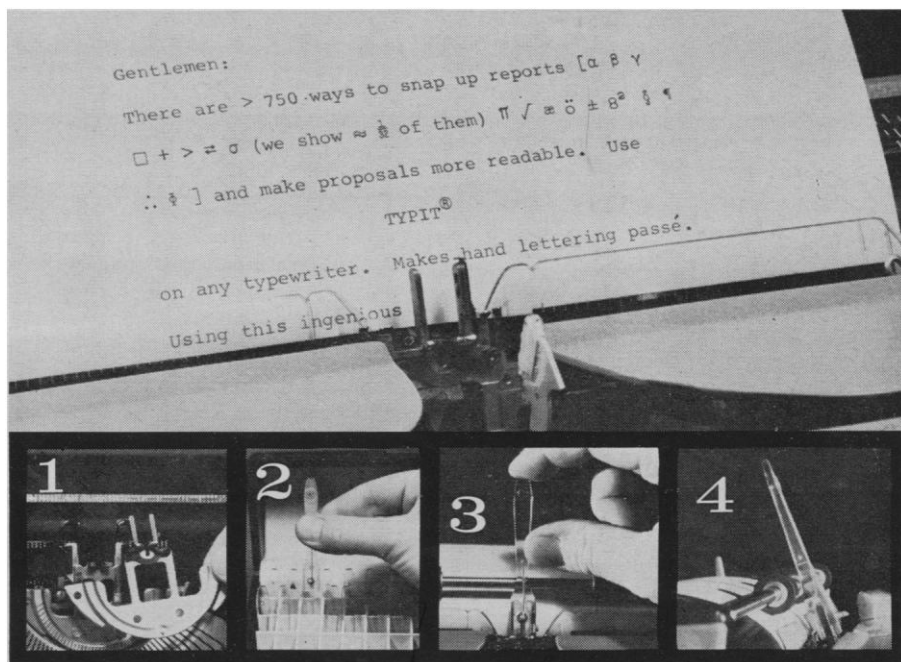

1 Have TYPIT® installed

2 Select the symbol

3 Insert the symbol

4 Strike any key:

type the symbol

NOW LEARN ABOUT

TYPIT®

manufactured by
mechanical enterprises, inc.
3127-A Colvin Street, Alexandria, Va.
Gentlemen:

Send: ☐ Catalog ☐ Representative

Name _____ Title _____

Company _____

Address _____

City _____ Zone _____ State _____