


TYGON® Flexible Plastic TUBING

- Flexible • Glass-clear
- Chemically inert
- 73 Standard sizes

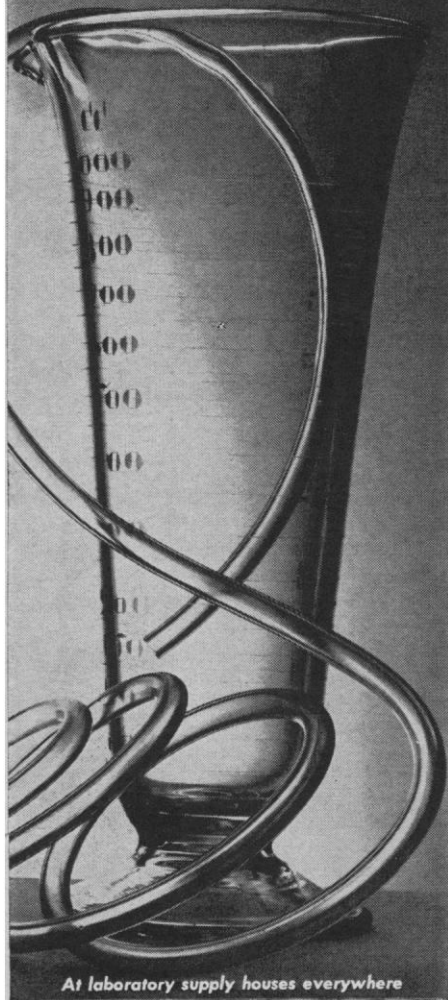

At laboratory supply houses everywhere

There is only one Tygon Tubing, a product of The United States Stoneware Company. For your protection, every foot is branded with the Tygon name and formulation number.

Plastic & Synthetics Division



U. S. STONWARE
Akron, Ohio 44309

Coast and Geodetic Survey Preliminary Report (17 April 1964).

This symposium was sponsored by the Department of Geology and Geophysics, University of California, Berkeley.

MARK N. CHRISTENSEN
BRUCE A. BOLT

Department of Geology and
Geophysics, University of
California, Berkeley

Botanical Field Meeting

Each year, usually toward the latter part of June, the North East Section of the Botanical Society of America has a field meeting. The central theme is plants in their natural environment. This year Drew University at Madison, New Jersey, was host (14-17 June 1964).

Kemble Widmer (state geologist for New Jersey) spoke on the relationship between the extremely complex geology (formations from archaean to the last glaciation are represented) and the distribution of plants in the Garden State. An exhibit of herbarium specimens of the flora of the Great Swamp was arranged by Florence M. Zuck. Visits by the group were made to the Great Swamp (the newest National Wildlife Refuge, dedicated 29 May 1964) and the Cedar Bog at High Point. The rather rare submerged aquatic *Hottonia inflata*, first reported from the Great Swamp by R. K. Zuck, was, perhaps, the outstanding botanical feature. The bog at High Point is one of the rare sites where all plants expected in a particular environment are well represented and can easily be seen from an encircling road. The display of the swamp calla was spectacular.

Louis Hand and Dorothy Everett spoke on the plants of the Pine Barrens of New Jersey in preparation for a field trip to this area. Everett's slides, produced by her and her husband, were some of the most technically perfect ever done for the flora of this area. The Pine Barrens are among the richest areas in the temperate region for number and variety of species of plants. Two outstanding and rare plants, the curly grass fern, *Schizaea pusilla*, and a curious morning glory, *Breweria Pickeringii* var. *caesariensis*, the latter a true endemic, were seen in the field, as well as hosts of three species of sun dews (*Drosera rotundi-*

folia, *D. intermedia*, and *D. filiformis*) and two orchids (*Pogonia ophioglossoides* and *Calopogon pulchella*).

At Island Heights, New Jersey, John Small (Rutgers University) spoke on the general botanical aspects of New Jersey and about Island Beach State Park in particular. He discussed the relationship of wind and wave action to the formation of Island Beach and the stabilizing influence of plants on the sand dunes in the area. Plant life is delicately balanced, and man's inroads must be curtailed if the area is to be maintained in its present state. Here we saw sea rocket (*Cakile edentula*), beach plum (*Prunus maritima*), and Spanish Oak (*Quercus falcata*) as plants typical of the region.

The host institution for the 1965 summer field meeting will be the University of Maine.

ROBERT K. ZUCK
Drew University, Madison, New Jersey

Forthcoming Events

September

16-18. American Assoc. of Medical Clinics, annual, Bal Harbour, Fla. (The Association, Box 58, Charlottesville, Va.)

17-18. Computing, 7th annual Northwest conf., Seattle, Wash. (R. K. Smith, Northwest Computing Assoc., Box 836, Seahurst, Wash.)

17-18. Engineering Management, conf., Cleveland, Ohio. (Inst. of Electrical and Electronics Engineers, Box A, Lenox Hill Station, New York, N.Y. 10021)

17-18. Polypropylene Fibers, symp., Southern Research Inst., Birmingham, Ala. (W. C. Sheehan, SRI, 2000 Ninth Ave. S., Birmingham, Ala. 35205)

17-19. Cancer, 5th natl. conf., Philadelphia, Pa. (American Cancer Soc., 219 E. 42 St., New York, N.Y. 10017)

17-19. British Assoc. of Urological Surgeons, annual, Sheffield, England. (Joint Secretariat, 47 Lincoln's Inn Fields, London, W.C.2, England)

17-20. Science Education, intern. conf., Banff, Alberta, Canada. (S. Trieger, Faculty of Education, Univ. of Alberta, Edmonton, Canada)

18. Hungarian Chemical Soc., Tihany. (M. T. Beck, Szabadsag ter 17, Budapest 5, Hungary)


19-26. Gynecology and Obstetrics, 4th world congr., Buenos Aires, Argentina. (R. Lede, Primera Catedra de Ginecología, Hospital de Clínicas, Córdoba 2149, Buenos Aires)

19-27. Scientific Films Assoc., 18th intern. congr., Athens, Greece. (SFA, 38, Avenue des Ternes, Paris 17^e, France)

20-23. Ceramic-Metal Systems, American Ceramic Soc., French Lick, Ind. (ACS, 4055 North High St., Columbus, Ohio)

20-23. American Inst. of Chemical Engineers, Las Vegas, Nev. (F. J. Van

LABCO's newest surgical, transfer and holding units

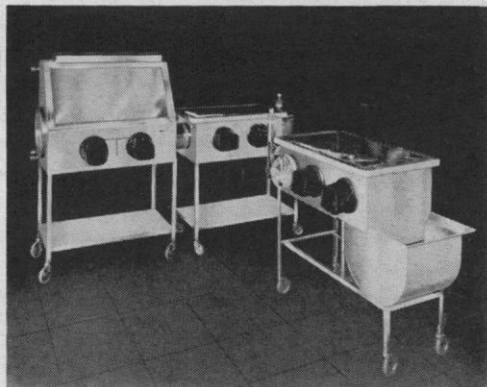

for the most sophisticated techniques of GERM-FREE animal research

These units were designed for germ-free research procedures used in the world's most advanced laboratories. All metal parts are of life-long corrosion-resistant stainless steel.

Long-term holding unit (GF 5051), left, has double transfer sleeves, is equipped with a foolproof valve system for continuous freon-testing of gloves. Wide glass front makes for excellent viewing conditions. Interior illuminated from outside by fluorescent light. Overall dimensions: 24" W. x 36" H. x 48" L.

Surgical unit (GF 4051), right, consists of

a germicide trough opening into a sterilized chamber equipped with air blower and filter to maintain germ-free environment. Available 26" W. x 36" H. x 64" L.; and 22" W. x 27" H. x 46" L.

Transfer unit (GF 4061) has two sets of gloves, wide pass-through door, air filter and blower to assure uninterrupted germ-free conditions. Standard size: 26" W. x 16" H. x 46" L.

Write for detailed information on LABCO's complete line of germ-free research equipment and enclosures.


LABCO

A DIVISION OF PARTSCO, INC.
2977 Lamb Avenue • Columbus, Ohio 43219

MINIMUM CONTACT—MAXIMUM SAFETY

with self-sticking
TIME LABORATORY
TAPES and LABELS

Self-sticking tapes and labels eliminate a direct source of personal contamination in laboratories. Pre-printed or plain tapes and labels provide a quick means of marking laboratory equipment. Just write necessary data on label (use pencil, pen or grease marker) and place it on any surface — glass, metal or plastic. Labels stick tight through autoclave (up to 250°), deep freeze (to -70°), or water bath. When no longer needed these tapes and labels can be quickly removed leaving no sticky residue. Vinyl Coated — available in white or colors.

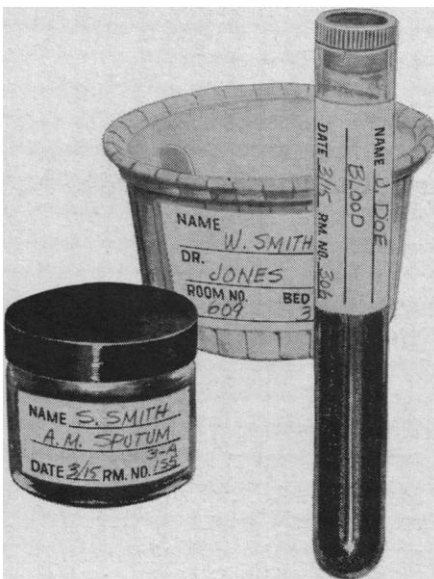

See your laboratory or hospital supplier for a complete selection of Time Tapes and Labels.

PROFESSIONAL TAPE CO., INC.
365M Burlington Avenue • Riverside, Illinois 60546

Antwerpen, 345 E. 47 St., New York, N.Y. 10017)

20-24. American Soc. of Oral Surgeons, Chicago, Ill. (E. W. Gilgan, 119 North Michigan Ave., Chicago 11)

20-25. Neuroradiology, 7th symp., New York, N.Y. (J. M. Taveras, Neurological Inst., Columbia-Presbyterian Medical Center, New York, N.Y. 10032)

20-26. Anaesthesiology, 3rd world congr., São Paulo, Brazil. (L. Rodrigues Alves, Caixa Postal 330, São Paulo)

21-24. Agricultural Engineering, intern. congr., Lausanne, Switzerland. (P. Regamey, Etat de Vaud, 14. Cité-Devant Lausanne)

21-24. German Soc. for Psychology, 24th congr., Vienna, Austria. (J. Rohrer, Deutsche Gesellschaft für Psychologie, Am Hof 1e, 5300 Bonn, Germany)

21-25. Animal Care Panel, 15th annual, New York, N.Y. (ACP, P.O. Box 1028, Joliet, Ill. 60434)

21-26. Documentation, 30th intern. conf., The Hague, Netherlands. (Intern. Federation for Documentation, 7 Hofweg, The Hague)

21-26. Electrochemical Thermodynamics and Kinetics, intern., London, England. (M. Fleischmann, Dept. of Physical Chemistry, Univ. of Newcastle upon Tyne, England)

21-26. Parasitology, 1st intern. congr., Rome, Italy. (A. Corradetti, Istituto di Parassitologia, Citta Universitaria, Rome)

22-24. Many-Body Problems in Physics and Chemistry, conf., Manchester, England. (Administration Assistant, Inst. of Physics and the Physical Soc., 47 Belgrave Sq., London, S.W.1, England)

22-25. Middle East Neurological Soc., Ankara, Turkey. (N. Avman, c/o Hacettepe Tip Fakültesi, Ankara)

22-25. Soil Micromorphology, 2nd intern., Arnhem, Netherlands. (A. Jongerius, Stichting voor Bodemartering, Postbus 10, Bennekom, Netherlands)

22-28. Radiology, 11th intern. congr., Rome, Italy. (L. Turano, Istituto de Radiologia, Univ. of Rome, Rome)

23-26. British Assoc. for Cancer Research, annual, Edinburgh, Scotland. (J. G. Bennette, Courtauld Inst., Middlesex Hospital, London, W.1, England)

23-26. Viral Diseases of Poikilothermic Vertebrates, New York, N.Y. (S. P. Snieszko, Eastern Fish Disease Laboratory, Leestown, P.O. Kearneyville, W.Va.)

24-27. American Medical Writers' Assoc., annual, Philadelphia, Pa. (American Medical Writers Assoc., 2000 P St., NW, Washington, D.C.)


25-26. Communications, 3rd Canadian symp., Montreal, Quebec. (F. G. R. Warren, P.O. Box 802, Station B, Montreal)

27-30. Society of American Foresters, 64th annual, Denver, Colo. (SAF, Mills Bldg., Washington, D.C. 20006)

27-1. Water Pollution Control Federation, 37th annual, Bal Harbour, Fla. (WPCF, 3900 Wisconsin Ave., Washington, D.C. 20016)

27-2. Society of Motion Picture and Television Engineers, 96th technical conf., New York, N.Y. (SMPTE, 619 W. 54 St., New York, N.Y. 10019)

28-30. Circuit and System Theory, conf., Monticello, Ill. (W. R. Perkins,

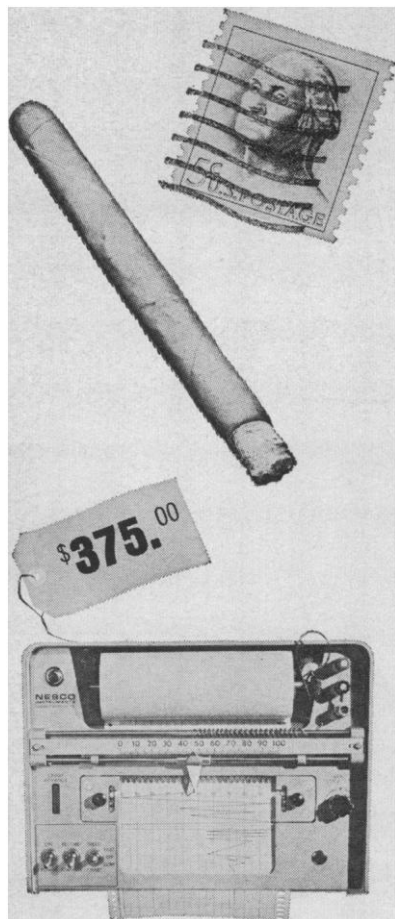

All three are

bargains

The third is a NESCO JY100-1 10mv, 5-inch chart recorder with ½% accuracy, ¼% sensitivity, ½ second span response, dual chart drive and capillary pen. One of the 12 units in this Series will meet 95% of your recording requirements: JY110 for 10mv to 100v ranges; JY120 for 1mv to 10v ranges. Options provide second chart speeds, zener references, event markers, integrator, rack mounting, etc. Ten-inch chart widths also available.

Sales offices in major cities.

Send for additional information and a

TEN DAY FREE TRIAL

Name _____

Company _____

Position _____

Address _____

City _____

State _____

Phone _____

**NESCO
INSTRUMENTS**

DIVISION OF DATAPULSE, INCORPORATED
509 HINDRY AVE, INGLEWOOD 1, CALIFORNIA
OR 8-3983 / TWX: 213-673-0390

Dept. of Electrical Engineering, Univ. of Illinois, Urbana)

28-2. Society for Applied Spectroscopy, 3rd natl. conf., Cleveland, Ohio. (E. Yeager, Dept. of Chemistry, Western Reserve Univ., Cleveland 44106)

29-1. Physics of Failure in Electronics, 3rd annual symp., Chicago, Ill. (M. Goldberg, IIT Research Inst., 10 W. 35 St., Chicago 60616)

29-1. Physics and Nondestructive Testing, symp., Dayton, Ohio. (W. J. McGonagle, Southwest Research Inst., P.O. Box, 2296, San Antonio, Tex. 78206)

29-1. American College of Preventive Medicine, New York, N.Y. (R. E. Coker, Jr., Box 1263, Chapel Hill, N.C.)

29-1. Technical Assoc. of the Pulp and Paper Industry, 1964 testing conf., Portsmouth, N.H. (TAPPI, 360 Lexington Ave., New York, N.Y. 10017)

29-2. American Roentgen Ray Soc., 65th annual, Minneapolis, Minn. (C. A. Good, Mayo Clinic, Rochester, Minn.)

30-2. American Council on Education, 47th annual, San Francisco, Calif. (L. Wilson, ACE, 1785 Massachusetts Ave., NW, Washington, D.C. 20006)

30-2. Earth Sciences, intern. conf., Cambridge, Mass. (H. G. Houghton, Dept. of Meteorology, Massachusetts Inst. of Technology, Cambridge)

30-2. Standards Engineers Soc., 13th annual, New York, N.Y. (SES, 170 Livingston Ave., New Providence, N.J.)

30-2. Vacuum, 11th natl. symp., Chicago, Ill. (G. H. Bancroft, Bendix-Balzars Vacuum, Inc., 1645 St. Paul St., Rochester, N.Y. 14621)

30-4. Spectroscopy, 11th intern. conf., Belgrad, Yugoslavia. (Sekretarijat, Prodrodno-matematicki fakultet, Fizickochemijski zavod Belgrad, Studeniski trg., 16, Bloc C, Yugoslavia)

October

1-2. Emission of Electrons from Solids, conf., Univ. of Keele, Keele, England. (Inst. of Physics and the Physical Soc., 47 Belgrave Sq., London, S.W.1, England)

1-3. American Assoc. for Surgery of Trauma, Chicago, Ill. (S. R. Gaston, 18 Fort Washington Ave., New York 10022)

2-3. Council for International Organizations of Medical Societies, 6th general assembly, Brussels, Belgium. (P. A. Messerli, 6 rue Franklin, Paris 16^e, France)


2-3. Psychotherapy of the Family, symp., Milwaukee, Wis. (B. C. Burris, Milwaukee Psychiatric Hospital, Milwaukee 53213)

2-9. Radiology, 8th inter-American congr., Caracas, Venezuela. (R. Merinfeld, Apartado Postal 9362 Candelaria, Caracas)

3-4. New England Intercollegiate Geological Conf., Yale Univ., New Haven, Conn. (J. Rodgers, Dept. of Geology, Yale Univ., New Haven 06520)

3-4. Medical Radiobiology, 7th natl. congr., Pisa, Italy. (Segreteria, Inst. di Radiologia dell'Università, Spedali Riuniti de "S. Chiara," Pisa)

3-13. Weights and Measures, 12th conf., Paris, France. (Intern. Bureau of Weights and Measures, Pavillon de Breteuil, Sèvres, Seine-et-Oise, France)

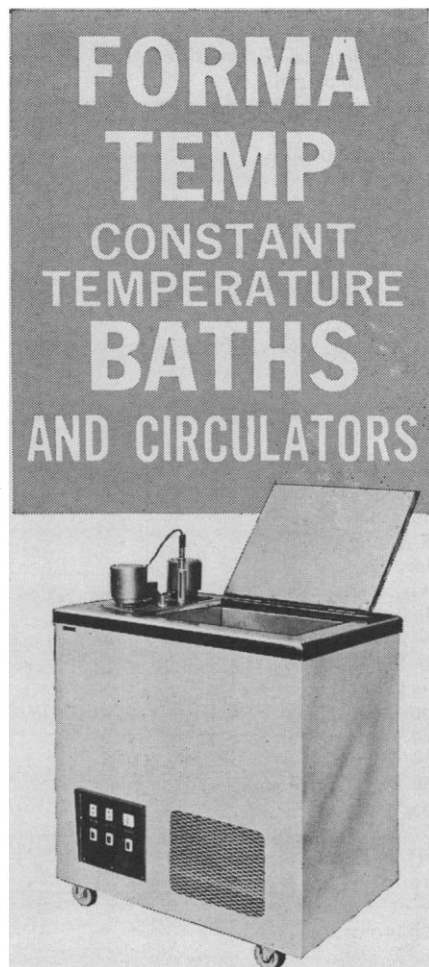

**FORMA
TEMP
CONSTANT
TEMPERATURE
BATHS
AND CIRCULATORS**



**High
B.T.U.
Capacity
at
Modest
Prices!**

- Refrigerated and Heated mechanically. Has self-contained, 2-pump circulation system for inside and outside circulation.
- Ultra-Sensitive Accuracy controlled to $\pm 0.02^\circ \text{C}$.
- Versatile, Always Reliable and easy to use as a bath or circulator.
- Interchangeable Solid State transistorized electronic control panel.
- Shipped as Complete Units, entirely self-contained and ready to operate.
- Available in floor models and table models, all stainless steel.

Write for **FREE Literature**



**FORMA
SCIENTIFIC
inc.**

P.O. BOX 649

MARIETTA, OHIO

4-9. American College of Surgeons, clinical congr., Chicago, Ill. (American College of Surgeons, 55 East Erie St., Chicago 60611)

5-6. Enzyme Regulation, 3rd intern. symp., Indianapolis, Ind. (G. Weber, Indiana Univ. School of Medicine, Indianapolis)

5-7. Association of Medical Illustrators, annual, Los Angeles, Calif. (C. Bridgman, Dept. of Anatomy, UCLA Center for Health Sciences, Los Angeles)

5-7. Radiation Effects on Electronics, natl. meeting, American Nuclear Soc., Syracuse, N.Y. (ANS, 244 East Ogden Ave., Hinsdale, Ill.)

5-8. Clay Mineral Soc., Univ. of Wisconsin, Madison. (M. L. Jackson, Univ. of Wisconsin College of Agriculture, Madison 6)

5-8. American Documentation Inst., annual, Philadelphia, Pa. (B. F. Cheydleur, Philco Corp., Willow Grove, Pa. 19090)

5-8. Research Methods and Instrumentation, 14th symp., Bethesda, Md. (J. B. Davis, Natl. Insts. of Health, Bethesda, Md. 20014)

5-9. Aeronautics and Space Engineering, Soc. of Automotive Engineers, Los Angeles, Calif. (E. V. Albert, 399 N. Sepulveda Blvd., El Segundo, Calif. 90245)

5-9. American Public Health Assoc., New York, N.Y. (B. F. Mattison, 1790 Broadway, New York, N.Y.)

5-10. German Physical Soc., Düsseldorf. (GPS, Gänsheidestr. 15a, Stuttgart, Germany)

6-8. Analytical Chemistry in Nuclear Technology, 8th conf., Gatlinburg, Tenn. (C. D. Susano, Oak Ridge Natl. Laboratory, P.O. Box X, Oak Ridge, Tenn.)

6-8. Cornea, world congr., Washington, D.C. (J. H. King, 1746 K St., NW, Washington, D.C.)

6-9. Optical Soc. of America, annual, New York, N.Y. (M. E. Wurga, OSA, 1155 16th St., NW, Washington, D.C. 20006)

6-9. Space Electronics, symp., Las Vegas, Nev. (C. H. Doersam, Jr., Box 177, Port Washington, N.Y.)

6-10. Clinical and Experimental Hypnosis, 16th annual, Pittsburgh, Pa. (Soc. for Clinical and Experimental Hypnosis, 353 W. 57 St., New York, N.Y. 10019)

7. California Acad. of Sciences, San Francisco. (G. E. Lindsay, California Academy of Sciences, Golden Gate Park, San Francisco)


7-9. Structure and Functions of Epidermal Barriers, intern. symp., Brno, Czechoslovakia. (Zd. Vlašin, Dermatological Clinic, 53, Pekařská, Brno)

7-9. Electronic Information Handling, natl. conf., Pittsburgh, Pa. (A. Kent, Univ. of Pittsburgh, Pittsburgh)

7-9. Institute of Management Sciences (TIMS)/Operations Research Soc. of America (ORSA), joint natl. meeting, Minneapolis, Minn. (G. B. Davis, School of Business Administration, Univ. of Minnesota, Minneapolis)

8-10. Agricultural Meteorology, 6th conf., Lincoln, Nebr. (American Meteorological Soc., 45 Beacon St., Boston 8, Mass.)

9-10. Undergraduate Courses and Curricula, midwestern regional conf., Univ.

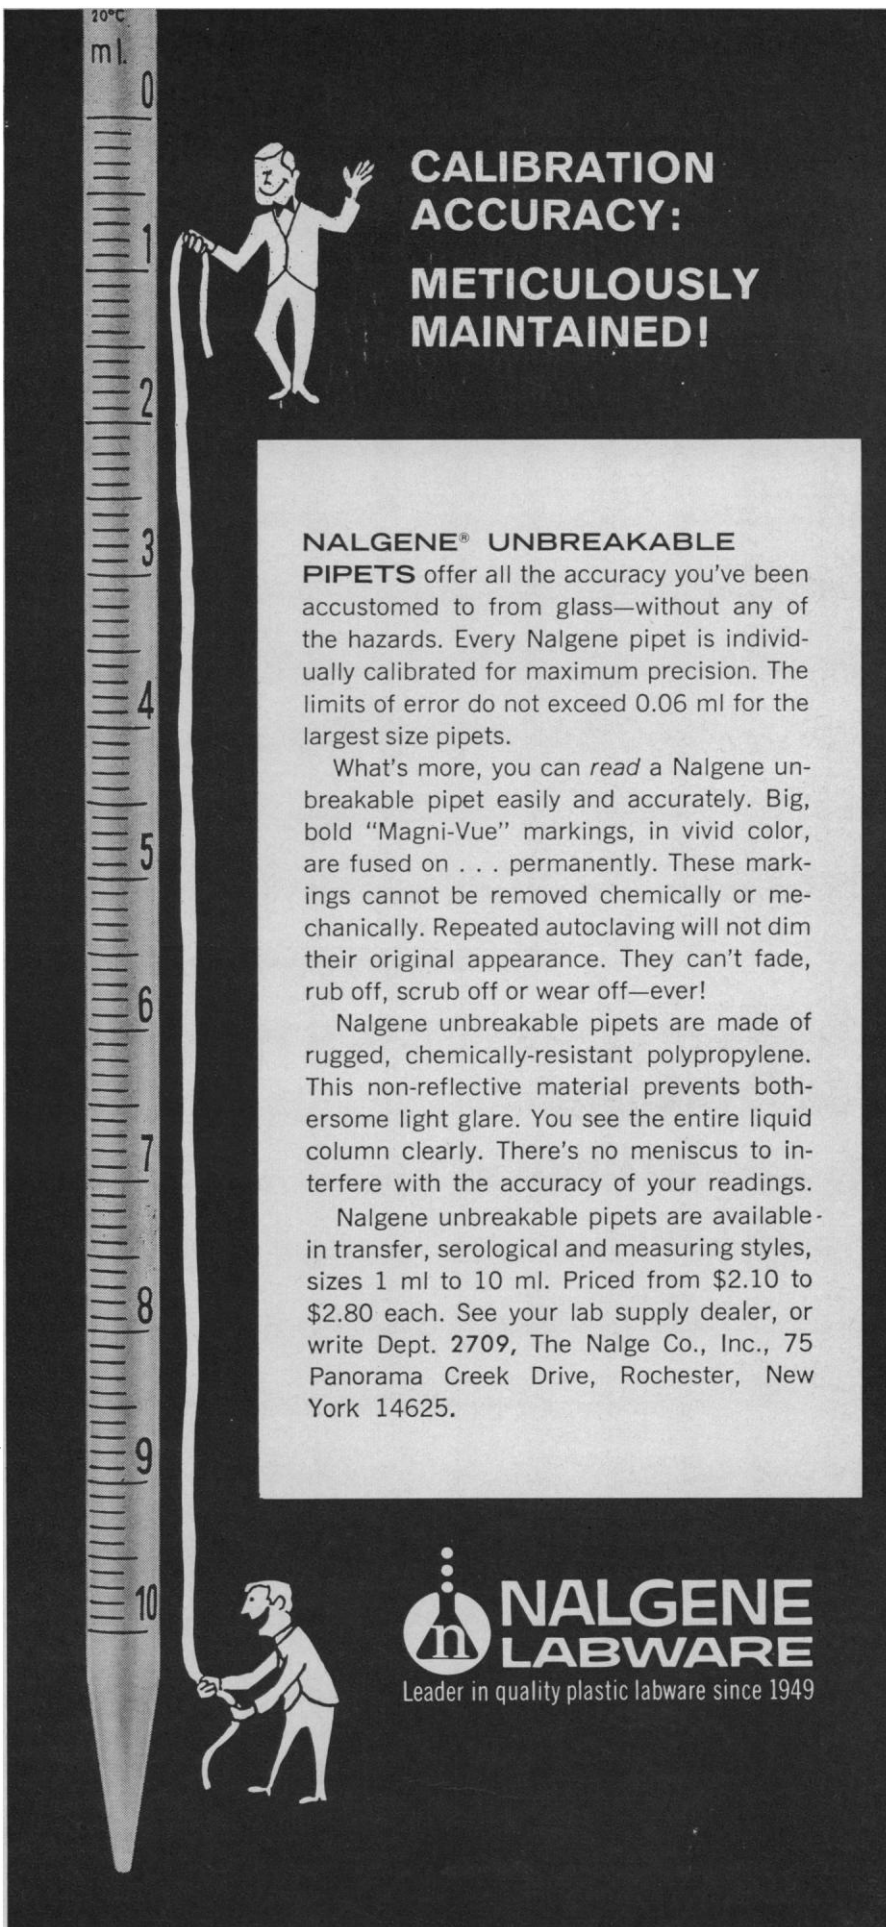


CALIBRATION ACCURACY: METICULOUSLY MAINTAINED!

**NALGENE® UNBREAKABLE
PIPETS** offer all the accuracy you've been accustomed to from glass—without any of the hazards. Every Nalgene pipet is individually calibrated for maximum precision. The limits of error do not exceed 0.06 ml for the largest size pipets.

What's more, you can *read* a Nalgene unbreakable pipet easily and accurately. Big, bold "Magni-Vue" markings, in vivid color, are fused on . . . permanently. These markings cannot be removed chemically or mechanically. Repeated autoclaving will not dim their original appearance. They can't fade, rub off, scrub off or wear off—ever!

Nalgene unbreakable pipets are made of rugged, chemically-resistant polypropylene. This non-reflective material prevents bothersome light glare. You see the entire liquid column clearly. There's no meniscus to interfere with the accuracy of your readings.

Nalgene unbreakable pipets are available in transfer, serological and measuring styles, sizes 1 ml to 10 ml. Priced from \$2.10 to \$2.80 each. See your lab supply dealer, or write Dept. 2709, The Nalge Co., Inc., 75 Panorama Creek Drive, Rochester, New York 14625.





**NALGENE
LABWARE**
Leader in quality plastic labware since 1949

NOW L&N pH METERS ARE AS CLOSE AS YOUR LAB SUPPLY DEALER

L&N pH Meters for laboratory use are now sold exclusively through a nationwide network of franchised dealers. With these expanded facilities, L&N pH Meters—and electrodes, parts and supplies as well—are stocked near you for easy, prompt delivery. Furthermore these dealers—with more than 100 convenient outlets—stand ready to assist you in your pH applications and to provide authorized factory service for this equipment. Need names? Write us at 4962 Stenton Avenue, Philadelphia 44, Pennsylvania for the complete list of dealers.



LEEDS & NORTHRUP
Pioneers in Precision

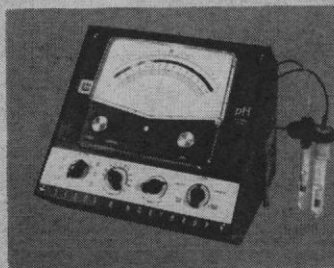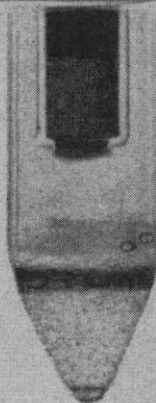

Worth writing for

ADM-30, "Detection and Analysis of Contamination" outlines the measurement of particulate contamination with Millipore filters as applied to hydraulic fluids, air, fuels, lubricants, solvents, garments, surfaces and other aerospace and industrial fluids. To get a copy of this manual, write to


Millipore

FILTER CORPORATION
145 Ashby Rd., Bedford, Mass.

Millipore® filters are cellulose plastic porous membranes made in twelve pore-size grades from 8 microns down to 10 millimicrons. In microfiltration or analysis, all matter larger than the filter pore size is screened from fluids and retained on the filter surface.

36 PAGES
FREE
OF CHARGE

OUTSTANDING RESISTANCE



to

HEAT AND COLD
SOLVENTS
ACIDS
CHEMICALS
FUELS


PLV

Viton® Tubing, Bar, Rod Stock
Outstanding features of PLV TUBING, BAR and ROD STOCKS are their exceptional resistance to fluids, heat and cold.

Applications from -95°F. to $+600^{\circ}\text{F.}$
Resistance to hydrocarbons, H_2SO_4 , HCl , HNO_3 , caustic solutions, and many other corrosive materials.

PLV products show prolonged operational life . . . cut down time . . . eliminate production headaches.

*E. I. DuPont



Write for information:
**PELMOR
LABORATORIES, INC.**
Research - Development
Processing - Consulting
403 Lafayette Street
Newtown, Pennsylvania
215-968-3825

of Kansas, Lawrence. (R. E. McNair, Assoc. of Midwest College Biology Teachers, Univ. of Kansas, Lawrence)

10. Paleontological Research Inst., annual, Ithaca, N.Y. (R. S. Harris, 109 Dearborn Pl., Ithaca 14850)

11-14. American Oil Chemists Soc., Chicago, Ill. (C. H. Hauber, AOCS, 35 E. Wacker Dr., Chicago 60601)

11-14. International Scientific Radio Union/Inst. of Electrical and Electronics Engineers, joint meeting, Univ. of Illinois, Urbana. (E. C. Jordan, Dept. of Electrical Engineering, Univ. of Illinois, Urbana)

11-15. Diseases of the Chest, 8th intern. congr., Mexico City, D.F. (M. Kornfeld, American College of Chest Physicians, 112 E. Chestnut St., Chicago 11, Ill.)

11-15. Electrochemical Soc., Washington, D.C. (ES, 30 E. 42 St., New York, N.Y. 10017)

11-16. Allergology, 5th intern. congr., Madrid, Spain. (F. Lahoz, Clínica de la Concepción, Avda. Reyes Católicos 2, Madrid 3)

11-16. American Assoc. of Medical Record Librarians, annual, Miami Beach, Fla. (M. J. Waterstraat, RRL, 840 North Lake Shore Dr., Chicago, Ill. 60611)

11-16. Pan American Assoc. of Ophthalmology, 7th, Montreal, Canada. (J. W. McKinney, PAAO, 921 Exchange Bldg., Memphis, Tenn.)

11-16. American Soc. of Plastic and Reconstructive Surgery, annual, San Francisco, Calif. (P. P. Pickering, 2850 Sixth Ave., Suite B, San Diego, Calif.)

12-14. Aviation Pathology, 5th scientific session, Washington, D.C. (Secretary, Joint Committee on Aviation Pathology, Armed Forces Inst. of Pathology, Washington, D.C. 20305)

12-14. Entry Technology, American Inst. of Aeronautics and Astronautics conf., Williamsburg, and NASA-Langley Research Center, Va. (S. P. Johnston, AIAA, 1290 Sixth Ave., New York, N.Y.)

12-14. Protection Against Radiations in Space, 2nd symp., Gatlinburg, Tenn. (F. C. Maienschein, Oak Ridge Natl. Laboratory, P.O. Box X, Oak Ridge, Tenn.)

12-15. Instrument Soc. of America, 19th Instrument-Automation conf., New York, N.Y. (ISA, 530 William Penn Pl., Pittsburgh, Pa. 15219)

13-15. Air Force Science and Engineering, 11th symp., Brooks Air Force Base, Tex. (G. E. Schafer, Headquarters Aerospace Medical Div., Brooks AFB)

13-16. Calorimetry, 19th conf., Washington, D.C. (W. N. Hubbard, Argonne Natl. Laboratory, 9700 S. Cass Ave., Argonne, Ill.)

13-16. Lubrication, 1st intern. conf., American Soc. of Mechanical Engineers/American Soc. of Lubrication Engineers, Washington, D.C. (W. J. Anderson, MS 6-1, NASA-Lewis Research Center, 21000 Brookpark Rd., Cleveland, Ohio)

13-17. Electron Microscopy Soc. of America, 22nd annual, Detroit, Mich. (A. R. Taylor, Virus Div., Parke, Davis & Co., Detroit 32)

14-15. American Soc. of Tool and Manufacturing Engineers, Minneapolis, Minn. (R. E. Gariss, 6523 El Pulcro St., Long Beach, Calif.)



HONEYWELL STROBONAR FOR PHOTOMICROGRAPHY

The new Honeywell Model 52A Strobosonar Electronic Flash Unit is a versatile and economical light source for all types of photomicrography, black and white or color.

Concentric with the electronic flash tube is an incandescent light with which the unit is positioned for correct light reflection. Users report intensity of flash is excellent even at maximum magnification. Absence of heat protects specimens from physical change and warping.

A universal bracket fits the unit for many assignments in both laboratory and field. The 52A can be flashed by any camera synchronized for electronic flash. Specify: Model 52A Strobosonar Electronic Flash; 110V-AC, 90 Watts; 16 ft. cord; 3 lbs.; 8" x 4½" x 5".

For illustrated folder on the 52A Strobosonar Electronic Flash, please write: David Moore, Mail Station 209, Honeywell, Denver, Colorado 80210.

Honeywell
PHOTOGRAPHIC PRODUCTS

11 SEPTEMBER 1964

14-16. **Gaseous Electronics**, 7th conf., Atlantic City, N.J. (S. Schneider, U.S. Army Electronics R&D Laboratories, Fort Monmouth, N.J. 07703)

14-16. **Parenteral Drug Assoc.**, annual conv., New York, N.Y. (PDA, Broad and Chestnut Sts., Philadelphia 7, Pa.)

14-16. **Remote Sensing of Environment**, 3rd symp., Ann Arbor, Mich. (D. C. Parker, Univ. of Michigan, Box 618, Ann Arbor 48107)

14-16. **Sonics and Ultrasonics**, symp., Santa Monica, Calif. (A. H. Meitzler, Bell Telephone Laboratories, Inc., Murray Hill, N.J.)

15-16. **Bioenergetics**, symp., Univ. of Western Ontario, London, Ontario, Canada. (K. P. Strickland, Dept. of Biochemistry, Faculty of Medicine, Univ. of Western Ontario, London)

15-16. **Systems Science**, first annual conf., Inst. of Electrical and Electronics Engineers, Univ. of Pennsylvania, Philadelphia. (H. G. Sparks, Moore School of Engineering, Univ. of Pennsylvania, Philadelphia)

15-17. **Correlation of Particles Emitted in Nuclear Reactions**, intern. conf., Gatlinburg, Tenn. (A. Zucker, Oak Ridge Natl. Laboratory, P.O. Box X, Oak Ridge, Tenn. 37830)

15-17. **Central Neuropsychiatric Assoc.**, Denver, Colo. (W. P. Shelton, 8215 Westchester Dr., Dallas 25, Tex.)

15-22. **Association of American Medical Colleges**, 75th annual, Denver, Colo. (P. J. Sanazaro, Div. of Education, Assoc. of American Medical Colleges, 2530 Ridge Ave., Evanston, Ill. 60201)

16-17. **Western Industrial Medical Assoc.**, Los Angeles, Calif. (C. Einert, 2151 Berkeley Way, Berkeley 4, Calif.)

16-17. **Systemics**, 11th annual symp., St. Louis, Mo. (H. C. Cutler, Missouri Botanical Garden, St. Louis)

16-20. **American Medical Women's Assoc.**, New York, N.Y. (M. A. Sears, Anderson Hospital, Houston 25, Tex.)

16-24. **American Soc. of Clinical Pathologists**, annual, Bal Harbor, Fla. (ASCP, 445 N. Lake Shore Dr., Chicago, Ill.)

17-18. **Society for Psychophysiological Research**, 4th annual, Washington, D.C. (L. A. Gustafson, SPR, 74 Fenwood Rd., Boston, Mass. 02115)

17-20. **College of American Pathologists**, Bal Harbor, Florida. (E. E. Simard, Box 136, Salinas, Calif.)

17-25. **International Aeronautic Federation**, general conf., Tel Aviv, Israel. (M. J. Randleman, Natl. Aeronautic Assoc., 1025 Connecticut Ave., NW, Washington, D.C. 20036)

18-21. **Association of Military Surgeons of the U.S.**, Washington, D.C. (Brig. Gen. F. E. Wilson, Suite 132, 1500 Massachusetts Ave., NW, Washington, D.C. 20005)

18-22. **Metallurgical Soc.**, fall meeting, Philadelphia, Pa. (D. A. Parks, Inst. of Metals Div., Metallurgical Soc. of AIME, 345 E. 47 St., New York, N.Y. 10017)


18-23. **American Acad. of Ophthalmology and Otolaryngology**, Chicago, Ill. (W. L. Benedict 15 Second St., SW, Rochester, Minn. 55901)

18-24. **Dental Education**, 2nd Latin American seminar, Mexico City. (D. Restrepo, Pan American Sanitary Bureau, 1501 New Hampshire Ave., NW, Washington, D.C. 20036)

Portable Cool...

Glow Box

THE SCIENTIST'S LIGHT BOX

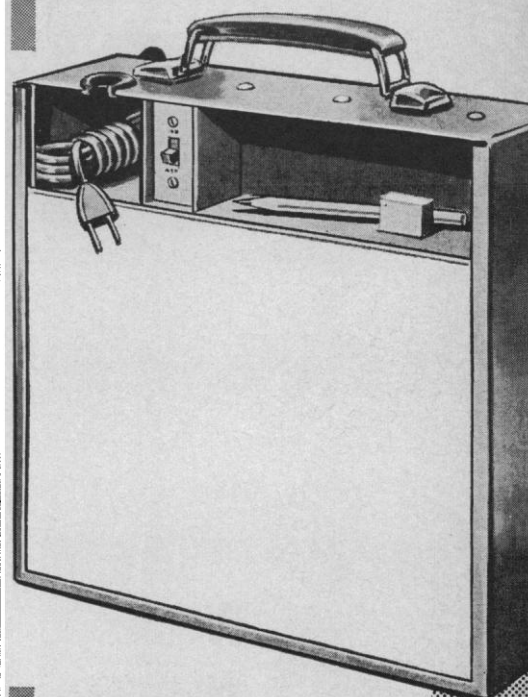


**TILTS EASILY
FOR TABLE-TOP
USE**

Model 12-12D-2X for charts
curves, spectra, X-ray film
8½" x 11"\$35.50
Model 12-20E-2X for double
size sheets 11" x 18" ..\$60.00



**FITS STANDARD
DESK DRAWER FOR
STORAGE OR USE**

Keep GLOW BOX in your
desk drawer immediately
available whenever you wish
to examine, compare, or
trace. It's so convenient!



**STANDS
UPRIGHT FOR
DEMONSTRATIONS**

The uniform, diffuse light
focuses attention on displays
of samples for lectures,
demonstrations, etc.




SEND CARD FOR LITERATURE



INSTRUMENTS for
RESEARCH and
INDUSTRY

VICKERS Image Splitting Measuring Eyepiece

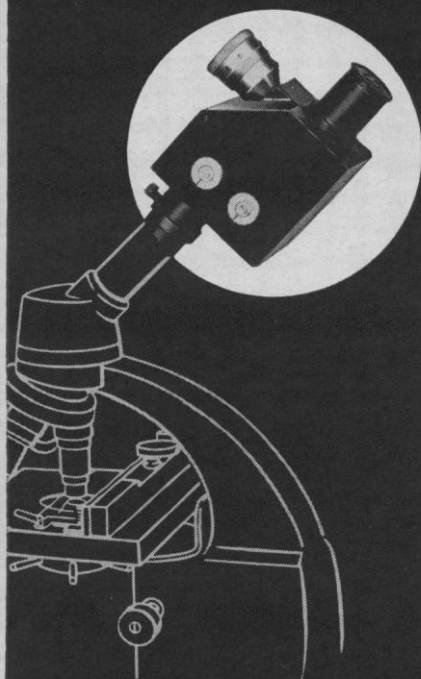

A revolutionary measuring technique

Unequalled accuracy of measurement
(0.1μ — $0.00005''$ or better)

Unequalled reproducibility of
measurement

Unequalled ease, speed and
simplicity of measurement



The ability to make precise
comparative measurements without
actually measuring at all

Send for brochure CM011550



**COOKE,
TROUGHTON
& SIMMS, Inc.**

91 WAITE STREET, MALDEN 48, MASSACHUSETTS

19-20. **Unconventional Inertial Sensors**, symp. (secret), Farmingdale, N.Y. (R. E. McIntyre, RMG-8, Bureau of Naval Weapons, Washington 25, D.C.)

19-21. **Academy of Psychosomatic** Soc. of Mechanical Engineers, Lafayette, Ind. (T. P. Goodman, Technological Inst., Northwestern Univ., Evanston, Ill.)

19-21. **Academy of Psychosomatic Medicine**, New York, N.Y. (R. N. Rutherford, 200 Broadway, Seattle, Wash.)

19-21. **Technical Assoc. of the Pulp and Paper Industry**, plastics-paper conf., Washington, D.C. (TAPPI, 360 Lexington Ave., New York 10017)

19-22. **Association of Official Agricultural Chemists**, 78th annual, Washington, D.C. (L. G. Ensminger, AOAC, Box 540, Benjamin Franklin Station, Washington, D.C. 20044)

19-23. **American Soc. of Civil Engineers**, New York, N.Y. (W. H. Wisely, ASCE, 345 E. 47 St., New York, N.Y. 10017)

19-23. **American Soc. for Metals**, Philadelphia, Pa. (A. R. Putnam, ASM, Metals Park, Ohio)

19-23. **Radiochemical Methods of Analysis**, symp., Salzburg, Austria. (Intern. Atomic Energy Agency, 11 Karntnerring, Vienna 1, Austria)

20-30. **Nov. UNESCO**, 13th session, general conf., Paris, France. (UNESCO, Place de Fontenoy, Paris 7^e)

21-22. **American Heart Assoc.**, Council on Arteriosclerosis, annual, Atlantic City, N.J. (D. M. Smith, AHA, 44 E. 23 St., New York, N.Y. 10010)

21-22. **Industrial Hygiene Foundation**, annual, Pittsburgh, Pa. (R. T. P. deTreville, IHF, 4400 Fifth Ave., Pittsburgh 15213)

21-23. **Aerospace and Navigational Electronics**, 11th East Coast conf., Baltimore, Md. (M. Hastings, Mail No. 1281 A, Baltimore Space and Defense Center, Westinghouse Electric Corp., P.O. Box 1693, Baltimore 21203)

21-23. **Pain**, intern. symp., Detroit, Mich. (R. S. Knighton, 2799 W. Grand Blvd., Detroit)

21-23. **Spectroscopy, Instrumentation and Chemistry**, 3rd Pacific meeting, San Francisco, Calif. (J. G. Conway, Lawrence Radiation Laboratory, Univ. of California, Berkeley 4)

21-24. **Acoustical Soc. of America**, 68th, Austin, Tex. (W. Waterfall, ASA, 335 E. 45 St., New York, N.Y. 10017)

21-25. **Cybernetics**, 4th intern. congr., Namur, Belgium. (Intern. Assoc. for Cybernetics, 13 rue Basse-Marcelle, Namur)

22-23. **New Mexico Acad. of Science**, Albuquerque. (K. S. Bergstresser, 739 42 St., Los Alamos, N.M.)

23-24. **Kentucky Acad. of Science**, Morehead. (G. Levey, College Box 2325, Berea, Ky.)

23-24. **American Physical Soc.**, Chicago, Ill. (R. G. Sachs, Argonne National Laboratory, Argonne, Ill. 60440)

23-25. **Association of Clinical Scientists**, Washington, D.C. (R. P. MacFate, 300 N. State St., No. 5422, Chicago, Ill. 60610)

23-25. **Experimental Gerontology**, symp., Basel, Switzerland. (Prof. Verzar, Inst. de Gerontologie Experimentale, Nonnenweg 7, Basel, Switzerland)

24-29. **American Acad. of Pediatrics**,

Precision Temperature Control! JUMO

CONTACT THERMOMETERS

with ROTARY
SETTING MAGNET

- Instant temperature adjustment
- All operating parts sealed in
- No loose connections — no erratic contacts
- Temperature maintained to 0.01°C

This regulating and control thermometer, in a single unit, gives excellent service for lengthy periods at up to 3000 switching actions per hour. The upper portion comprises the temperature selector, the lower part the mercury reservoir and control thermometer with stem. A molded bakelite cap encloses the terminals and carries the rotary setting magnet, rotation of which moves the setting bar to the desired temperature setting. Regulation is effected by a contact wire attached to the setting bar and extending through a sliding contact into the control thermometer where it makes contact with the mercury as the latter rises in the capillary.

Catalog No. S-98770
150mm stem length
Catalog No. S98772
300mm stem length

RANGE	PRICE
0-50°C	\$28.00
0-100°C	\$28.00
0-150°C	\$30.00
0-200°C	\$31.00
0-250°C	\$33.00
0-300°C	\$35.00

Please specify stem length
and range when ordering
Special Ranges Available On
Order


For use with Jumo Thermom-
eters, we recommend our
#S98885 Electronic Relay \$75.00

**STANDARD SCIENTIFIC
SUPPLY CORP.**



808 Broadway, New York, N.Y. 10003
Glendale, Calif. 91201
So. San Francisco, Calif. 94080

Laboratory Apparatus • Reagents and Chemicals

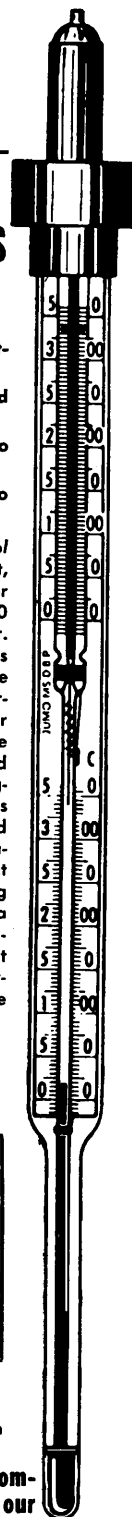

annual, New York, N.Y. (AAP, 1801 Hinman Ave., Evanston, Ill.)

25-31. American Soc. for **Horticultural Science**, Caribbean Region, 12th annual, Maracay, Venezuela. (E. H. Casseres, Londres 40, México 6, D.F.)

26-27. American Inst. of **Aeronautics and Astronautics**/Canadian Aeronautics and Space Inst., joint meeting, Ottawa, Ont., Canada. (P. J. Burr, AIAA, 1290 Sixth Ave., New York, N.Y. 10019)

26-27. **Combustion** Inst., western states section, fall meeting, Univ. of Utah, Salt Lake City. (Secretary, CI, 16902 Bollinger Dr., Pacific Palisades, Calif. 90272)

26-28. **Antimicrobial Agents and Chemotherapy**, 4th conf., American Soc. for Microbiology, New York, N.Y. (ASM, 115 Huron View Blvd., Ann Arbor, Mich.)

26-28. Chemical Inst. of Canada, 14th **Chemical Engineering** meeting, Hamilton, Ont. (CIC, 48 Rideau St., Ottawa 2)

26-28. Society of **Rheology**, 35th annual, Pittsburgh, Pa. (H. Markovitz, Mellon Inst., 4400 Fifth Ave., Pittsburgh 13)

26-14. Pan American **Standards** Committee, textiles seminar, Lima, Peru. (American Standards Assoc., 810 18th St., NW, Washington, D.C.)

27. Oak Ridge Inst. of **Nuclear Studies**, Oak Ridge, Tenn. (W. G. Pollard, Box 117, Oak Ridge)

27-29. **Joint Computer Conf.**, San Francisco, Calif. (R. I. Tanaka, c/o Lockheed Missiles and Space Co., 3251 Hanover St., Palo Alto, Calif.)

28-30. Society of **Experimental Stress Analysis**, annual, Cleveland, Ohio. (B. E. Rossi, 21 Bridge Square, Westport, Conn.)

28-30. **Inertial Guidance Test**, 2nd symp., Holloman Air Force Base, N.M. (F. P. Ray, Holloman AFB)

28-30. **Nuclear Science**, 11th symp., Philadelphia, Pa. (U.S. Office of Aerospace Research, 4th and Independence Ave., SW, Washington, D.C.)

28-30. **Rock Mechanics**, 6th symp., Rolla, Mo. (C. Christianson, Dept. of Mining Engineering, School of Mines and Metallurgy, Univ of Missouri, Rolla)

28-30. **Southeastern Library Assoc.**, 21st biennial conf., Norfolk, Va. (E. F. Jesse, c/o Armed Forces Staff College Library, Norfolk)

29-31. American Soc. for **Aesthetics**, Chicago, Ill. (J. R. Johnson, Cleveland Museum of Art, Cleveland 6, Ohio)

29-31. **Electron Devices**, Inst. of Electrical and Electronics Engineers, Washington, D.C. (M. Mass, Hewlett-Packard Co., 1501 Page Mill Rd., Palo Alto, Calif.)

29-31. **Gerontological Soc.**, 7th annual, Minneapolis, Minn. (GS, 660 South Euclid, St. Louis, Mo. 63110)

29-31. **Indiana Acad. of Science**, Indianapolis. (C. F. Dineen, Biology Dept., St. Mary's College, Notre Dame, Ind.)

29-31. Society of **Photographic Scientists and Engineers**, annual symp., Washington, D.C. (W. S. Dempsey, FMA, Inc., 4925 Fairmont Ave., Washington, D.C.)


29-31. Society for the **Scientific Study of Religion**, Washington, D.C. (S. Z. Klausner, SSSR, 1424 16th St., NW, Washington, D.C.)

30-1. **Meteoritical Soc.**, 27th meeting, Arizona State Univ., Tempe. (C. B. Moore, Dept. of Geochemistry, Arizona State Univ., Tempe)

11 SEPTEMBER 1964

DC-to-50 MC 10 MV / CM solid-state oscilloscope

for accurate,
reliable measurements...
even in difficult
environments

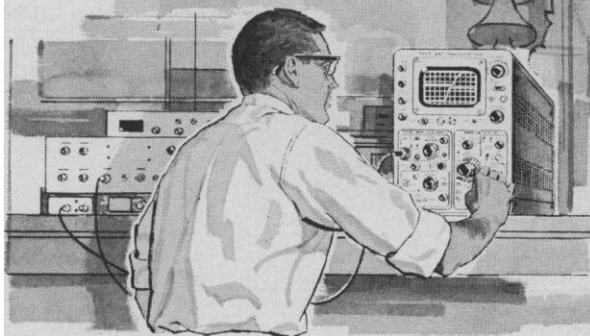

Type 647 Features with 10A2 and 11B2 Plug-In Units

■ Dual-trace operation. 10 mv/cm sensitivity. Dc-to->50 Mc passband. Less than 7-nsec risetime.

■ 6-cm by 10-cm display area. Internal, no-parallax graticule. Controllable graticule illumination. 14-kv accelerating potential.

■ 2 time bases, independent triggering. Sweep rates to 0.1 μ sec/cm. 10X sweep magnifier.

■ Sweep delay 50 sec to 1 μ sec. Single-sweep operation. Wideband (>50 Mc) triggering. External horizontal input.

■ Bright line automatic triggering. $\div 10$ external trigger attenuator, (on main time-base triggering). 'Ground' input positions on each vertical channel.

■ 1-kc voltage calibrator, (crystal controlled). Push-button trace finder. Dc-coupled Z-axis amplifier. Current-probe calibrator.

■ 100 v—130 v line voltage. No calibration changes with line fluctuations. 50-to-400 cps line frequency. Low power—185 watts, approximately. Convection cooled—no fan needed.

Type 647 Oscilloscope (without plug-ins) . . .	\$1225
Type 10A2 Dual-Trace Unit	\$675
Type 11B2 Time-Base Unit	\$825
2 P6008 Probes	\$ 70

U.S. Sales Prices f.o.b. Beaverton, Ore.

FOR MORE INFORMATION—OR TO ARRANGE A DEMONSTRATION—PLEASE CALL YOUR TEKTRONIX FIELD ENGINEER.

Tektronix, Inc.

P.O. BOX 500 • BEAVERTON, OREGON 97005 • Phone: (Area Code 503) Mitchell 4-0161 • Telex: 036-691
TWX: 503-291-6805 • Cable: TEKTRONIX • OVERSEAS DISTRIBUTORS IN 25 COUNTRIES
TEKTRONIX FIELD OFFICES in principal cities in United States. Consult Telephone Directory.
Tektronix Australia Pty., Ltd., Melbourne; Sydney • Tektronix Canada Ltd., Montreal; Toronto
Tektronix International A.G., Zug, Switzerland • Tektronix Ltd., Guernsey, C. I.
Tektronix U. K. Ltd., Harpenden, Herts



The Type 647 Oscilloscope and plug-in units add new convenience to display and measurement of high sensitivity, wide band, dual trace applications. Adaptable and versatile, the oscilloscope retains accuracy, within stated specifications, under extensive temperature variations . . . fluctuating line voltages . . . other difficult conditions.

TEMPERATURE

Non-Operating —55°C to +75°C. Operating —30°C to +65°C.

SHOCK

Non-Operating 20 G's max, 2 shocks, each direction, along each of 3 major axes.

HUMIDITY

Non-Operating meets Mil-Std-202B, Method 106A, except freezing, vibration, through 5 cycles (120 hours).

VIBRATION

Non-Operating or Operating. 0.025" pk-pk, 10-55-10 cycles, (4 G's max), 1 min cycles, 15 min each major axis.

ALTITUDE

Non-Operating 50,000 ft. Operating 15,000 ft. 50-to-400 cps line freq.