

the department of sociology at the University of California, Riverside, on 1 July.

Sheldon Wolff has become professor of cytogenetics and a research cytogeneticist at the University of California Medical Center, San Francisco. He had been on leave from Oak Ridge National Laboratory as visiting professor of radiation biology at the University of Tennessee.

Louis J. Battan, professor of meteorology and associate director of the Institute of Atmospheric Physics at the University of Arizona, has been elected president of the American Meteorological Society.

Whittie J. McCool, in the division of operational safety of the Atomic Energy Commission, has been appointed the AEC's scientific representative in Tokyo, succeeding **Peter A. Morris**, who has returned to the U.S. to become director of the division of operational safety.

Recent Deaths

William Parker Anslow, Jr., 53; professor and former chairman of the department of physiology at the University of Virginia medical school; 17 March.

Howard Coonley, 89; former director of the American Standards Association and first president of the International Organization for Standardization; 25 February.


Enrique E. Ecker, 79; professor emeritus of immunology at Western Reserve University; 5 March.

Franklin Hollander, 67; chief of the gastrointestinal physiology research laboratory at Mount Sinai Hospital, New York; 24 March.

Alfred N. Richards, 90; professor emeritus and former vice president of medical affairs at the University of Pennsylvania; president of the National Academy of Sciences, 1947-1950; 24 March.

Joel Stebbins, 87; director emeritus of the Washburn Observatory, University of Wisconsin; 16 March.


Erratum: In the report "Radiocarbon samples: chemical removal of plant contaminants" by C. V. Haynes, Jr. [151, 1391 (18 March 1966)], the word "no" was erroneously omitted from the first sentence of the fourth paragraph. The paragraph should have begun, "To test the method further, an artificial sample was prepared by mixing 8.18 g of charcoal that had no C^{14} activity. . . ."

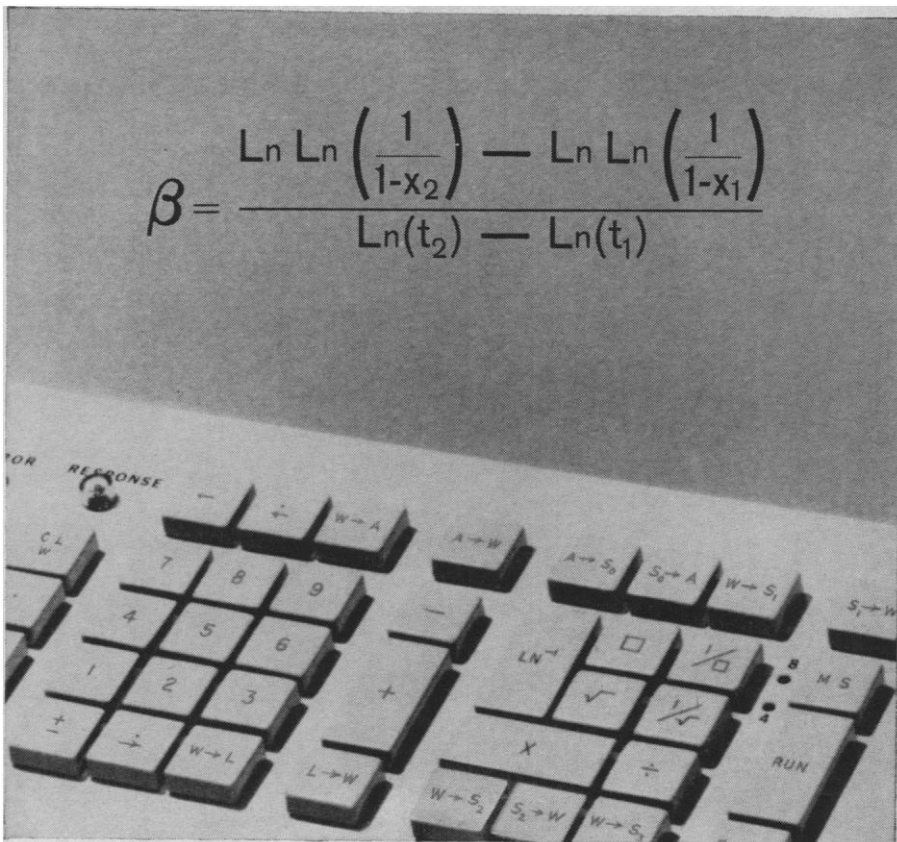

You can solve for β in seconds...with LOCI-2

LOCI-2, the most powerful desk-top computer ever devised, makes short work of expressions like this one for failure rate coefficient β . This new programmable instrument provides broad computer capabilities combined with the immediacy and simplicity of a slide rule. Designed specifically for the personal use of scientists and engineers, LOCI-2 owes its computational power to the fact that it utilizes an absolutely unique logarithmic approach to data manipulation which results in extraordinary versatility and simplicity of operation.

LOCI-2 is programmed by means of pre-scored tab cards (no keypunch needed). It is furnished with a total of 19 storage registers, which provide a program flexibility exceptional for a unit of desk-top size. In the manual mode it may be operated as an extended calculator, capable



To solve for β in the above expression:
(with appropriate program card in the LOCI-2 reader)
1. Enter value for x_1 (press "P₂" key)
2. Enter value for x_2 (press "Run" key)
3. Enter value for t_1 (press "Run" key)
4. Enter value for t_2 (press "Run" key)
The value of β is automatically displayed.

of performing addition, subtraction, multiplication, division, and exponentiation, as well as taking logarithms and extracting roots. In the automatic, programmed mode, it has a flexible and powerful repertoire of commands with which iterative procedures are easily and compactly coded.* There are also commands for making decisions and constructing program loops.

LOCI-2 is even used "on-line" as an extremely economical means of data acquisition and reduction

in many applications such as controlling process variables, reduction of nuclear scaler readings, etc.

LOCI-2 prices range from \$2570 to \$8450. If you would like to learn more about this remarkable instrument, write for complete descriptive literature.

*An extensive library of scientific and mathematical programs is furnished free of charge to LOCI-2 purchasers.

WANG
LABORATORIES, INC.

DEPT. D-4, 836 NORTH STREET, TEWKSBURY, MASS. 01876 - TEL: (617) 851-7311