




30 YEARS OF SCIENTIFIC ACHIEVEMENT

# OPTICAL INTERFERENCE FILTERS

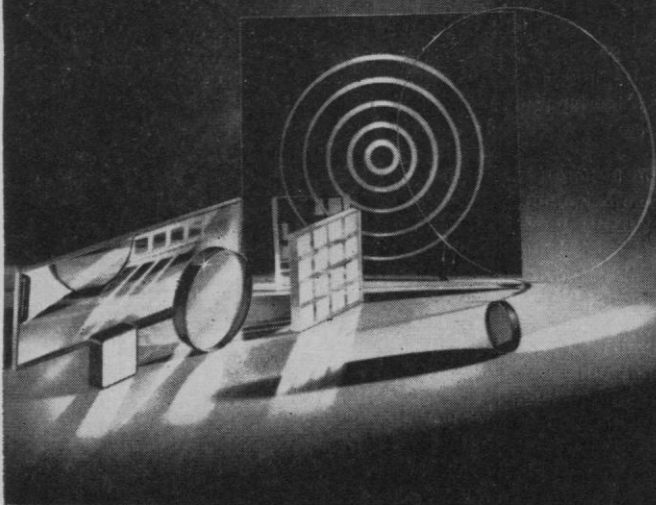

ULTRAVIOLET      VISIBLE      NEAR-INFRARED

One of the world's major suppliers of multilayer, all-dielectric, optical interference filters, Baird-Atomic offers the most efficient means of filtering in the *ultraviolet*, *visible*, and *near-infrared* regions of the spectrum!

Immediately available in a wide range of shapes and sizes, these *reasonably priced* Optical Interference Filters offer many advantages over absorption and other types of filters including:

- VERY HIGH TRANSMISSION
- NARROW BANDWIDTHS
- SHARP CUT-OFFS AND CUT-ONS
- SYMMETRICALLY SHAPED PASS-BANDS
- EXCELLENT BLOCKING
- LOW REJECTION

Filter applications include *space and military programs*, *interferometry*, *detection systems*, *navigational aids*, *flame photometry*, *colorimetry*, *laser applications*, *astronomy*, *color densitometry*, *microphotography*, *photomicrophotography*, *biology*, *psychology*, and *medical research*.

Delivery is either from stock or within 2 weeks after receipt of order. Accelerated delivery schedules can be arranged. Comprehensive literature is immediately available on request.

SCIENTISTS: Investigate challenging career opportunities at Baird-Atomic — an equal opportunity employer.

ELECTRONIC PRODUCTS AND COMPONENTS DIVISION



## BAIRD-ATOMIC

33 UNIVERSITY RD., CAMBRIDGE, MASS. 02138, Tel: 617 864-7420  
OFFICES: ATLANTA BOSTON CHICAGO DALLAS DETROIT LOS ANGELES  
NEW YORK PHILADELPHIA PITTSBURGH SAN FRANCISCO WASHINGTON, D.C.  
EUROPE: BAIRD-ATOMIC (EUROPE) N.V., 26-27 VEENKADE, THE HAGUE, HOLLAND



## PHYSIOLOGY BIOLOGY PB-3 SCOPE

OSCILLOSCOPE  
BIO-AMPLIFIER  
STIMULATOR

COMPACT • ECONOMICAL • VERSATILE

An oscilloscope, bio-amplifier, and stimulator in a single unit for teaching and research in the life sciences.



ECG



EMG



EEG



NERVE REACTION  
POTENTIAL



PLANT CELL  
POTENTIAL



MUSCLE FIBER  
POTENTIAL

### PB-3 SCOPE SPECIFICATIONS

#### VERTICAL AMPLIFIER

BAND WIDTH	SENSITIVITY	RISE TIME	IMPEDANCE ACCURACY	
D.C. to 50 KC	Oscilloscope 50 MV to 50V/CM  Bio-amplifier in 10 $\mu$ V/CM to 100 MV/CM	Less than 7 $\mu$ sec.	Oscilloscope 1 Meg— Single End  Bio-amplifier 20 Megs— Balanced 10 Megs— Single End	$\pm 5\%$

TIME BASE		CRT		STIMULATOR	PHYSICAL
SPEED	TRIG- GERING	DIA.	PHOSPHOR	Amplitude .04 to 100 volt frequency 1 to 1000 cps Duration .04 to 32 ms	DIM. & WT. 16"x18"x12" 45 lbs.
10 $\mu$ sec. CM to 1 sec/cm	Internal or External Slope, + or -	5"	P7 (Filters available)		

Catalog Number 7092—680

Price \$750.

For 115 Vac 50-60 cycles 90 watts

Other oscilloscope models available

For additional information—

write for Bulletin PB3-65

## PHIPPS & BIRD, INC.



Manufacturers & Distributors of Scientific Equipment

6th & Byrd Streets — Richmond, Virginia

*You get fast, reliable  
results with . . .*  
**LOW-COST  
MACALASTER<sup>®</sup>  
COENZOMETER**



Don't let the low-cost fool you! This highly reliable instrument offers laboratories speed and efficiency in measuring rates of enzyme reactions involving Coenzyme I.

**LDH Activities measured in 2 minutes.  
GOT activities, 5 minutes.**

Basically, the Coenzometer (developed in Biophysics Dept., Harvard Medical School) is a single wave length ultraviolet photometer. UV absorbence of sample is compared by a barrier photocell with the unabsorbed light registered on the second reference photocell. Water jacket, when used with the water bath, keeps cuvette temperature constant.

GOT and LDH activities may be efficiently measured with Worthington Determatubes<sup>®</sup> eliminating need for preparing reagents. Only water and serum required. For other applications standard 13 x 100 test tubes are used.

**Other applications which normally would require more expensive equipment!**

Urinary LDH, serum  $\alpha$ hydroxybutyric dehydrogenase, isocitric dehydrogenase, glutamic pyruvic transaminase, glucose-6-phosphate . . . any substance having absorption at 350 millimicrons.

Comes complete w/cooling bar without pump for operation on 115 V, 60 cycle AC; Manual; Pipettes, Graduated, 2.5 ml; 8 oz. Deeminac for deionized water; 100 ml Beaker, Warranty.

**ACCESSORY**

MSC 43100A Bath, Water, Constant Temp. . . \$95

Write for complete data.

**MACALASTER  
SCIENTIFIC  
CORPORATION**  
P.O. Box 363, Nashua, N.H. 03060

**INDEX TO ADVERTISERS—27 May 1966**

Ace Glass Inc. . . . .	1166	Nalge Co., Inc. . . . .	1179
Aldrich Chemical Co., Inc. . . . .	1295	National Appliance Co. . . . .	1156
American Edelstaal, Inc. . . . .	1303	Neslab Instruments, Inc. . . . .	1291
AMSCO Industrial Dynamics, Div. of American Sterilizer Co. . . . .	1309	New Brunswick Scientific Co., Inc. . . . .	1149
Baird-Atomic . . . . .	1313	Nikon Inc., Instrument Div. . . . .	1150
Beckman Instruments, Inc. . . . .	1135, 1155, 1178	Northern Scientific Inc. . . . .	1143
Bel-Art Products . . . . .	1298	Owens-Illinois . . . . .	1157
Brinkmann Instruments . . . . .	1171	Packard Instrument Co., Inc. . . . .	1190
Buchler Instruments, Inc. . . . .	1184	Paillard Inc. . . . .	1291
Chemical Rubber Co. . . . .	1185	Pharmacia Fine Chemicals Inc. . . . .	1298
Coleman Instruments Corp . . . . .	1302	Phipps & Bird, Inc. . . . .	1313
Corning Glass Works . . . . .	1168, 1290	Photovolt Corp. . . . .	1296
Custom Scientific Instruments, Inc. . . . .	1304	Polaroid Corp. . . . .	1142
Difco Laboratories . . . . .	1303	Professional Tape Co., Inc. . . . .	1296
Digital Equipment Corp. . . . .	1187	Quickfit Reeve Angel, Inc. . . . .	1164
Esterline Angus Instrument Co., Inc. . . . .	1137	Raytheon Co. . . . .	1311
Fabri-Tek Inc. . . . .	1147	Raytheon Co., Sorensen Opera- tion . . . . .	1145
Fisher Scientific Co. . . . .	1173	RCA Scientific Instruments . . . . .	1175
Flow Laboratories Inc . . . . .	1183	Sanborn Div., Hewlett-Packard Co. . . . .	1174
Gates, George W., & Co. . . . .	1316	Scientific Glass Apparatus Co., Inc. . . . .	1307
Gilford Instrument Laboratories Inc. . . . .	1158	Scientific Products . . . . .	1146
Gilson Medical Electronics . . . . .	1188	Sigmamotor, Inc. . . . .	1303
Hamner Electronics Co., Inc. . . . .	1292	Sprague-Dawley, Inc. . . . .	1316
Hewlett-Packard Co. . . . .	1176	Teachers Insurance and Annuity Assoc. . . . .	1310
Hewlett-Packard, F&M Scientific Div. . . . .	1317	Technicon Chromatography Corp. . . . .	1167
Histology Service, Inc. . . . .	1316	Thermolyne Corp. . . . .	1295
Institute for Scientific Informa- tion . . . . .	1312	Thomas, Arthur H., Co. . . . .	1318
Instrumentation Specialties Co., Inc. . . . .	1162	Thomas, Charles C, Publisher . . . . .	1170
International Equipment Co. . . . .	1152, 1186	Torsion Balance Co. . . . .	1159
Isotopes, Inc. . . . .	1172	Tracerlab . . . . .	1144
Keithley Instruments . . . . .	1301	TRG Control Data Corp. . . . .	1305
Kirschner Manufacturing Co. . . . .	1309	Ultra-Violet Products, Inc. . . . .	1294
Klett Manufacturing Co., Inc. . . . .	1293	Unitron Instrument Co. . . . .	1163
Lab Cages, Inc. . . . .	1151	University of Chicago Press . . . . .	1290
Lea & Febiger . . . . .	1294	U.S. Stoneware . . . . .	1184
Leeds & Northrup . . . . .	1180, 1181	Varian Associates, Recorder Div. . . . .	1297
LKB Instruments, Inc. . . . .	1148, 1161	Waring Products Co., Div. of Dynamics Corporation of America . . . . .	1160
Macalaster Scientific Corp. . . . .	1314	Warner-Chilcott Laboratories In- struments Div. . . . .	1140, 1141, 1169
Maryland Plastics, Inc. . . . .	1293	Whittaker Corp., Gencom Div. . . . .	1308
Materials Research Corp. . . . .	1293	Wild Heerbrugg Instruments, Inc. . . . .	1306
Mercer Glass Works Inc. . . . .	1297	Wilmot Castle Co. . . . .	1165, 1316
Metabolic Research Foundation . . . . .	1316	Worthington Biochemical Corp. . . . .	1291
Millipore Filter Corp. . . . .	1304	Yellow Springs Instrument Co. . . . .	1182

# PERSONNEL PLACEMENT

## POSITIONS WANTED

**Information Scientist.** Recent B.Sc. Pharmacy desires position in pharmaceutical field offering an opportunity to apply her scientific capabilities to mutual advantage. Excellent references. Box 113, SCIENCE. X

**Microbiologist, Ph.D.,** postdoctoral and medical school teaching experience in virology and immunology. Major interest in animal virology. Seeking academic or full-time research position. Available 1 August 1966. Box 114, SCIENCE. 6/1

**Ph.D. Biochemical Physio-Pharmacologist.** Age 35. Publications. Research-development experience in Britain, Europe, Asia, and United States. Languages. National international technico-economic coordination RD. Desires research management or liaison for international division pharmaceutical or allied industry. Box 115, SCIENCE. X

(a) **Physiology Ph.D. 1966;** ASCP, technology experience; cytology, histochemistry research; seeks clinical research or teaching position. (b) **Veterinary Ph.D. 1966;** genetics M.S.; statistics-computer programming; available for research opportunity. Write WOODWARD MEDICAL PERSONNEL BUREAU, 185 North Wabash, Chicago 60601. X

**Physiologist, Ph.D.,** 15 years of teaching-research experience. Ten publications. Desires teaching-research or teaching position in health professional schools or college located in small city. Box 116, SCIENCE. X

**Toxicologist DVM, M.S.,** pharmacology research and industrial experience. Box 117, SCIENCE. X

## POSITIONS OPEN

**Assistant Research Scientist.** Well-motivated, responsible person who can work with minimal direction to do immunology research in biochemistry. M.S. in Biochemistry preferred, or equivalent experience. Excellent benefits plus free tuition N.Y.U. Contact Personnel, N.Y.U. Medical Center, 568 First Ave., N.Y.C. 10016.

## BIOCHEMIST

To direct clinical laboratory with research orientation in voluntary psychiatric hospital. Experience or qualifications to conform with requirements of Laboratory Director required. Salary \$12,000. Apply Dr. Arnold G. Blumberg, Director Medical Services, Hillside Hospital, P.O. Box 38, Glen Oaks, New York 11004.

## BROCK UNIVERSITY Department of Biosciences

Applications are invited, from persons with experience in establishing and maintaining stores in Biology or Chemistry, for the position of Senior Storekeeper in this new Department. Duties commence July 1966. Apply, stating experience and giving the names of two referees to the Head, Department of Biosciences, Brock University, St. Catharines, Ontario, Canada.

## ENZYMOLOGIST-Ph.D.

Expansion of the Biosynthesis Department has created a new position. We seek a Ph.D. Biochemist with significant experience in enzymology and with demonstrated supervisory ability. Must be able to establish a program involving the biosynthesis of radioactive labeled compounds. Experience with labeled compounds is desirable, but not essential.

Send confidential resume & salary requirements to Alan R. Aronson, Personnel Mgr.

## NEW ENGLAND NUCLEAR CORP.

575 Albany Street  
Boston, Mass. 02118  
An equal  
opportunity employer



## POSITIONS OPEN

### ANIMAL BEHAVIORIST PSYCHOLOGIST

Challenging opportunity for a Ph.D. or M.S. with strong interest in behavioral science.

Research project involves working with other scientists in defining the neurophysiological, pharmacological, and behavioral effects of air pollutants.

Excellent opportunities for advancement. Civil Service requirements apply. Liberal benefits including life insurance, health insurance and sick leave, vacation and retirement plans. Major costs of travel as well as transportation of household goods and personal effects to Cincinnati, Ohio, area will be paid by employer. U.S. citizenship required. Send resume (transcripts and list of publications desirable) or application (Standard Form 57), available from any post office to:

CHIEF, LABORATORY OF MEDICAL AND  
BIOLOGICAL SCIENCES

ROBERT A. TAFT SANITARY ENGINEER-  
ING SERVICE

4676 COLUMBIA PARKWAY

CINCINNATI, OHIO 45226

An equal opportunity employer

## POSITIONS OPEN

MASSEY UNIVERSITY OF MANAWATU  
PALMERSTON NORTH, NEW ZEALAND

LECTURER OR SENIOR LECTURER IN  
PHYSIOLOGY

Applications are invited from suitably qualified graduates in Science, Medicine or Veterinary Science for this post. Research experience would be desirable but is not essential. Physiology is taught in this University for Science, Agricultural Science and Veterinary Science degree courses. The research interests of the present staff are mainly centered on gastrointestinal physiology, but facilities are available for research in other fields of physiology. Further details of the post, departmental activities and facilities may be obtained from Professor D. A. Titchen, to whom preliminary inquiries may be addressed.

Salary: Senior Lecturer £2,100 — £2,500 p.a. (x £100)  
Lecturer £1,300 — £2,000 p.a. (x £100)

Further details, and conditions of appointment may be obtained from the Association of Commonwealth Universities (Branch Office), Marlborough House, Pall Mall, London, S.W.1., or the Registrar of the University.

Applications close in New Zealand and London on 30 June, 1966.

## DIRECTOR FOOD SCIENCE

Position on the staff of our Department of Foods and Nutrition for person to direct Food Science Program. Areas of concern include new developments in food technology and residue contamination of foods, including radioactivity. Will act as Liaison with the Food and Drug Administration, U.S. Department of Agriculture and other technical associations. Ph.D. in Food Science or related field with knowledge of nutrition, food processing and composition. Please send resume to: Personnel Department, American Medical Association, 535 North Dearborn, Chicago, Illinois 60610.

# LITERATURE SCIENTISTS

Due to expansion and the resultant increase in activity the Science Information Services Department of the Warner-Lambert Research Institute now has several opportunities for people interested in literature science.

We would prefer candidates with an advanced degree in either chemistry or the biological sciences. Experience in industrial research and/or information retrieval would be very desirable but is not an absolute requirement. Primary position responsibilities will include the abstracting and indexing of biological, biomedical, and chemical literature; literature searches and the development and operation of various indexing and retrieval systems.

The Research Institute is located within easy traveling distance of New York and Philadelphia in an attractive suburban location.

Relocation expenses will be paid.

To apply please send resume including salary requirements to Mr. R. L. Bowlby.

## WARNER LAMBERT RESEARCH INSTITUTE

Tabor Road, Morris Plains, N. J.

An Equal Opportunity Employer

## POSITIONS OPEN

(a) **Ph.D. Biochemist**, viral oncology research; to \$15,000; southeastern university. (b) **B.S. Parasitology**, experienced; Central hospital; \$7200. (c) **B.S./M.S. Microbiologist**, public health; West; to \$10,500. *Faculty Appointments:* (d) **Cytology/Histology**; eastern college; to \$9000. (e) **Ph.D. Bacteriology-Biology**; Southeast university. (f) **Ph.D. Chemistry**, physical chemistry background; Midwest university; to \$14,000. (g) **Anatomy-Physiology**, Northeast community college; to \$8000. Write **SCIENCE SERVICE, The Medical Bureau, 900 N. Michigan Avenue, Chicago, Illinois 60611.** X

### PHYSIOLOGIST — REPRODUCTION

Major ethical pharmaceutical company has immediate opening for a Ph.D. biologist, 0-5 years postdoctoral experience, with formal training in reproductive physiology. A background in biochemistry, radioisotopes and surgical procedures is desirable. Must be capable of conducting independent research and originating new ideas.

Pathological, clinical, chemical, and ancillary support available. Please send complete resume to

Box 118, SCIENCE

An equal opportunity employer

### RESEARCH ASSOCIATE

Position on the staff of our Department of Drugs for man or woman with reading ability in the Romance languages and training or experience in Biology or Pharmacy. Duties include indexing of Biomedical articles published in foreign periodicals. Excellent opportunity for professional growth, complete benefit program. Please send resume stating salary requirement.

### AMERICAN MEDICAL ASSOCIATION

535 North Dearborn  
Chicago, Ill. 60610

**SCIENCE DEPARTMENT, STATE UNIVERSITY COLLEGE AT BUFFALO**, seeks a generalist in physical science and science education beginning September 1966; 12-hour teaching load in foundation course to start; rank to associate professor; salary to \$10,000 for ten months Ph.D. required. Write: **T. E. Eckert, Chairman; 1300 Elmwood Ave., Buffalo, N.Y. 14222.**

### COMMONWEALTH AGRICULTURAL BUREAU INFORMATION SCIENTISTS AND TAXONOMISTS

Interesting and rewarding careers occur from time to time in the Commonwealth Agricultural Bureaux for graduates in biology or agriculture with a flair for writing and languages or for taxonomy.

The Bureaux, which are supported by the Governments of the Commonwealth, are located in the United Kingdom, usually in close association with a major research institute in the field concerned. They provide a comprehensive world information service for research workers in the agricultural sciences, including entomology, mycology, plant pathology, animal breeding and genetics, veterinary science, animal nutrition, dairy science and technology, forestry, helminthology, horticulture and plantation crops, pastures and field crops, plant breeding and genetics, soils and fertilizers, weed control and agricultural economics.

Abstracting of the world's literature in these fields is carried out by Scientific Information Officers with salaries in a scale rising to £2,431.

Taxonomists are employed in the identification services of the Commonwealth Institute of Entomology, the Commonwealth Mycological Institute and the Commonwealth Bureau of Helminthology, all of which are located in the London area. For these positions the basic requirement is a good degree in biology, together with experience in identifying insects, fungi or helminths. Salaries for taxonomists are in a scale rising to £3,107 per annum.

For further information and particulars of current vacancies apply to the Secretary, Commonwealth Agricultural Bureaux, Farnham House, Farnham Royal, Bucks., England.

## POSITIONS OPEN

**DIRECTOR HEALTH EDUCATION**—Responsible for guiding and directing long established nationwide program in health education. Reports directly to President and Board of Directors. Serves as official liaison between National Dairy Council and national leaders and groups in the fields of health and nutrition education. Provides leadership in program direction and coordination of four departments within the Health Education Division. Interprets developments and trends in health education to the national and local professional staff and to the dairy industry. Excellent opportunity for professional growth and development at the national level. Prefer experienced Ph.D. or Ed.D. Masters degree with qualifications a minimum requirement. Preference will be given to person with demonstrated ability in implementing action programs in health education incorporating nutrition. Starting salary commensurate with training and experience. Liberal fringe and retirement benefits. Write: **Milton Hult, President, National Dairy Council, 111 North Canal Street, Chicago, Illinois 60606.**

### MASSEY UNIVERSITY OF MANAWATU PALMERSTON NORTH, NEW ZEALAND

#### SENIOR LECTURER OR LECTURER IN CLINICAL PATHOLOGY

Applications from suitably qualified persons are invited for the above-mentioned position in the Department of Animal Health. Applicants must have a degree in Veterinary Science or Science with experience in Clinical Pathology and Interest in Chemical Pathology and/or Haematology and an interest in the application of Clinical Biochemical methods to Veterinary Clinical diagnosis. The successful applicant would be responsible for undergraduate teaching; for developing research in this field and for the organisation of Clinical Pathology services to the Veterinary Clinics. It is also envisaged that the application of Clinical Biochemical methods in veterinary medicine would be developed.

The Department includes Veterinary Pathology, Microbiology and Parasitology and is responsible for teaching these subjects in the Veterinary faculty.

Salary: Lecturer £1,300 — £2,000 p.a. (x £100)  
Senior Lecturer £2,100 — £2,500 p.a. (x £100)

Further details of the position and of the University may be obtained from the Association of Commonwealth Universities (Branch Office), Marlborough House, Pall Mall, London, S.W.1., or from the Registrar of the University.

Applications close in New Zealand and London on 31 July, 1966.

### Predoctoral Assistantships and Traineeships in Physiology

Excellent opportunities for graduate students leading to the Ph.D. Ample stipends and free tuition. Training and research in endocrinology, gastrointestinal, water and electrolyte metabolism, cardiovascular, sensory physiology, biophysics and bioengineering. Write for details to:

**Head, Department of Physiology  
University of Illinois at the Medical Center  
P. O. Box 6998  
Chicago, Illinois 60680**

**X-Ray Diffraction Technician**—B.S. Past experience with x-ray camera work essential (single crystal and powder patterns). Starting salary \$6300; rising to \$6675 after one year. Research connected with photographic and counter recording of diffraction patterns obtained from biological materials. Equal Opportunity Employer. Contact Russell P. Ketcham, Personnel Director, Roswell Park Memorial Institute, Buffalo, New York 14203.

## PHARMACEUTICAL CHEMISTS

Progressive Western New York pharmaceutical manufacturer has openings in Product Technology Laboratory, Quality Control Laboratory, and Scientific Research Group. B.S. degree minimum requirement, experience in pharmaceutical product development or research desirable. Salary to \$15,000 per year.

Submit complete summary indicating educational and professional background, including present and expected salary to Mr. Jay R. Schuster, c/o

### STRASENBURGH PHARMACEUTICALS

Division of Wallace & Tiernan Inc.

P.O. Box 1710, Rochester, N.Y., 14603

An Equal Opportunity Employer

# The Market Place

BOOKS • SERVICES • SUPPLIES • EQUIPMENT

## SUPPLIES AND EQUIPMENT

### SPRAGUE-DAWLEY, INC.

Pioneers in the development of the  
STANDARD LABORATORY RAT.

P.O. Box 4220

Madison, Wisconsin

CE 3-5318

## SPECIAL LIGHT SOURCES

- Mercury Point Sources
- Raymaster Blacklight (long and short wave ultraviolet)
- Sodium Vapor
- Mercury Vapor
- Zirconium, Xenon, Deuterium and Hydrogen Arc Lamps
- Imported Spectral Lamps
- Photochemical or High Intensity "Uviarcs"
- Auxiliary Operating Equipment for above

WRITE FOR FREE CATALOG OR CONTACT YOUR LABORATORY SUPPLY DEALER



**GATES**  
GEORGE W. GATES & CO.  
LUCILLE AVE. FRANKLIN SQUARE, L.I., N.Y.

Circle 89 on Readers' Service Card

## PROFESSIONAL SERVICES

### CONTRACT STERILIZATION AVAILABLE.

**Wilmot Castle Company** offers a wide variety of methods and equipment for sterilizing and certified sterility testing on production line basis. Many years experience with a wide range of products. Our R & D facilities are staffed with skilled researchers specializing in sterilization and ready to undertake solution of your sterilization problems. Call, write or wire, Research Lab, Wilmot Castle Company, Rochester, New York.

## HISTOLOGY SERVICE

**RAPID SERVICE Large Orders Quickly Processed! Quickly Shipped! Professional supervision of every order. Free estimates on special problems. Distant points serviced swiftly. Special stains and techniques available. Fully protected shipments. HISTOLOGY SERVICE, INC. 4801 N. Broad St., Philadelphia, Pa. Zipcode 19141, (215) Davenport 4-5800**

### Complete Bio-Analytical Services


Automated Wet Chemistry,  
UV, GLC, Clinical,

Hormones, Drugs, Lipids

**Metabolic Research Foundation**  
2201 W. Holcombe Boulevard  
Houston, Texas 77025  
MRF Phone: 713-664-4932

Circle 90 on Readers' Service Card

## SERIES 5750 RESEARCH GAS CHROMATOGRAPH

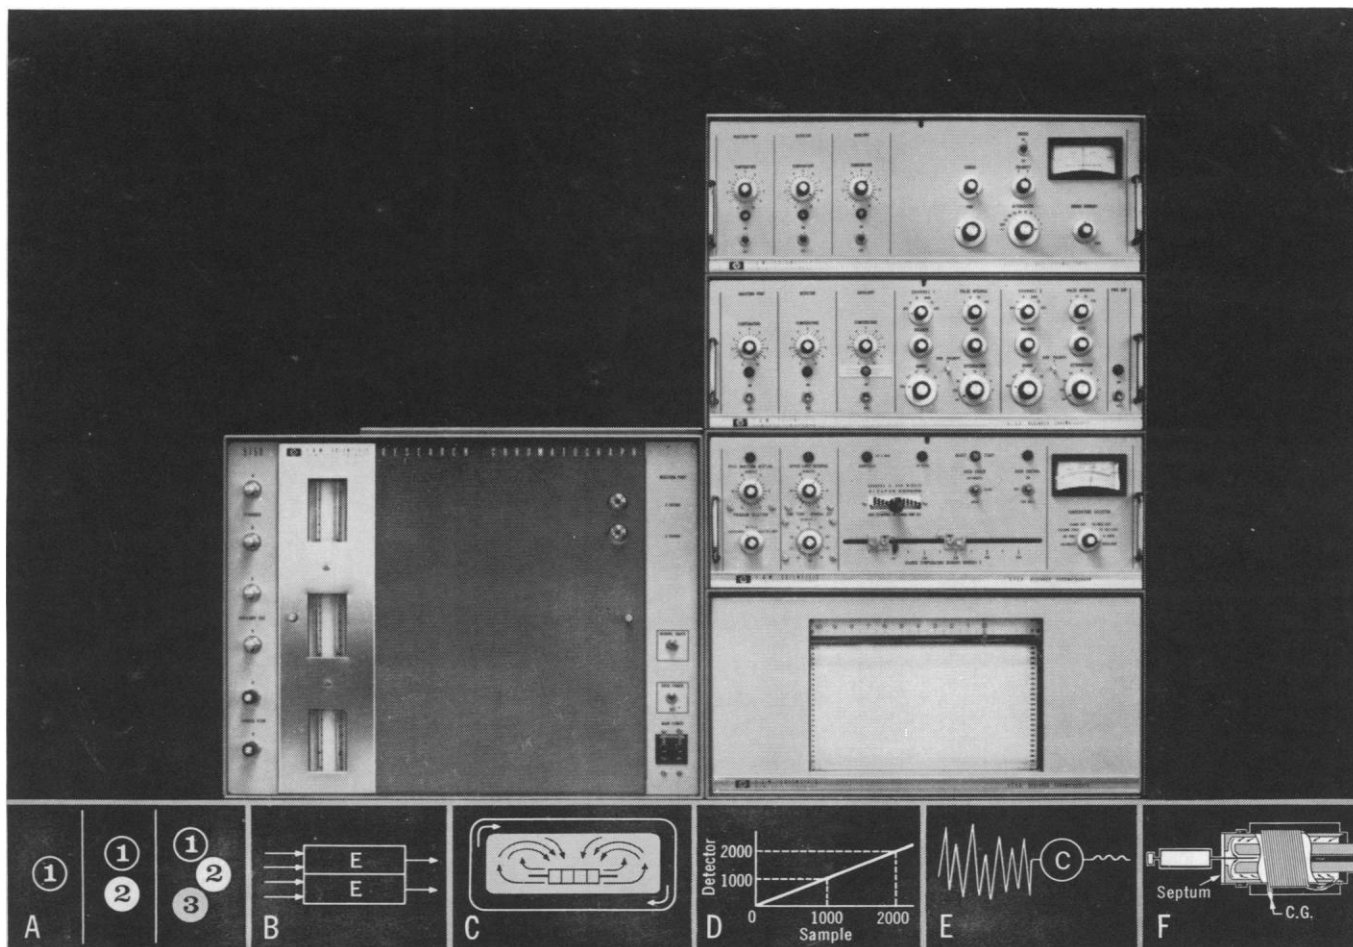

# ALL THE IMPROVEMENTS ARE IN PERFORMANCE

Now, only two years after we first released the Series 810 Research Gas Chromatograph, we're introducing its successor, the Series 5750 Research GC, a second-generation instrument that incorporates many important performance improvements. Six of these, illustrated symbolically above, are especially noteworthy.

### A—THREE DETECTOR POSITIONS—

The Series 5750 permits the simultaneous installation of any three detectors, from a choice of flame ionization, thermal conductivity, electron capture and micro cross-section . . . each equipped with separate and independent temperature controls.

### B—DUAL-CHANNEL ELECTROMETER—

Now available with either a single-channel or the new dual-channel electrometer, the 5750 offers the analyst a compact package suited exactly to his need and budget. Since *each* channel has dual input capability, the dual channel electrometer can be used for simultaneous operation of two detectors and still permit dual column compensation.

**C—FAST RESPONSE, EXCELLENT OVEN TEMPERATURE UNIFORMITY—** Redesigning from top to bottom, the 5750 oven possesses the best combination of

response and temperature uniformity of any commercially available gc: it heats between 50 and 400°C in ten minutes, cools from 400 to 50°C in 8 minutes . . . with a gradient of less than  $\pm 0.5\%$  in isothermal and  $\pm 1\%$  during programmed operation (measured in air).

### D—HIGH-LINEARITY FLAME DETECTOR

The linear dynamic range of the new dual flame detector is tenfold better than the best previously reported (linear up to 2 ml of propane giving peak width at base of 7 seconds, peak current of  $2 \times 10^{-5}$  amp, equivalent to  $3.7 \times 10^{-4}$  grams C/sec.)

### E—IMPROVED FLOW CONTROL—

A newly designed flow controller in Series 5750 gas chromatographs maintains flow rates at preselected levels with a precision about five times better than that obtainable with presently available commercial flow controllers.

### F—ADVANCED INJECTION PORT DESIGN—

Retaining all the versatility of the previous design, the 5750's new injection port permits true on-column injection, eliminates dead volume, minimizes thermal gradients, opposes backflash, and provides for the use of inserts. The result is strikingly effective: sol-

vent and sample peak width is clearly reduced and there is an increase in apparent column efficiency.

Based on these and other functional advances in instrument technology, the 5750 is still the most useful gas chromatograph around, capable of better qualitative and quantitative precision than any other gc, regardless of price. Model 5751A with dual flame detector single-channel electrometer and recorder is priced at \$4400 (f.o.b. Avondale, Pa.).

For more information, call the Chemical Instrumentation Sales Representative at one of the 41 Hewlett-Packard sales offices in the U.S.

F & M Scientific, Division of Hewlett-Packard, Route 41 and Starr Road, Avondale, Pennsylvania 19311. In Europe: F & M Scientific Europa N.V., Basisweg (Sloterdijk), Amsterdam, The Netherlands.




**F & M SCIENTIFIC**  
DIVISION OF HEWLETT-PACKARD



# Thomas Red Label MICRO COVER GLASSES

Very flat, with precision  
controlled thickness

Remarkably free from brittleness

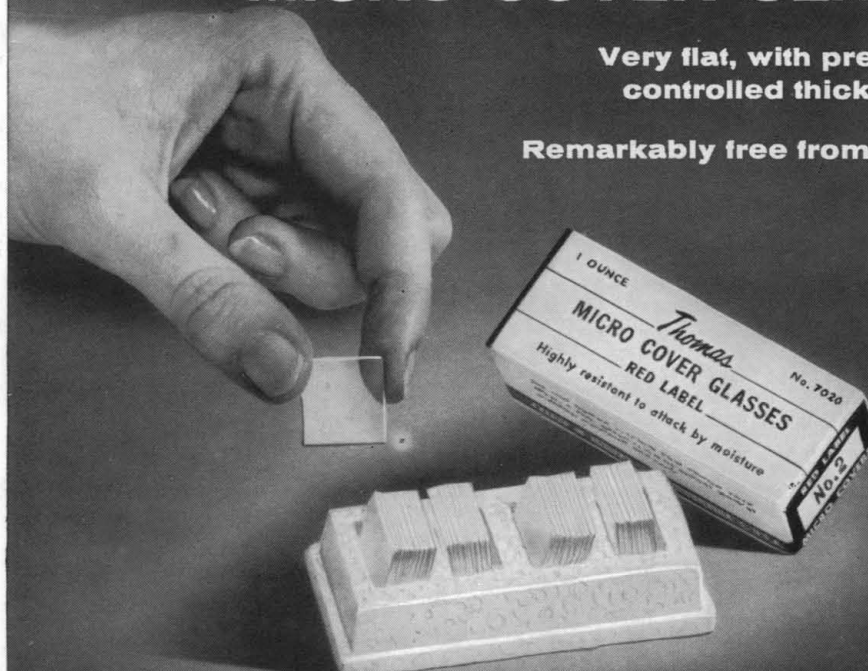

colorless optical glass • corrosion resistant • lead free

Cut from Chance colorless micro sheet of the highest resistance to attack by moisture, remarkably free from brittleness and very flat. Because of production in *mechanically drawn flat strips*, precision controlled thickness is obtained. Covers meet all requirements of U. S. Federal Specification DD-G-426a. They are free from lead oxide and therefore suitable for tissue culture work.

The relative absence of brittleness, which has

always been one of the outstanding physical characteristics of Chance micro sheet, greatly reduces breakage in handling and cleaning, particularly of large rectangles.

Sizes most widely used are now packed in a 1 oz. box of polystyrene foam with lift-off cover. Covers can be withdrawn singly without touching the surface. Remaining sizes are packed in small cardboard boxes.

	Per ounce	Per oz. in 6 oz. carton*	Per oz. 72 oz.** assortments	Per oz. 144 oz.** assortments
7020. SQUARES, No. 1, 18, 22 and 25 mm square.....	2.45	2.21	1.96	1.84
Ditto, No. 2.....	2.10	1.89	1.68	1.58
7022. CIRCLES, No. 1, 18, 22 and 25 mm diameter.....	4.35	3.92	3.48	3.26
Ditto, No. 2.....	3.70	3.33	2.96	2.78
7024. RECTANGLES, No. 1, 22 × 30 mm up to and incl. 48 × 60 mm.....	2.45	2.21	1.96	1.84
Ditto, No. 2.....	2.10	1.89	1.68	1.58

\*One size, shape and thickness only

\*\*Assorted sizes, shapes and thicknesses

For additional sizes and thicknesses, see  
our current general catalog



**ARTHUR H. THOMAS COMPANY**

*Scientific Apparatus and Reagents*

VINE STREET AT 3RD • P. O. BOX 779 • PHILADELPHIA 5, PA., U. S. A.