

The final session, on mechanisms, commenced with a review of the molecular events which might be altered by radiation. This was followed by a consideration of the role of the hormonal environment on the radiosensitivity of oocytes and by several papers suggesting alterations of enzymes and of proteins as possible mechanisms for the differential radiosensitivity of the immature organism. The symposium ended with a discussion of the relative importance of radiation damage to inductor and competent tissues in the response of the embryo.

An increasing tendency toward quantitative experimentation and the impact of modern concepts in biology on the study of radiobiologic phenomena was particularly notable. It was evident that there is continuing effort to understand the mechanisms and processes of normal development underlying the many experiments with radiation and radioactive material.

The symposium was held in Richland, Washington, 5 to 8 May, under the sponsorship of the Battelle Memorial Institute Pacific Northwest Laboratories and the U.S. Atomic Energy Commission. Approximately 150 scientists, representing 11 countries, participated in the meeting. Approximately 65 papers were selected from those submitted, to provide a coherent development of the field. The texts and related discussion are available as the *Symposium Proceedings*, from the Clearing House for Federal Science and Technological Information (National Bureau of Standards, Springfield, Va. 22151).

MELVIN R. SIKOV

Biology Department, Battelle Northwest, Richland, Washington 99352

Forthcoming Events

April

16-18. Carnahan Conf. on **Electronic Crime Countermeasures**, 4th annual, Lexington, Ky. (J. S. Jackson, Electrical Engineering Dept., Univ. of Kentucky, Lexington 40506)


20-23. Southwestern **Surgical Congr.**, Dallas, Tex. (J. A. Barney, 301 Pasteur Medical Bldg., Oklahoma City, Okla. 73103)

20-24. American **Geophysical Union**, Washington, D.C. (W. E. Smith, AGU, 2100 Pennsylvania Ave., NW, Washington, D.C. 20037)

21-23. **Aerospace Nuclear Applications**, Huntsville, Ala. (A. D. Smith, American

Circle No. 36 on Readers' Service Card →

BAUSCH & LOMB 
SCIENTIFIC INSTRUMENT DIVISION

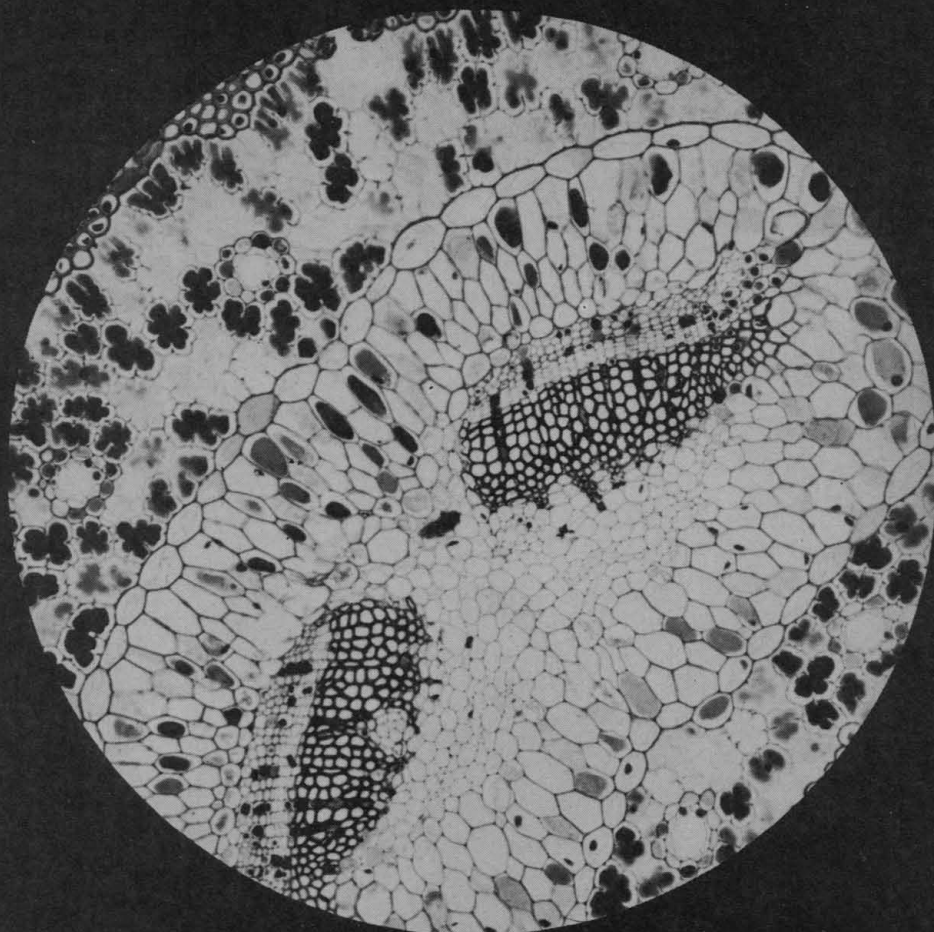

Bausch & Lomb Full Image Flat Field Teaching Microscopes Expedite Understanding



Students in general biology, zoology, botany, bacteriology need Bausch & Lomb full performance educational microscopes. Don't give them instruments that show only a third of the field in focus. Give them Bausch & Lomb full image flat fields that show them the whole area sharp and clear from edge to edge. This kind of optical performance teamed up with the mechanical excellence so typical of Bausch & Lomb speeds understanding, improving retention.

Get the full facts in our Educational Microscope Catalog, 20827, along with our free demonstration offer. Write today.

Bausch & Lomb, 20827 Bausch Street, Rochester, N.Y. 14602

Nuclear Soc., 10102 Redland St., Huntsville 35802)

21-23. Conference on **Stress Corrosion Cracking**, Los Angeles, Calif. (J. A. Fellows, American Soc. for Metals, Metals Park, Ohio 44073)

22-25. American Assoc. for **Child Care in the Hospital**, San Francisco, Calif. (H. H. Glaser, Stanford Children's Convalescent Hospital, Palo Alto, Calif. 94304)

23-25. **Illinois State Acad. of Science**, Chicago, Ill. (K. Harmet, Dept. of Biology, Northern Illinois Univ., De Kalb)

23-26. Association of **Clinical Scientists**, Detroit, Mich. (R. P. MacFate, ACS, 125 N. Rutledge St., Pentwater, Mich. 49449)

24-25. **Mississippi Acad. of Sciences**, Clinton. (C. Q. Sheely, Drawer CQ, State College, Miss. 39762)

24-25. **Nebraska Acad. of Science**, Lincoln. (C. B. Schultz, Univ. of Nebraska, Lincoln 68508)

24-25. **South Carolina Acad. of Science**, Columbia. (L. H. Stevenson, Biology Dept., Univ. of South Carolina, Columbia 29208)

25-30. American Ceramic Soc., Inc., 72nd annual mtg., Philadelphia, Pa. (The Society, 4055 N. High St., Columbus, Ohio 43214)

26-30. **Group Medicine**, 1st intern. congr., Winnipeg, Canada. (R. E. Beamish, Manitoba Clinic, 790 Sherbrook St., Winnipeg 2, Man., Canada)

26-1. American Soc. for **Microbiology**, Boston, Mass. (R. W. Sarber, 1913 I St., NW, Washington, D.C. 20006)

27-29. **Frequency Control Symp.**, 24th annual, Atlantic City, N.J. (J. M. Stanley, Electronics Components Lab., Fort Monmouth, N.J. 07703)

27-29. American **Surgical Assoc.**, White Sulphur Springs, W. Va. (C. G. Shires, 5323 Harry Hines Blvd., Dallas, Tex. 75235)

27-30. **National Telemetry Conf.**, Los Angeles, Calif. (A. V. Balakrishnan, Dept. of Engineering, Univ. of California, Los Angeles 90024)

27-2. American Acad. of **Neurology**, Miami Beach, Fla. (S. A. Nelson, Executive Director, The Academy, 4005 W. 65 St., Minneapolis, Minn. 55435)

28-30. **Blood Coagulation and Hemostasis**, Sherbrooke, P.Q., Canada. (R. Losito, Dept. of Medicine, Univ. of Sherbrooke, Sherbrooke)

28-30. Conference on the **Fatigue Problem**, Los Angeles, Calif. (J. A. Fellows, American Soc. for Metals, Metals Park, Ohio 44073)

28-30. **Pi Gamma Mu**, Denver, Colo. (E. B. Urquhart, 1719 Ames St., Winfield, Kan. 67156)

29-1. **Instrument Soc. of America**, 2nd education symp., Montreal, Canada. (C. M. Skillern, The Foxboro Co., Foxboro, Mass.)

30-1. **Kansas Acad. of Science**, Wichita. (R. J. Robel, Div. of Biology, Kansas State Univ., Manhattan 66502)

May

1. **Missouri Acad. of Science**, Warrensburg. (E. A. McGinnes, Jr., 1-31 Agriculture, Univ. of Missouri, Columbia 65201)

1-2. **North Dakota Acad. of Science**,


NOW...uniformly coat TLC plates regardless of plate thickness

Read how both models of Shandon Unoplan® Levellers coat even layers with certainty on every TLC plate. Or better, send for complete catalog on Thin Layer Chromatography and Thin Layer Electrophoresis to Shandon Scientific Company, Inc., 515 Broad Street, Sewickley, Pa. 15143 (Pittsburgh District).



Unoplan Model P brings plates into plane against guide rail lips by a few pumps of rubber bulb. After coating, air pressure is released and plates slide out end with thin, uncoated margin on each side for handling ease. \$150.

Unoplan Semi-Automatic Model SA has platform covered with aluminum sheet, and plates rest on two rubber strips. Swinging the lever closes hinged side and raises platform against lips of guide rails. Reversing the lever drops down hinged side allowing plates to be lifted out easily without damaging layers. \$230.

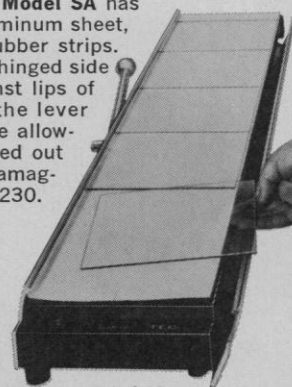


TLC Adjustable Spreader fits guide rails of either model. \$48.

SHANDON

PITTSBURGH • LONDON • FRANKFURT

Circle No. 82 on Readers' Service Card

Cabinet of a thousand faces.

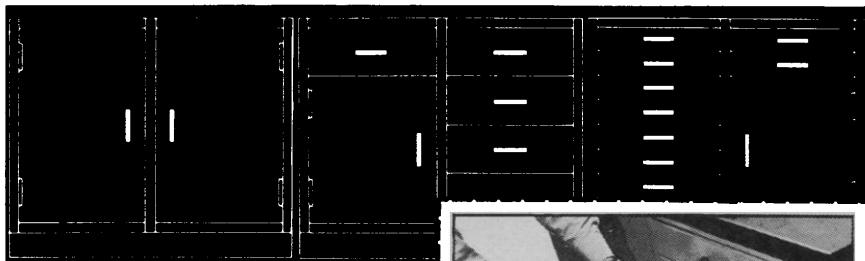

Switch doors to drawers, to shelves ... in the twist of a screwdriver

Blickman's patented Conflex laboratory furniture adapts to changing lab needs in minutes. Without special tools. Nearly 1,000 door and drawer combinations.

Mix and match doors and drawers ... turn 3 1/2"-deep drawers into 7 1/4"-deep drawers ... adjust shelves in 1/2" increments.

Specify Conflex furniture ... the laboratory furniture that changes with the times!

Send the coupon for complete details and specs.



BLICKMAN

WEEHAWKEN, NEW JERSEY

S. Blickman, Inc.
6903 Gregory Avenue
Weehawken, N.J.
07087

- ☐ Rush free Conflex Laboratory Furniture catalog
- ☐ Have a lab specialist phone us


Name/Title _____

Institution _____

Address _____

City/State/Zip _____

**Ultra-sensitive
UV detector
has 10,000
to 1 range**

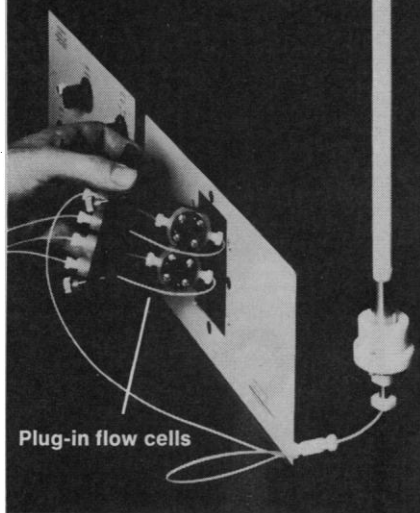

This new UV flow photometer has the high sensitivity required for chromatographic trace analysis along with the broad range and flow capacity needed for preparative work. □ Chromatronix Model 200 combines a linear absorbance range from .0001 to 3.0 O.D. with very low noise and drift—less than .0004 O.D. Low drift is insured by a unique multiplexed double-beam system, which uses a single vacuum diode detector to eliminate differential temperature drift. □ Measurements can be made on any of ten absorbance ranges (from .01 O.D. full scale to 5.12 O.D. full scale) or on a single 0 to 100% transmittance scale. Recorder outputs of 1 mv and 10 mv are supplemented by a 0 to 1 ma output, which will drive low-cost galvanometric recorders. □ Two interchangeable plug-in flow cells are available: an 8- μ l cell for micro-column analyses and a 32- μ l cell for monitoring preparative separations, density-gradient centrifugation and electrophoresis. The optical chamber is sealed and can be purged with dry gas to prevent condensation in cold rooms. □ Chromatronix also offers a new ultra-sensitive, wide range conductivity monitor for chromatography. Inquiry will bring you literature on it as well.



CHROMATRONIX

Chromatronix, Inc., 2743 Ninth St.
Berkeley, Calif. 94710. Phone (415) 841-7221.

Circle No. 87 on Readers' Service Card

Grand Forks. (B. G. Gustafson, Secretary-Treasurer, Univ. of North Dakota, Grand Forks 58201)

1-2. Society for Pediatric Research, Atlantic City, N.J. (R. E. Greenberg, Dept. of Pediatrics, Stanford Univ., Stanford, Calif. 94305)

2-3. American Federation of Clinical Research, Atlantic City, N.J. (J. E. Brown, 2011 Eye St., NW, Washington, D.C. 20006)

3-6. European Federation of Chemical Engineering, 93rd, Vienna, Austria. (W. F. De Geest, Lijzenstraat 24 Berchem-Antwerp, Belgium)

3-6. Society of Professional Well Log Analysts, symp., 11th annual, Los Angeles, Calif. (J. D. Clark, 13507 Tosca, Houston, Tex. 77024)

3-8. International Radiation Protection Assoc., 2nd, Brighton, England. (B. Godbold, Central Electricity Generating Board, 20 Newgate St., London, E.C.1, England)

4-5. Industrial Electronics and Control Instrumentation Transducer Conf., 2nd annual, Gaithersburg, Md. (R. B. Spooner, IMPAC Instrument Service, 201 E. Carson St., Pittsburgh, Pa. 15219)

4-6. Instrument Soc. of America, 8th Biomedical Sciences Instrumentation Symp., Denver, Colo. (L. J. Brannick, E. R. Squibb & Sons, Inc., New Brunswick, N.J. 08901)

4-8. American Nurses Assoc., Miami, Fla. (Mrs. A. R. Warner, Dept. 10, Columbus Circle, New York 10019)

4-8. Society of Plastics Engineers, New York, N.Y. (J. H. Hyden, SPE, 656 W. Putnam Ave., Greenwich, Conn. 06830)

4-8. Veterinary Conf. and Wildlife Disease Assoc., joint biennial mtg., Atlanta, Ga. (W. G. Winkler, Program Chairman, Veterinary Science Dept., Univ. of Wisconsin, Madison 53706)

5-6. Institute of Electrical and Electronics Engineers Appliance Technical Conf., 21st annual, Mansfield, Ohio. (W. H. Lynn, Registration Chairman, Tappan Co., 250 Wayne St., Mansfield, Ohio 44906)

5-6. Association of American Physicians, Atlantic City, N.J. (J. B. Hickman, Indiana Univ. Medical Center, 1100 W. Michigan St., Indianapolis 46202)

5-7. Biometric Soc., eastern North American regional, Chapel Hill, N.C. (D. G. Gosslee, P.O. Box 713, Oak Ridge, Tenn. 37830)

5-7. Purdue Industrial Waste Conf., 25th, Lafayette, Ind. (D. E. Bloodgood, School of Civil Engineering, Purdue Univ., Lafayette 47907)

5-7. Institute of Mathematical Statistics, Chapel Hill, N.C. (L. Katz, Statistical Lab., Michigan State Univ., East Lansing 48823)

5-7. Modern Welding Techniques Conf., Los Angeles, Calif. (J. A. Fellows, American Soc. for Metals, Metals Park, Ohio 44073)

5-8. Virginia Acad. of Science, Richmond. (R. C. Berry, The Academy, P.O. Box 9211, Richmond 23227)

6-8. Society of Mining Engineers, Socorro, N.M. (P. H. Johnson, New Mexico State Bureau of Mines and Mineral Resources, Campus Sta., Socorro 87801)

6-9. American Inst. of Industrial Engineers, Cleveland, Ohio. (J. J. Jericho, AIIE, 345 E. 47 St., New York 10017)

A Really Small Dew Point Sensor

It's shown here actual size and is used with the YSI Model 91 Dew Point Hygrometer to measure dew point temperature and vapor pressure in small spaces and static gas environments.



2 1/4" long
3/8" diameter

A second, slightly larger sensor, measures in moving air and at low ambient temperature.

The sensors are interchangeable and will operate remotely on long leads.

Both dew point and ambient temperatures are available for continuous, simultaneous recording.

Write, and we'll send specifications on the full line of YSI's new humidity instruments.

YELLOW SPRINGS INSTRUMENT CO.
YELLOW SPRINGS, OHIO 45387

Circle No. 86 on Readers' Service Card

7-8. National **Information Retrieval** Colloquium, 7th annual, Philadelphia, Pa. (P. Bagley, Information Engineering, 3401 Market St., Philadelphia)

7-9. Northeastern **Anthropological** Conf., Ottawa, Ont., Canada. (F. G. Vallee, Carleton Univ., Ottawa)

7-9. International **Communication** Assoc. Conf., 18th annual, Minneapolis, Minn. (R. W. Pace, Communication Program, Univ. of Montana, Missoula 59801)

8-10. Society of **Biological Psychiatry**, San Francisco, Calif. (C. Shagass, Eastern Pennsylvania Psychiatric Institute, Henry Ave. and Abbottsford Rd., Philadelphia 19129)

8-11. American **Psychoanalytic** Assoc., San Francisco, Calif. (H. Fischer, Executive Secretary, APA, 1 E. 57 St., New York 10022)

10. Association for the Advancement of **Psychotherapy**, Inc., 9th natl. conf., San Francisco, Calif. (S. Lesse, 15 W. 81 St., New York 10024)

10-12. American Assoc. of **Plastic Surgeons**, Colorado Springs, Colo. (C. W. Monroe, 715 Lake St., Oak Park, Ill. 60301)

10-14. **Metallurgical** Soc., Las Vegas, Nev. (J. V. Richard, Secretary, The Society, 345 E. 47 St., New York 10017)

10-15. **Chemical Vapour Deposition**, 2nd intern. conf., Los Angeles, Calif. (W. W. Smeltzer, Dept. of Metallurgy and Metallurgical Engineering, McMaster Univ., Hamilton, Ont., Canada)

10-15. **Electrochemical** Soc., Los Angeles, Calif. (E. G. Enck, Executive Secretary, The Society, 30 E. 42 St., New York 10017)

11-12. Council of **Biology Editors**, Ottawa, Ont., Canada. (K. Heumann, 9650 Rockville Pike, Bethesda, Md. 20014)

11-13. Instrument Soc. of America, 16th **Aerospace Instrumentation** Symp., Seattle, Wash. (J. M. Taylor, 3246 116th S.E., Bellevue, Wash. 98004)

11-13. American Soc. for **Quality Control** Technical Conf. and Exhibit, 24th annual, Pittsburgh, Pa. (R. W. Shearman, Administrative Secretary, The Society, 161 W. Wisconsin Ave., Milwaukee, Wis. 53203)

11-13. **Television Measuring Techniques** Conf., London, England. (R. Larry, Institution of Electronic and Radio Engineers, 8-9, Bedford Sq., London, W.C.1, England)

11-14. International **Microwave** Symp., Newport Beach, Calif. (R. H. Duhamel, Granger Assoc., 1601 California Ave., Palo Alto, Calif. 94304)


11-15. **High Pressure**, 3rd intern. conf., Aviemore, Invernesshire, Scotland. (J. Schoeffer, Institution of Mechanical Engineers, 1 Birdcage Walk, London, S.W.1, England)

11-15. American **Industrial Hygiene** Assoc., Detroit, Mich. (G. D. Clayton, AIHA, 25711 Southfield Rd., Southfield, Mich. 48075)

11-15. American **Psychiatric** Assoc., San Francisco, Calif. (B. W. Hogan, APA, 1700 18th St., NW, Washington, D.C. 20009)

12-14. **Metal Matrix Composites** Conf., San Francisco, Calif. (J. A. Fellows, American Soc. for Metals, Metals Park, Ohio 44073)

20 MARCH 1970

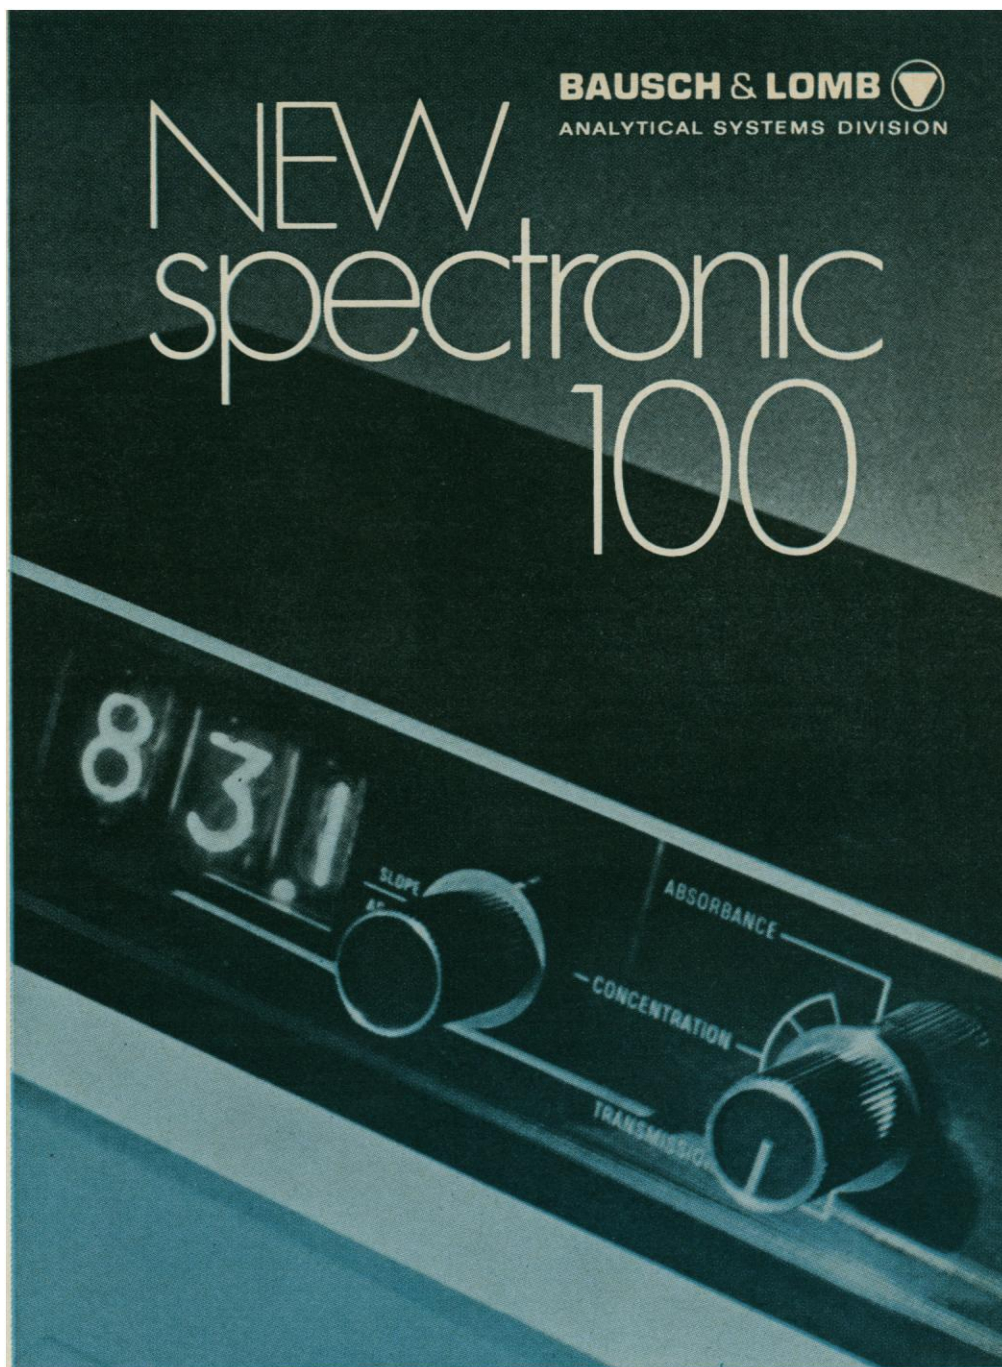

four place digital readout, three modes: linear T and A, plus concentration

The new Spectronic® 100 is one of the most versatile, yet accurate and reliable Spectrophotometers available in the medium price range. It provides the customer with maximum operational ease and instrument appeal as well as unprecedented measurement flexibility and versatility. It permits the analyst to read results in transmittance, absorbance, or absolute concentration units directly from single, multiple or micro-flow thru cells, using a digital Nixie tube display. BCD output is available from a 40 pin connector at the rear of the instru-

ment enabling the user to quickly and conveniently use any one of a variety of recording or printout devices — analog or digital.

Wavelength range extends from 325nm-925nm, with a 8.0nm bandpass. Readout to four digits: in transmittance from 000.0-100.0%, in absorbance from 0.000 to 2.000A and in concentration from 0000-2000 with selectable positioning of the decimal point.

Reliability of the Spectronic 100 is demonstrated in the short term stability of better than 0.001A, and long term stability of less than 0.001A/hr., coupled with zero drift of less than 0.2% per day.

For more details, write for Catalog 33-6031. If you'd like to see one in your lab, we'll gladly arrange a demonstration. Contact Analytical Systems Division, Bausch & Lomb, 9003-15 Linden Avenue, Rochester, New York 14625.

Visit our booth at the FASEB Convention.




Spectronic 100 Spectrophotometer

Circle No. 30 on Readers' Service Card

SAGE ADDS VERSATILITY TO YOUR MICROSCOPE

Complete Cinemicrography Systems


Complete systems for taking time lapse and normal speed 16 mm motion pictures through up-right and inverted microscopes. Assure sharp, clear pictures of living materials at high magnifications. Table-top and console models available.

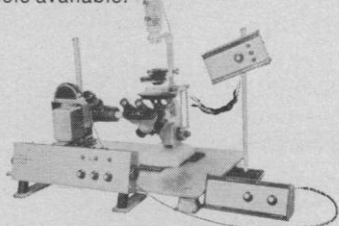

Series 500 Models (shown) — from \$1,810
For information, circle #90 on reader service card.

Photomicrography Exposure Meters


Precalibrated and direct-reading, Sage exposure meters make photomicrography, swift, sure, semi-automatic. Cover film speed range of ASA 20-3000. All camera backs may be used. Models available for A-O, B&L Zeiss microscopes and Leitz Aristophot Stand.

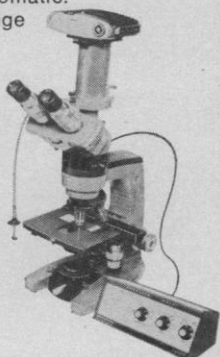

Model 297 (shown)
for A-O Series
10 & 20 — Price \$350
For information, circle #91 on reader service card.

Air Curtain Incubator

The incubator without an enclosure! Holds temperature of biological specimens under the microscope to $\pm 0.3^\circ\text{C}$ anywhere within 30° to 40°C range. Blows soft stream of warm or ambient air onto a specimen as demanded by a thermistor attached to specimen.

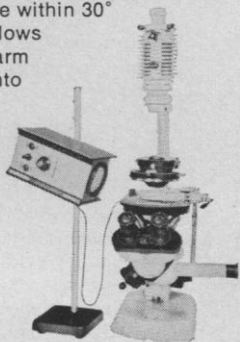

Model 279 (shown) — \$395
For information, circle #92 on reader service card.

SAGE INSTRUMENTS, INC.

Subsidiary of Orion Research Incorporated
230 Ferris Avenue, White Plains, N.Y. 10603
914 949-4121

See us at FASEB Booth A-17

13-15. **Electronics Components Conf.**, Washington, D.C. (D. Burks, Sprague Electric Co., North Adams, Mass. 01247)

14. **Modern Methods of Analyses of Surfaces Symp.**, Murray Hill, N.J. (J. D. Levine, Symp. Chairman, RCA Labs, Princeton, N.J.)

14-15. **Materials Selection Symp.**, Cleveland, Ohio. (W. M. Mueller, American Soc. for Metals, Metals Park, Ohio 44073)

14-15. **Southern Textile Research Conf.**, 10th annual, Hilton Head Island, S.C. (D. W. Snyder, Crompton Shenandoah Co., Drawer 907, Waynesboro, Va. 22980)

14-16. **Cardiovascular Diseases**, 6th annual symp., Hartford, Conn. (R. M. Jere-saty, Section of Cardiopulmonary Medicine, St. Francis Hospital, Hartford)

14-16. **American Inst. of Chemists**, Pittsburgh, Pa. (P. B. Slawter, 79 Madison Ave., New York 10016)

15-19. **International Assoc. of Professional Numismatists**, 19th general assembly, Scheveningen, The Hague, Netherlands. (A. Cronheim, Director, Holland Organizing Centre, 16 Lange Voorhout, The Hague)

17-18. **Modern Methods of Chemical Separations Symp.**, Buffalo, N.Y. (L. B. Church, Dept. of Chemistry, State Univ. of New York at Buffalo, Buffalo 13214)

17-20. **American Inst. of Chemical Engineers and Puerto Rican Inst. of Chemical Engineers**, 3rd joint mtg., San Juan, Puerto Rico. (P. Santiago, Caribbean Gulf Refining, San Juan)

17-21. **Pulp Bleaching**, 5th intern. conf., Atlanta, Ga. (R. A. Joss, Canadian Pulp and Paper Assoc., 2300 Sun Life Bldg., Montreal, P.Q., Canada)

17-30. **International Electrotechnical Commission**, Washington, D.C. (D. Hogan, U.S.A. Standards Inst., 10 E. 40 St., New York 10016)

18-20. **National Aerospace Electronics Conf.**, Dayton, Ohio. (Inst. of Electrical and Electronics Engineers, Dayton Office, 134 E. Monument St., Dayton 45402)

18-20. **American Gastroenterological Assoc.**, Boston, Mass. (H. D. Janowitz, Mt. Sinai Hospital, 11 E. 100 St., New York 10029)

18-20. **Neonatal Enteric Infections Caused by *Escherichia coli***, Conf., New York, N.Y. (L. R. Neville, New York Acad. of Sciences, 2 E. 63 St., New York 10021)

18-20. **Instrument Soc. of America, Power Instrumentation Symp.**, 13th, Kansas City, Mo. (R. A. Russell, Box 8405, Kansas City 64114)

18-20. **Steels for Dynamic Loading**, Cleveland, Ohio. (W. M. Mueller, American Soc. for Metals, Metals Park, Ohio)


18-21. **Photosynthetic Unit**, intern. conf., Gatlinburg, Tenn. (R. M. Pearlstein, Oak Ridge Natl. Lab., P.O. Box Y, Oak Ridge, Tenn. 37830)

18-22. **Air Force Materials Symp.** '70, Miami Beach, Fla. (J. Shipp, Executive Director, AFMS '70, P.O. Box 38, Dayton, Ohio 45420)

18-22. **Medical Library Assoc.**, New Orleans, La. (H. B. Schmidt, Executive Secretary, MLA, 919 N. Michigan Ave., Chicago, Ill. 60611)

18-22. **Society of Photographic Scientists and Engineers**, 23rd annual conf., New York, N.Y. (F. Brown, Logetronics,

new discovery

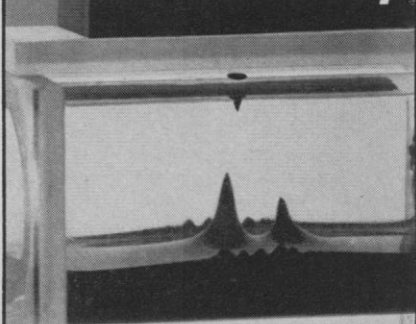

MAGNETIC FLUIDS . . . stimulate new product ideas

Magnetic fluids (ferrofluids) are an exciting new discovery. Ferrofluids react strongly when a magnetic field is applied to them and yet completely retain their liquid character, such as the magnetic fluid stalactite and stalagmites shown in the above photograph. They incorporate tiny magnetic particles colloiddally suspended in a carrier liquid forming a new type of fluid.

Ferrofluids can be positioned, controlled, communicated with, and caused to produce a variety of physical effects by remote magnetic sources.

Entirely new products are being created by employing magnetic fluids; applications in the medical field appear especially promising.

Phenomena include:

- Spatial positioning against forces of gravity, centrifugal force, and pressure etc.
- Impartation of artificial specific gravity — permits flotation of high density liquid or solid materials
- Levitation of magnetic bodies.
- Fluid mechanical instabilities causing liquid spikes.
- Control of surface wave propagation.
- Electromagnetic coupling to produce organized flow.
- Magnetic control of the speed and trajectory of a ferrofluid jet
- Generation and transmission of electromagnetic pulses.

Ferrofluidics Corporation — pioneering in the research and production of magnetic fluids — produces families of magnetic fluids in many different base liquids including water, esters, hydrocarbons, silicones, fluorocarbons and others.



An evaluation kit containing 10 c.c. of kerosene-base fluid and a syringe dispenser can be purchased for \$75. Quantity discount schedule on magnetic fluids is available. Direct inquiries and purchase orders to:



FERROFLUIDICS CORPORATION

144 Middlesex Turnpike
Burlington, Massachusetts 01803
Telephone: 617 272-5206

Circle No. 93 on Readers' Service Card

SCIENCE, VOL. 167

7001 Louisdale Rd., Springfield, Va. 22150)

19-20. International Conf. on **Magnet Technology**, Hamburg, Germany. (W. Jentschke, German Hamburg Electron Synchrotron, Notkeskieg 1, D-2, Hamburg 52)

19-22. Society for **Experimental Stress Analysis**, Huntsville, Ala. (B. E. Rossi, 21 Bridge Sq., Westport, Conn. 06880)

20-22. Conference on **Fracture Control: Theory and Application**, Chicago, Ill. (A. M. Mueller, American Soc. for Metals, Metals Park, Ohio 44073)

20-22. **Teratology Soc.**, 10th annual, Annapolis, Md. (R. W. Miller, 402 Wisconsin Bldg., Bethesda, Md. 20014)

22-29. International **Cancer Congr.**, 10th, Houston, Tex. (M. M. Copeland, Univ. of Texas, P.O. Box 20465, Houston 77025)

24-28. Institute of **Food Technologists**, San Francisco, Calif. (C. L. Willey, IFT, 221 N. LaSalle St., Chicago, Ill. 60601)

24-28. International Congr. of **Social and Preventive Medicine**, 3rd, Venice, Italy. (S. Vanasia, General Secretary, The Congress, 71, via M. Macchi, Milan, Italy)

24-29. Chemical Inst. of Canada/Canadian Soc. for **Chemical Engineering**, Toronto, Ont. (W. M. Campbell, Ontario Research Foundation, Sheridan Park, Ontario, Canada)

24-30. European **Cultural Foundation Congr.**, 7th, Rotterdam, Netherlands. (Secretariat, Holland Organizing Centre, 16, Lange Voorhout, The Hague, Netherlands)

25-26. Symposium on **Biochemistry of Brain and Memory**, Kenosha, Wis. (S. P. Datta, Univ. of Wisconsin-Parkside, Kenosha 53140)

25-26. Progress in **Gas Dynamic Research by Optical Methods**, Syracuse, N.Y. (D. S. Dosanjh, Dept. of Mechanical and Aerospace Engineering, Syracuse Univ., Syracuse 13210)

25-29. European Conf. on **Psychosomatic Research**, 8th, Knokke, Belgium. (M. E. Houben, Universitaire St. Jozeikliniek voor Psychiatrie, 3070 Kortenberg, Belgium)

26-29. **Textile Institute Conf.**, 5th annual, London, England. (Textile Inst., 10 Blackfriars St., Manchester 3, England)

27-29. **Alcohol and Drug Addiction Foundation Symp.**, Toronto, Canada. (R. M. Gilbert, Addiction Research Foundation, 344 Bloor St. W., Toronto 179, Ont.)

30-1. Pan American **Cancer Cytology Congr.**, Jamaica, B.W.I. (J. E. Ayre, Westbury Quadrangle, 113 S. Service Rd., Jericho, N.Y. 11753)

June

1-5. Symposium on Use of **Computers for Automatic Control of Traffic**, Versailles, France. (G. Ruppel, Intern. Federation of Automatic Control, Postfach 1139, Dusseldorf 1, Germany)

1-6. International **Mineral Processing Congr.**, 9th, Prague, Czechoslovakia. (U. P. Vyskub Rud, Modranska 23, Prague 4)

1-6. World **Mining Congr.**, 6th, Madrid, Spain. (A. G. Readett, Natl. Coal Board, Hobart House, Grosvenor Pl., London, S.W.1, England)

20 MARCH 1970



325-925nm range, 8nm bandpass high stability and reliability

The wide wavelength range of the new Spectronic® 70 is continuous. Phototubes and filters are automatically interchanged—no manual changing is required. Readout is in absorbance units and linear transmittance—on a large, mirror-scale meter. A fast optical system of an entirely new design combines fine accuracy and mechanical stability with easy operation. The all solid state electronics with the latest in integrated circuit technology assure high stability and reliability, and exceptional precision.



Operation is extremely simple: set wavelength, adjust for 100% T or 0.0A with reference, introduce sample and read. An accessory outlet allows instant attachment of a variety of readouts including strip-chart recorders, digital readouts, the B&L Concentration Computer for direct concentration readings, and a digital voltmeter for Nixie tube display.


Unprecedented sampling flexibility permits use of cylindrical cells up to 50mm path length and rectangular cells—either semi-micro, short path or constant temperature cells.

For more details, write for Catalog 33-6030. If you'd like to see one in your lab, we'll gladly arrange a demonstration. Contact Analytical Systems Division, Bausch & Lomb, 9003-70 Linden Avenue, Rochester, New York 14625.

Visit our booth at the FASEB Con-

THIS PHASE SENSITIVE DETECTOR

*...is ultra-stable,
linear, wideband,
priced very low and...*

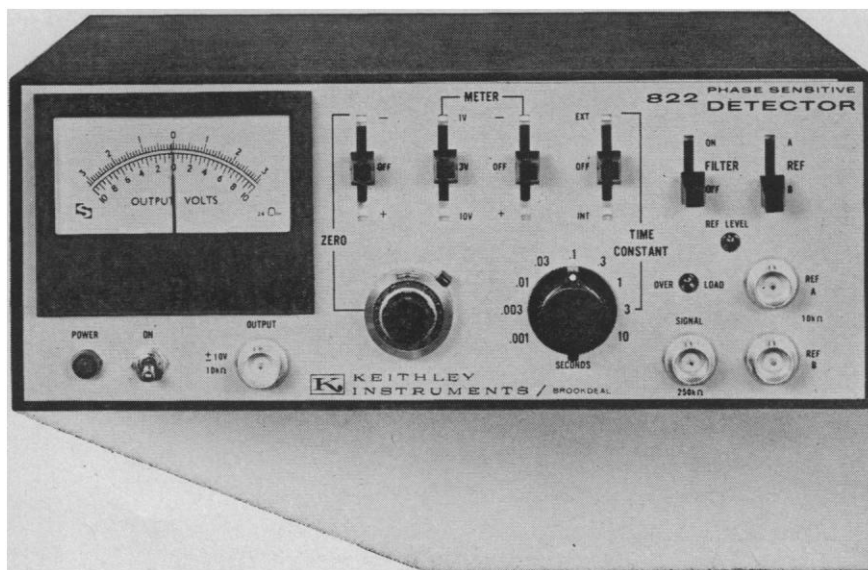

CAN ALSO REPLACE EXPENSIVE LOCK-IN AMPLIFIERS.

The Model 822 takes general purpose lock-in performance out of the high cost instrument class and brings it down to the economy class. It does it with snappy performance, recovering signals 70 dB below noise. Look at these specs: 1 Hz to 1 MHz operation, without tuning or adjustments. 100 microvolts resolution to 1 volt full scale, referred to input. Stability exceeding 0.005% of full output/ $^{\circ}\text{C}$. ± 10 volts dc output from 10 kilohms impedance drives digital voltmeters, A to D converters and potentiometric recorders.

Its wideband design eliminates need for tuning and prevents

phase and gain instabilities often associated with tuned devices. As a result, system gain is constant in the Model 822—calibration is unnecessary. So is a high price tag. The Model 822 is yours for only \$770.

For technical literature and demonstration, contact your Keithley Sales Engineer. Or, write Keithley Instruments, Inc., 28775 Aurora Road, Cleveland, Ohio 44139. Telephone: (216) 248-0400. In Europe: 14 Ave. Villardin, 1009 Pully, Suisse. Prices slightly higher outside the U. S. A.



KEITHLEY

1-6. World Congr. of **Occupational Therapists**, 5th, Zurich, Switzerland. (G. Stauffer, Kraftstr. 22, 8044, Zurich)

2-4. Conference on **Stress Corrosion Cracking**, New Orleans, La. (J. A. Fellows, American Soc. for Metals, Metals Park, Ohio 44073)

2-5. Mid-American Symp. on **Spectroscopy**, 22nd, Chicago, Ill. (W. A. Loseke, IIT Research Inst., 10 W. 35 St., Chicago 60616)

3-5. American **Chemical Soc.**, Central regional, 2nd, Columbus, Ohio. (R. W. Bird, 2540 Olentangy River Rd., Columbus 43210)

4-5. **Environmental and Water Resources Engineering Conf.**, 9th annual, Nashville, Tenn. (E. L. Thackston, Vanderbilt Univ., Box 133, Sta. B, Nashville 37203)

4-5. **Molecular Biology**, 4th intern. symp., New York, N.Y. (E. G. Bassett, Research Products Div., Miles Laboratories, Inc., Elkhart, Ind. 46514)

7-9. **Computer Applications in the Earth Sciences**, 8th colloquium, Lawrence, Kans. (D. F. Merriam, Kansas Geological Survey, Univ. of Kansas, Lawrence 66044)

7-10. American Soc. of **Mechanical Engineers**, Boston, Mass. (A. B. Conlin, Jr., 345 E. 47 St., New York 10017)

8-9. **Choice Criteria and Management Systems for Estuarine Resources Conf.**, Charleston, S.C. (J. C. Hite, Dept. of Agricultural Economics, Clemson Univ., Clemson, S.C. 29631)

8-10. International Conf. on **Communications**, San Francisco, Calif. (A. M. Peterson, Stanford Research Inst., Menlo Park, Calif. 94025)

8-10. Association for **Gnotobiotics**, Notre Dame, Ind. (M. Pollard, Dept. of Microbiology, Univ. of Notre Dame, Notre Dame 46556)

8-10. Conference on **Powder Metallurgy**, Detroit, Mich. (J. A. Fellows, American Soc. for Metals, Metals Park, Ohio 44073)

8-12. International **Gas Conf.**, 11th, Moscow, U.S.S.R. (R. H. Tonwaide, General Secretary, Intern. Gas Union, 4 Av. Palmerston, Brussels 4, Belgium)

8-12. International Symp. on **Plant Protein: Their Improvement through the Application of Nuclear Techniques**, Vienna, Austria. (J. H. Kane, U.S. Atomic Energy Commission, Washington, D.C. 20545)

9-12. American **Astronomical Soc.**, Boulder, Colo. (H. M. Gurin, 211 Fitz Randolph Rd., Princeton, N.J. 08540)

9-12. Canadian Federation of **Biological Societies**, 13th annual, Montreal. (K. K. Carroll, Dept. of Biochemistry, Univ. of Western Ontario, London 72, Canada)

10-12. **Low Energy X- and Gamma Ray Sources and Applications**, 3rd symp., Boston, Mass. (J. W. Hitch, Div. of Isotopes Development, U.S. Atomic Energy Commission, Washington, D.C. 20545)

11-13. **Endocrine Soc.**, St. Louis, Mo. (N. L. Mattox, Suite 304, 1211 N. Sharel, Oklahoma City, Okla. 73103)

12-14. Society of **Biological Psychiatry**, Atlantic City, N.J. (G. N. Thompson, 2010 Wilshire Blvd., Los Angeles, Calif. 90057)

13-14. American **Diabetes Assoc.**, St. Louis, Mo. (J. R. Connelly, 18 E. 48 St., New York, N.Y. 10017)

14-18. **Botanical Soc. of America**,

northwestern section, New London, Conn. (R. K. Zack, Dept. of Botany, Drew Univ., Madison, N.J. 07940)

14-18. **American Nuclear Soc.**, Los Angeles, Calif. (O. J. Du Temple, 244 E. Ogden Ave., Hinsdale, Ill. 60521)

14-18. **National Plastics Exposition and Conf.**, Cleveland, Ohio. (L. P. Williams, 250 Park Ave., New York 10017)

14-19. **Air Pollution Control Assoc.**, 63rd annual, St. Louis, Mo. (A. Arch, 4400 Fifth Ave., Pittsburgh, Pa. 15213)

14-19. **Mass Spectrometry and Allied Topics**, 18th annual conf., San Francisco, Calif. [J. M. McCrea, Applied Research Lab. (73), U.S. Steel Corp., Monroeville, Pa. 15146]

14-19. **Canadian Assoc. of Pathologists**, Winnipeg, Man. (C. W. Penner, Winnipeg General Hospital, Winnipeg 3)

15-16. **Catalytic Hydrogenation and Analogous Pressure Reactions**, 3rd conf., New York, N.Y. (L. R. Neville, New York Acad. of Sciences, 2 E. 63 St., New York 10021)

15-17. **American Neurological Assoc.**, 95th annual, Atlantic City, N.J. (S. A. Trufant, Cincinnati General Hospital, Cincinnati, Ohio 45229)

15-17. **National Conf. of Standards Laboratories**, Gaithersburg, Md. (R. J. Barra, Westinghouse Defense and Space Center, P.O. 746, Baltimore, Md. 21203)

15-18. **American Soc. for Engineering Education**, Columbus, Ohio. (W. L. Collins, 2100 Pennsylvania Ave., NW, Washington, D.C. 20037)

15-18. **American Meteorological Soc. Symp.**, Boulder, Colo. (J. London, Dept. of Astro-Geophysics, Univ. of Colorado, Boulder 80302)

15-18. **Tissue Culture Assoc.**, 21st annual, Washington, D.C. (V. P. Perry, American Foundation for Biological Research, 11125 Rockville Pike, Rockville, Md. 20853)

15-19. **International Symp. on Information Theory**, Noordwijk, Netherlands. (P. E. Green, Jr., M.I.T. Lincoln Lab., Lexington, Mass. 02173)

15-19. **Nuclear Data for Reactors**, 2nd intern. conf., Helsinki, Finland. (J. H. Kane, Div. of Technical Information, U.S. Atomic Energy Commission, Washington, D.C. 20545)

15-19. **Vacuum Metallurgy**, intern. conf., Anaheim, Calif. (E. L. Foster, Battelle Memorial Inst., 505 King Ave., Columbus, Ohio 43201)

15-19. **American Water Resources Assoc. Conf.**, Milwaukee, Wis. (G. Karadi, Dept. of Applied Sciences and Engineering, Univ. of Wis., Milwaukee 53201)

16-17. **Environmental Variables in Animal Experimentation**, 2nd annual, Metropolitan Branch, American Assoc. for Lab. Animal Science, New Brunswick, N.J. (D. Miller, Smith Kline & French, 1500 Spring Garden St., Philadelphia, Pa.)

16-18. **Conference on Cold Forming of Metal Parts**, Cleveland, Ohio. (J. A. Fellows, American Soc. for Metals, Metals Park, Ohio 44073)

16-18. **American Helicopter Soc.**, 26th annual natl. forum, Washington, D.C. (H. M. Lounsbury, 30 E. 42 St., New York 10017)

16-19. **Canadian Psychiatric Assoc.**,

Our Breed-in.

They're the class of '70. Inbred mouse strains developed and maintained by Dr. Leonell C. Strong.

These strains of mice have been the most generally accepted in cancer research. And in other studies requiring inbred mice. Recently, they've been the toast of the Continent through a limited marketing program by Charles River France. Now, we'll produce them commercially this Spring for the first time in the U.S. DBA/2, C57BL/6, C3H, A and BALB/c. And from these, appropriate hybrid lines.

All foundation and expansion colonies have been Caesarean-derived and maintained in germfree isolaters. All of your inbred mice will be produced under our COBS® system. Nearly all strains will also be available in germfree. In all, the same top quality you've received in our randombred mice.

We'd be happy to make your research effort a Strong one. Call or write Charles River Breeding Laboratories, Wilmington, Mass. 01887 or Charles River France in Elbeuf.

Charles River
BREEDING LABORATORIES, INC.
WILMINGTON, MASSACHUSETTS 01887





Worthington Nucleotides

... new addition to the house of enzymes


Worthington Biochemical, the house that enzymes built, has added a new wing—a broad line of nucleotides.

Our list of more than 230 products—high-purity research, diagnostic, and specialty enzymes—is supplemented by a basic list of 75 high-purity nucleotides. The two product lines are complementary, offering several advantages to the user of biochemicals.

- our standards and guarantees of quality extend equally to both enzymes and nucleotides
- our technical capability as a prime source of enzymes is applied with equal rigor to the quality control and testing of nucleotides
- your time and effort is saved through ordering your high-purity biochemicals from a single, reliable source

Take advantage of our enzymes and nucleotides being under the same roof. Order them direct from Worthington.

Ask for our new comprehensive catalog of high-purity biochemicals.

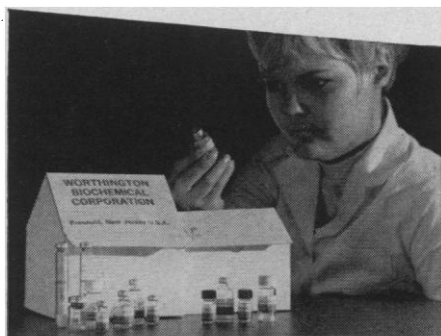

Worthington Biochemical Corporation
Freehold, New Jersey 07728

Please send the following:

- ☐ Worthington Biochemical Catalog
☐ Enzyme Diagnostic Reagent Catalog
☐ Information on Worthington Specialty Enzymes

Name _____

Title _____

Institution _____

Address _____

City _____

State _____

Zip _____

20th annual, Winnipeg, Man. (W. A. Blair, 225 Lisgar St., Ottawa, Ont., Canada)

17-18. **European Dialysis and Transplant Assoc.**, 7th annual, Barcelona, Spain. (W. Drokker, 75 de Lairessestraat, Amsterdam, Netherlands)

17-19. **Cryogenic Engineering Conf.**, Boulder, Colo. (J. L. Smith, Jr., Rm. 41-204, Massachusetts Inst. of Technology, Cambridge, Mass. 02130)

17-20. **American Rheumatism Assoc.**, Detroit, Mich. (M. M. Walsh, 1212 Ave. of the Americas, New York 10036)

17-21. **American Therapeutic Soc.**, Chicago, Ill. (R. T. Smith, 37 Narbrook Pk., Narberth, Pa. 19072)

17-24. **Chemical Engineering and Congr. of Chemical Engineers**, Frankfurt-am-Main, Germany. (J. Dohent, Natl. Chemical Exposition, 86 E. Randolph St., Chicago, Ill. 60601)

18-19. **Current Concepts of the Histology of the Oral Mucosa Symp.**, Chicago, Ill. (C. A. Squier, College of Dentistry, Univ. of Illinois at the Medical Center, Chicago 60680)

18-20. **Bibliographical Soc. of America**, Philadelphia, Pa. (W. H. Bond, Houghton Library, Harvard Univ., Cambridge, Mass. 02138)

18-20. **American Assoc. of Bioanalysts**, New York, N.Y. (D. Birenbaum, 802 Ambassador Bldg., St. Louis, Mo. 63101)

20-25. **American Soc. of Radiologic Technologists**, Miami Beach, Fla. (G. J. Eilert, 527 S. Main St., Fond du Lac, Wis. 54935)

21-24. **American Dairy Science Assoc.**, 65th annual, Gainesville, Fla. (C. Cruse, 903 Fairview Ave., Urbana, Ill. 61801)

21-24. **American Leather Chemists Assoc.**, Lake Placid, N.Y. (M. T. Roddy, c/o Tanners Council Research Laboratories, Univ. of Cincinnati, Cincinnati, Ohio 45221)

21-25. **American Association for the Advancement of Science**, Pacific Div., Berkeley, Calif. (R. C. Miller, California Acad. of Sciences, Golden Gate Park, San Francisco 94118)

21-25. **American Medical Assoc.**, Chicago, Ill. (W. E. Burmeister, 535 N. Dearborn St., Chicago, Ill. 60610)

21-25. **American Veterinary Medical Assoc.**, Las Vegas, Nev. (D. A. Price, 600 Michigan Ave., Chicago, Ill. 60605)

21-26. **American Soc. for Testing and Materials**, Toronto, Ont., Canada. (T. A. Marshall, Jr., ASTM, 1916 Race St., Philadelphia, Pa. 19103)

22-24. **International Conf. on the Role of Tryptophan Metabolism in Biochemistry and Pathology**, Madison, Wis. (T. C. Meyer, Univ. of Wisconsin, Madison 53706)


22-25. **Canadian Soc. of Agronomy**, Ottawa, Ont. (R. Loiselle, Ottawa Research Sta., Central Experimental Farm, Ottawa)

22-25. **Symposium on Bioinorganic Chemistry**, Blacksburg, Va. (R. E. Dessy, Dept. of Chemistry, Virginia Polytechnic Inst., Blacksburg 24061)

22-25. **Canadian Soc. of Horticultural Science**, Ottawa, Ont. (E. C. Loughheed, Dept. of Horticulture, Univ. of Guelph, Guelph, Ont.)

22-25. **American Assoc. of Petroleum Geologists**, Calgary, Alta., Canada. (J. M.

THE MOST^{*} (OF EVERYTHING) FOR THE MONEY

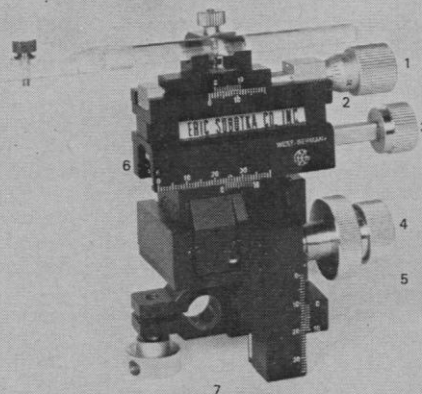


MINIATURE MICROMANIPULATOR MM-33

from the Sobotka organization

- 1 Fine motion "X" direction with 20mm range
- 2 Micrometer drum and vernier reading to 0.1mm with an accuracy of 10 microns for each division.
- 3 Coarse motion "X" direction with 40mm range
- 4 Coaxial vertical and horizontal movements, 30mm vertical and 22mm horizontal
- 5 All controls placed in linear plane for ease and convenience
- 6 Ball bearing slideways for no wear, no backlash performance
- 7 Only 18 oz. eliminates swaying on any type stand

*At \$200.00 the MM-33 offers the most in accuracy, convenience, compactness and ultra-precision throughout the instrument.

Write or call for the facts.

eric  sobotka
company, inc.

Importers and Distributors of
Microscopes and Scientific Instruments

Finn Court, Farmingdale, N.Y. 11735 • 516-293-9272

Browning, Tenneco Oil and Minerals, P.O. Box 1051, Calgary)

22-25. Canadian Soc. of **Soil Science**, Ottawa, Ont. (A. R. Mack, Central Experimental Farm, Ottawa)

22-25. **Thyroid Conf.**, 6th annual, Vienna, Austria. (R. Hofer, c/o Wiener Medizinische Akademie, Alserstrasse 4, A-1090, Vienna)

22-26. American Assoc. of **Avian Pathologists**, Inc., Las Vegas, Nev. (G. H. Snoeyenbos, Univ. of Massachusetts, Amherst 01002)

22-27. **Mathematical Statistics and Probability**, 6th, Berkeley, Calif. (E. L. Scott, Dept. of Statistics, Univ. of California, Berkeley 94720)

23-26. State of the Art in **Corrosion Testing Methods Symp.**, Toronto, Canada. (W. H. Ailor, American Soc. for Testing and Materials, Reynolds Metals Co., 4th and Canal Sts., Richmond, Va. 23218)

24. **Biometric Soc.**, Western North American regional, Berkeley, Calif. (J. S. Williams, Statistical Lab., Colorado State Univ., Fort Collins 80521)

24-26. National **Aeronautics and Space Administration**, Ames Research Center, Moffett Field, Calif. (M. R. Heinrich, NASA, Ames Research Center, Moffett Field 94035)

24-26. American **Automatic Control Conf.**, Atlanta, Ga. (D. Lyons, Dept. of Textiles, Clemson Univ., Clemson, S.C. 29631)

24-26. Canadian **Wood Chemistry Symp.**, 3rd, Vancouver, B.C. (D. A. I. Goring, Pulp and Paper Research Inst. of Canada, 570 St. John's Rd., Pointe Claire, P.Q.)

24-27. **Drugs and Cerebral Function Symp.**, 2nd annual, Denver, Colo. (M. L. Smith, Suite 1120, 2045 Franklin, Denver 80205)

24-27. **Hydrobiology**, natl. symp., Miami Beach, Fla. (J. C. Warman, Water Resources Research Inst., Auburn Univ., Auburn, Ala. 36830)

24-27. Western Soc. of **Malacologists**, 3rd annual, Stanford, Calif. (C. Skoglund, 3846 E. Highland Ave., Phoenix, Ariz. 85018)

24-1. International Symp. on **Mechanical Properties and Processes of the Mantle**, Flagstaff, Ariz. (L. R. Sykes, Columbia Univ., Palisades, N.Y. 10964)

25-27. Conference of **Immunologists**, San Diego, Calif. (W. O. Weigle, Scripps Clinic and Research Foundation, La Jolla, Calif. 92037)

25-27. **Leukocyte Culture Conf.**, 5th, Ottawa, Canada. (J. Harris, Ottawa General Hospital, Ottawa 2)


28-2. **Health Physics Soc.**, 15th annual, Chicago, Ill. (W. J. Blair, Biology Dept., Battelle Northwest, Richland, Wash. 99352)

28-4. American **Library Assoc.**, Detroit, Mich. (D. H. Clift, Executive Director, The Association, 50 E. Huron St., Chicago, Ill. 60611)

28-4. American **Optometric Assoc.**, 73rd annual congr., Honolulu, Hawaii. (G. Allen, Jr., 7000 Chippewa St., St. Louis, Mo. 63119)

29-1. **Drug Metabolism in Man**, New York, N.Y. (E. S. Vesell, Pennsylvania State Univ. College of Medicine, Hershey, Pa.)

**Where can you find
high precision,
versatility and
ruggedness in a
moderately priced
microscope?**

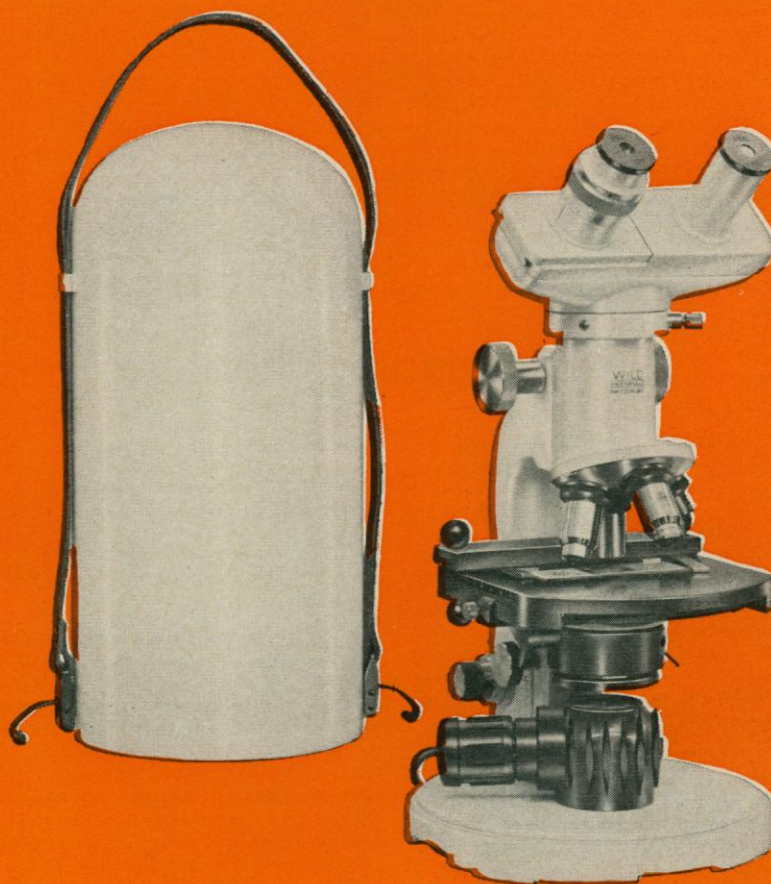

IN THE WILD M-11.

Features: Superb Swiss optics, lasting mechanical precision, light weight, protective steel hood. Base accepts various light sources, including 6v/20w Koehler lamp, and low voltage lamp, for car battery hook-up. The M-11 also accepts photomicrographic cameras, phase contrast attachments, and binocular camera lucida.

Applications: Medical schools, scientific expeditions, biomedical and industrial laboratories.

Price: About that of a good one-track routine microscope. The M-11 is in a class by itself. Write for Booklet M-11.

WILD®
HEERBRUGG

WILD HEERBRUGG INSTRUMENTS, INC.,
FARMINGDALE, NEW YORK 11735

WILD OF CANADA, LTD., 881 LADY ELLEN PLACE, OTTAWA 3, ONTARIO
WILD DE MEXICO, SA, LONDRES 256, MEXICO 6, D.F.

Circle No. 26 on Readers' Service Card