

Sweden. (Secretary General, Institut Alfred Fournier, 25, boulevard Saint-Jacques, Paris 14<sup>e</sup>, France.)

8-15. International Statistical Inst., 30th, Stockholm, Sweden. (Secretary General, ISI 30th Session, Fack, Stockholm 5.)

8-15. International Union for the Scientific Study of Population, Stockholm, Sweden. (F. Lorimer, c/o American University, Washington 16.)

11-14. Heat Transfer, national conf., University Park, Pa. (G. M. Dusinger, Pennsylvania State Univ., University Park.)

11-17. World Federation for Mental Health, 10th annual, Copenhagen, Den-

mark. (Miss E. M. Thornton, 19 Manchester St., London, W.1, England.)

12-16. Canadian Teachers' Federation, annual, Edmonton, Alberta, Canada. (G. G. Croskery, 444 MacLaren St., Ottawa 4, Ont.)

12-18. Theory of Functions, internatl. colloquium, Helsinki, Finland. (B. Eckmann, Ecole Polytechnique, Federale, Zurich, Switzerland.)

12-25. International Soc. of Soil Mechanics and Foundation Engineering, 4th Conf., London, England. (A. Banister, Institution of Civil Engineers, Great George St., London, S.W.1.)

18-21. American Astronomical Soc., Urbana, Ill. (J. A. Hynek, Smithsonian

Astrophysical Observatory, 60 Garden St., Cambridge 38, Mass.)

19-21. National Council of Teachers of Mathematics, Northfield, Minn. (M. H. Ahrendt, NCTM, 1201 16 St., NW, Washington 6.)

19-22. American Veterinary Medical Assoc., annual, Cleveland, Ohio. (J. G. Hardenbergh, AVMA, 600 S. Michigan Ave., Chicago 5, Ill.)

19-23. Clay Conf., 6th natl., Berkeley, Calif. (Dept. of Conferences and Special Activities, Univ. of California Extension, Berkeley 4.)

19-23. Clinical Chemistry, 2nd international European cong., Stockholm, Sweden. (K. Agner, Box 12024, Stockholm 12.)

19-24. Finite Groups, internatl. colloquium, Tübingen, Germany. (H. Wielandt, Faculty of Mathematics and Natural Science, Eberhard-Karls-Universität, Tübingen.)

19-24. High Energy Physics Symp., Oak Ridge, Tenn. (University Relations Div., Oak Ridge Inst. of Nuclear Studies, P.O. Box 117, Oak Ridge.)

19-24. New England Assoc. of Chemistry Teachers, 19th summer conf., Waterville, Maine. (Rev. J. A. Martus, College of the Holy Cross, Worcester 10, Mass.)

19-24. Origin of Life, internatl. symp., Moscow, U.S.S.R. (G. A. Deborin, Inst. of Biochemistry, U.S.S.R. Acad. of Sciences, B. Kaluzskaya 33, Moscow, B.71.)

20-22. Liquid Scintillation Counting Conf., Evanston, Ill. (C. G. Bell, Jr., Technological Inst., Northwestern Univ., Evanston.)

20-23. Western Electronic Convention, annual, San Francisco, Calif. (D. B. Harris, Electron Tube Research, General Electric Microwave Lab., Palo Alto, Calif.)

21-24. Pi Lambda Theta, New York, N.Y. (C. Johnson, Pi Lambda Theta, 307 Portland Bldg., 1129 Vermont Ave., NW, Washington 5.)

22-5. International Scientific Radio Union, 12th general assembly, Boulder, Colo. (K. A. Norton, Boulder Laboratories, National Bur. of Standards, Boulder.)

24-26. International Soc. for Biological Rhythm, 6th conf., Semmering, Austria. (A. Sollberger, Anatomical Department, Karolinska Institutet, Stockholm 60, Sweden.)

25-27. Pacific Division-AAAS, annual, in conjunction with American Inst. of Biological Sciences, Stanford, Calif. (R. C. Miller, California Academy of Sciences, Golden Gate Park, San Francisco, Calif.)

25-28. American Farm Economic Assoc., natl., Asheville, N.C. (L. S. Hardin, Dept. of Agricultural Economics, Purdue Univ., Lafayette, Ind.)

25-29. American Institute of Biological Sciences, annual, Stanford, Calif. (H. T. Cox, AIBS, 2000 P St., NW, Washington 6.)

## COMPLETE ENGLISH TRANSLATION


of any paper from any Russian journal listed below, beginning with the first issue of the indicated year, is available at the price indicated.

Journal	Year translation began	Price per translated report (Effective as of May 1, 1956)
Journal of General Chemistry	(1949)	\$ 7.50
Journal of Applied Chemistry	(1950)	
Bulletin of the Academy of Sciences of the USSR, Div. Chem. Sci.	(1952)	
Colloid Journal	(1952)	
Journal of Analytical Chemistry	(1952)	
Cement	(1956)	
Glass and Ceramics	(1956)	
The Metallurgist	(1956)	\$12.50
Automation and Remote Control	(1956)	
Journal of Atomic Energy	(1956)	\$ 5.00
Sections of the Proceedings (Doklady) of the Academy of Sciences of the USSR:	(1956)	
Chemistry Section		
Chemical Technology Section		
Agrochemistry Section		
Geochemistry Section	(1957)	
Pharmacology and Toxicology		
Physical Chemistry Section		
Applied Physics Section		
Geological Sciences Section	(1957)	
Biochemistry Section		

Papers from these Journals will be provided exactly as they appear in the C.B. published translation, with all tabular material, diagrams, and photographs integral with the text.

In ordering papers, please cite: Title, author, journal, year, and pagination. If the pagination cited is that of the original Russian journal, please so indicate. Write Dept. S.

Consultants Bureau is still seeking Scientist-Translators.  
A complete command of idiomatic English is required.



### CONSULTANTS BUREAU, Inc.

227 W. 17 St.

New York 11, N.Y.


Telephone: ALgonquin 5-0713

The following 28 meetings are being held in conjunction with the AIBS meeting at Stanford, Calif.

American Bryological Soc., annual. (W. C. Steere, Dept. of Biological Sciences, Stanford Univ.)

# GLASS ABSORPTION CELLS

made by **KLETT**

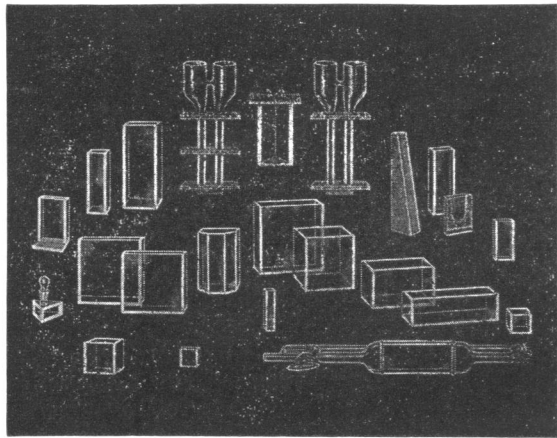


Makers of Complete Electrophoresis Apparatus

— SCIENTIFIC APPARATUS —  
 Klett-Summerson Photoelectric Colorimeters—  
 Colorimeters — Nephelometers — Fluorimeters—  
 Bio-Colorimeters — Comparators — Glass Stand-  
 ards—Klett Reagents.

**Klett Manufacturing Co.**  
 179 East 87 Street, New York, New York

# LEISS

## Single and Double MIRROR-MONOCHROMATORS

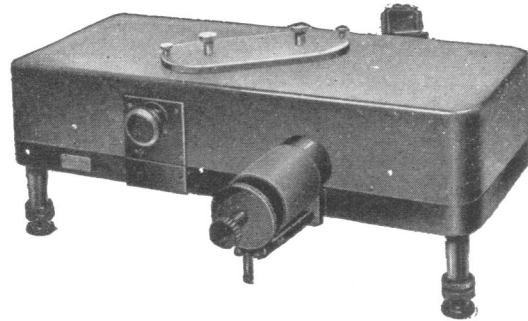

with exchangeable prisms for the visible, ultraviolet, infrared from 200 millimicrons to 20 microns

Write for Bulletin #980 to

**PHOTOVOLT CORP.**  
 95 Madison Ave. New York 16, N. Y.


Get **UNITRON'S FREE**  
**Observer's Guide and Catalog**  
 on **Astronomical Telescopes . .**

*This valuable 38-page book is yours for the asking!*

With the artificial satellite and space travel almost a reality, astronomy has become today's fastest growing hobby. UNITRON'S new handbook contains full-page illustrated articles on astronomy, observing, telescopes and accessories. Of interest to beginner and advanced amateurs alike.

**Contents include —**

- Observing the sun, moon, planets and wonders of the sky
- Constellation map
- Hints for observers
- Glossary of telescope terms
- How to choose a telescope
- Amateur clubs and research programs



**UNITRON**  
*Instrument Division*  
 of **UNITED SCIENTIFIC CO.**


204-6 MILK STREET • BOSTON 9, MASS.

Please rush to me, free of charge, UNITRON'S new Observer's Guide and Telescope Catalog.

Name.....  
 Street.....  
 City..... State.....



# Large Volume!... Super-Speed... refrigerated centrifuge

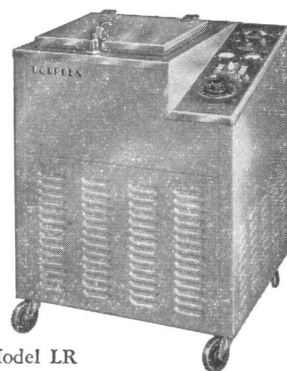

Model LR

The Model LR features a new design refrigeration system which employs forced air circulation through side and bottom cooling areas to provide a continuous laminar flow of cool air streams onto all portions of the rotor. Chamber temperatures may be set as low as  $-15^{\circ}\text{C}$  and automatically maintained within  $\pm 1^{\circ}\text{C}$ . Rotor compartment temperatures are easily maintained at  $0^{\circ}\text{C}$  and lower, even during runs at maximum speed for extended periods.

Instrumentation includes a continuous reading electric tachometer, two hour timer, automatic temperature controller, variable speed controller, ammeter for rotor acceleration control and various operating safety controls.

A full 1 Hp. Universal motor provides direct power to any rotor employed, without the use of cumbersome high speed attachments, pulleys or gears. All rotors are interchangeably used in both refrigerated and non-refrigerated Lourdes' centrifuges without the use of special adapters.

More compact and competitively priced, the Model LR offers highest quality construction, maximum operating efficiency and unsurpassed performance.

FOUR INTERCHANGEABLE ROTORS			
ROTOR	CAPACITY (Max.)	RPM (Max.)	RCF x G (Max.)
1 1/2" Angle	1,500cc (6x250cc)	11,000	20,000
9" Angle	400cc (8x50cc)	15,300	30,000
9" Angle	360cc (24x15cc)	15,300	30,000
Swinging Cup	96cc (8x12cc)	12,000	21,500

NOTE: Adapters available for smaller tubes.

*Backed by over a decade of laboratory instrument manufacturing experience, each LOURDES' unit is guaranteed for a period of one year.*

**LOURDES INSTRUMENT CORP.**  
 53rd STREET and 1st AVENUE • BROOKLYN 32, N. Y.

WRITE FOR LITERATURE. REFER TO S-67

LARGEST MANUFACTURER OF SUPER-SPEED CENTRIFUGES!

American Fern Soc., annual. (I. L. Wiggins, Dept. of Biological Sciences, Stanford Univ.)

American Microscopical Soc., annual. (G. M. Smith, Dept. of Biological Sciences, Stanford Univ.)

American Phytopathological Soc., annual (W. B. Hewitt, Dept. of Plant Pathology, Univ. of California, Davis). 26-28 Aug. only.

American Soc. for Horticultural Science, annual. (H. P. Olmo, Dept. of Viticulture, Univ. of California, Davis.)

American Soc. of Human Genetics. (E. J. Gardner, Dept. of Zoology, Utah State College, Logan.)

American Soc. of Ichthyologists and Herpetologists. (W. C. Brown, Menlo College, Menlo Park, Calif.)

American Soc. of Limnology and Oceanography. (D. E. Wohlschlag, Dept. of Biological Sciences, Stanford, Univ.)

American Soc. of Naturalists, annual. (D. Perkins, Dept. of Biological Sciences, Stanford Univ.)

American Soc. of Plant Physiologists, annual. (W. R. Briggs, Dept. of Biological Sciences, Stanford Univ.)

American Soc. of Plant Taxonomists, annual. (I. L. Wiggins, Dept. of Biological Sciences, Stanford Univ.)

American Soc. of Zoologists, annual. (J. F. Oliphant, Dept. of Biological Sciences, Stanford Univ.)

Biometric Soc., WNAR. (D. E. Wohlschlag, Dept. of Biological Sciences, Stanford Univ.)

Botanical Soc. of America, annual. (W. C. Steere, Dept. of Biological Sciences, Stanford Univ.)

Ecological Soc. of America, annual. (I. L. Wiggins, Dept. of Biological Sciences, Stanford Univ.)

Genetics Soc. of America, annual. (D. Perkins, Dept. of Biological Sciences, Stanford Univ.)

Mycological Soc. of America, annual. (R. M. Page, Dept. of Biological Sciences, Stanford Univ.)

National Assoc. of Biology Teachers.

(Miss E. Larson, Box 2841, Carmel, Calif.)

Nature Conservancy, annual. (W. Drake, Canyon, Calif.)

Phycological Soc. of America, annual. (G. F. Papenfuss, Dept. of Botany, Univ. of California, Berkeley 4.)

Sigma Delta Epsilon. (Mrs. C. B. Parker, 7 Lloyd Rd., Malvern, Pa.)

Society for Experimental Biology and Medicine, Pacific Coast Section. (J. P. Baumberger, Dept. of Physiology, Stanford Univ.)

Society of General Physiologists. (D. Mazia, Univ. of California, Berkeley 4.)

Society for Industrial Microbiology, annual. (J. C. Lewis, Agricultural Research Service, USDA, 800 Buchanan St., Albany 10, Calif.)

Society for the Study of Evolution, annual. (R. W. Holm, Dept. of Biological Sciences, Stanford Univ.)

Society of Protozoologists, annual. (J. F. Oliphant, Dept. of Biological Sciences, Stanford Univ.)

Society of Systematic Zoology, Pacific section. (D. P. Abbott, Hopkins Marine Station, Pacific Grove, Calif.)

Western Soc. of Naturalists, annual. (W. M. Hiesey, Carnegie Institution of Washington, Stanford, Calif.)


in balances ...

and weights, too!

"On my recent sales calls I have noticed that more and more people are becoming conscious of the importance of having good weights to use with good balances.

"When you buy an Ainsworth balance you are buying quality and accuracy. But, even with a good balance it is tough to weigh accurately with poor weights. Ainsworth highly polished non-magnetic Brunton metal weights have a smooth surface for resistance to contamination and corrosion. The hard rhodium plating on their bronze weights maintains accuracy longer. You can depend on Ainsworth weights being within tolerance and staying that way longer...and, with Class S Weights by Ainsworth a fellow doesn't have to worry about corrections in most analytical and semi-micro work.

"These are just a couple of the 'little things that count' in accurate weighing."

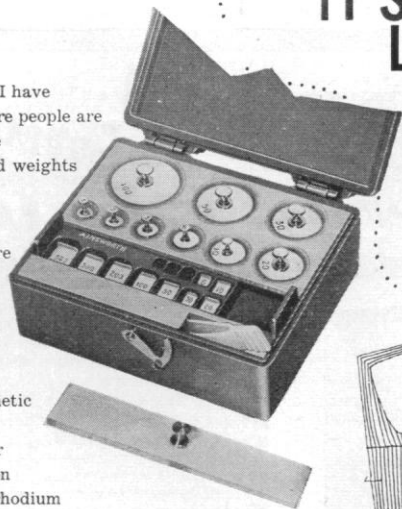

IT'S THE LITTLE THINGS THAT COUNT



Just call your laboratory supply salesman...he can give you more information about Ainsworth proved and improved balances and weights

• or write for catalog

WM. AINSWORTH & SONS, INC.  
2151 LAWRENCE STREET • DENVER 5, COLORADO

26-28. Gas Dynamics Symp., 2nd, Evanston, Ill. (A. B. Cambel, Technological Inst., Northwestern Univ., Evanston.)

26-29. Boundary Layer Research, internatl. symp., Freiburg, Breisgau, Germany. (H. Görtler, Mathematisches Institut der Universität, Hebelstrasse 40 Freiburg, Breisgau.)

26-29. Mathematical Assoc. of America, 38th summer, University Park, Pa. (H. M. Gehman, Univ. of Buffalo, Buffalo 14, N.Y.)

26-30. American Mathematical Soc., 62nd summer, University Park, Pa. (J. H. Curtiss, AMS, 190 Hope St., Providence 6, R.I.)

26-30. Infrared Spectroscopy Inst., 8th annual, Nashville, Tenn. (N. Fuson, Infrared Spectroscopy Inst., Fisk Univ., Nashville 8.)

26-31. Low Temperature Physics and Chemistry, 5th internatl. conf., Madison, Wis. (J. R. Dillinger, Dept. of Physics, Univ. of Wisconsin, Madison 6.)

27. Society for Industrial and Applied Mathematics, summer, University Park, Pa. (D. L. Thomsen, Jr., 807 Enquirer Bldg., Cincinnati 2, Ohio.)

27-29. American Sociological Soc., annual, Washington, D.C. (Mrs. M. W. Riley, ASS, New York Univ., Washington Sq., New York 3.)

27-30. Biological Photographic Assoc., 27th annual, Rochester, Minn. (S. J. McComb, Section of Photography, Mayo Clinic, Rochester.)

28-30. Gas Chromatography, internatl. symp., East Lansing, Mich. (H. J. Noebels, IGC Symp., Instrument Soc. of America, 313 Sixth Ave., Pittsburgh, Pa.)

28-31. Soil Conservation Soc. of America, annual, Asilomar, Calif. (H. W. Pritchard, 838 Fifth Ave., Des Moines 14, Iowa.)

(See issue of 21 June for comprehensive list)

# 50 MICROCURIE C<sup>14</sup> PACKAGES

BUY UP TO TEN PACKAGES FROM STOCK WITHOUT AEC LICENSE

IMMEDIATE  
SHIPMENT

LICENSE EXEMPT

HIGHEST  
GUARANTEED  
RADIOPURITY

\$12.00 for 50 $\mu$ c

\$25.00 for 50 $\mu$ c

Barium Carbonate - C<sup>14</sup>  
Cyanide - C<sup>14</sup> (sodium)  
Acetate - 1 - C<sup>14</sup> (sodium)  
Bicarbonate - C<sup>14</sup> (sodium)  
Formate - C<sup>14</sup> (potassium)  
Benzoic acid - 7 - C<sup>14</sup>  
Palmitic acid - 1 - C<sup>14</sup>  
Urea - C<sup>14</sup>  
Glycine - 1 - C<sup>14</sup>  
Lauric acid - 1 - C<sup>14</sup>  
Acetate - 2 - C<sup>14</sup> (sodium)  
Butyrate - 1 - C<sup>14</sup> (sodium)  
Propionate - 1 - C<sup>14</sup> (sodium)

Formaldehyde - C<sup>14</sup>  
Glycine - 2 - C<sup>14</sup>  
Alanine - 1 - C<sup>14</sup>  
Alanine - 2 - C<sup>14</sup>  
Methionine - CH<sub>3</sub> - C<sup>14</sup>  
Phenylalanine - 3 - C<sup>14</sup>  
Succinic acid - 1 - C<sup>14</sup>  
Succinic acid - 2 - C<sup>14</sup>  
Fructose - C<sup>14</sup>  
Glucose - C<sup>14</sup>


WRITE FOR CATALOG 1056-A



2005 HOPKINS ST. **RESEARCH SPECIALTIES CO.** BERKELEY 7, CALIF.

*new  
instruments  
for infusion  
and retracting  
of liquids*

**FOR GENERAL  
APPLICATION**

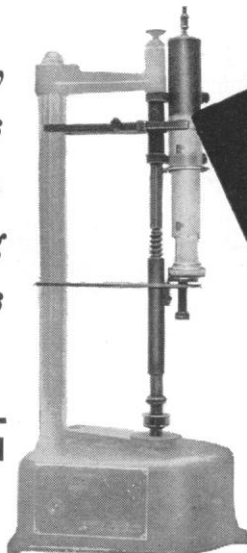

**HERE** is an economical and convenient means for delivering small quantities of liquids at accurately controlled rates.

A threaded shaft, carrying a syringe holder and a pusher, is mounted in place of the regular drum spindle and rotated in the same manner. Syringes are clamped in place, or released by turning a single thumbscrew. The unit is designed to be attached to, and driven by, our Bird Kymograph #70-060. This propeller may be used with equal facility on our older model (four-speed kymograph).

Since any Luer syringe, from 5 ml. to 50 ml. capacity may be used, and since the kymograph drive provides a

## Syringe Driver

choice of five speeds, a wide range of delivery rates is available, as indicated in the following table.

This instrument has clinical applications in anaesthesia, surgery, gynecology, radiology and neuropsychiatry. It is particularly useful for administering small volumes of injectible drugs which are to be given over a period of time.

71-04990 Syringe Driver and Kymograph (less drum and drum shaft) and without syringe. \$156.50 each

71-0499 Syringe Driver only ... \$72.50 each

Approximate Delivery Rates in Milliliters per minute.					
Syringe Capacity	5	10	20	30	50
Speed No. 1	.0046	.0059	.0118	.0157	.024
Speed No. 2	.023	.030	.059	.078	.12
Speed No. 3	.116	.148	.29	.39	0.6
Speed No. 4	.58	.78	1.48	1.96	3
Speed No. 5	2.9	3.7	7.4	9.8	15

### SYRINGE RETRACTOR

Similar to the Bird Syringe Driver, (Catalogue No. 71-0499), but is designed for **withdrawing** samples of blood (or other liquids) at accurately controlled rates.

71-04492—Syringe Retractor and Kymograph (less drum and drum shaft) and without syringe ... \$181.50  
71-04991—Syringe Retractor, complete with change-gears ... \$ 97.50

**PHIPPS & BIRD, INC.**


Manufacturers & Distributors of Scientific Equipment



6th & Byrd Streets - Richmond, Va.

# EXACT CONTROL

**of Moisture Content  
To Improve your Product  
or Protect Your Materials  
or for Processes or Tests**

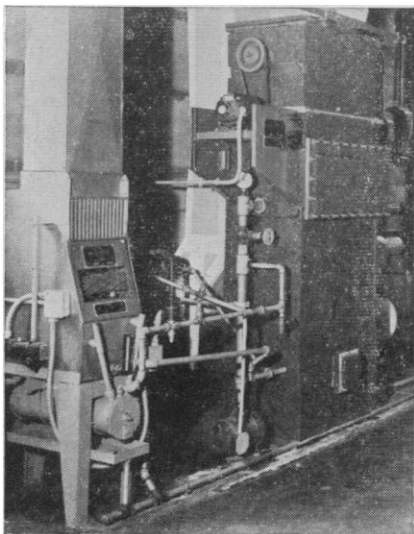

● This Niagara Air Conditioning Method dries air directly and measurably, using a moisture-absorbing liquid spray. It makes humidity control a separate function from lowering or raising temperatures and gives you precise control with thermostats alone; no moisture-sensitive devices are needed. You have simpler, more trustworthy, less expensive control instrumentation. Niagara precise-control installations have the best record for reliability.

Niagara Air Conditioning provides you with any temperature and relative humidity you need. Using "Hygrol" absorbent, it is not expensive to operate, saving the refrigeration commonly used to condense moisture and making re-heat unnecessary in most cases. It gives large capacity with compact, easily-maintained equipment. Ask for descriptive Bulletins No. 112 and No. 121.

## NIAGARA BLOWER COMPANY

Dept. SC-6, 405 Lexington Ave.  
New York 17, N. Y.

District Engineers  
in Principal Cities of U. S. & Canada

## EQUIPMENT NEWS

*The information reported here is obtained from manufacturers and from other sources considered to be reliable. Science does not assume responsibility for the accuracy of the information. All inquiries concerning items listed should be addressed to Science, Room 740, 11 W. 42 St., New York 36, N.Y. Include the name(s) of the manufacturer(s) and the department number(s).*

■ **POWER SUPPLY** for 14-stage multiplier phototubes furnishes sufficient current for a number of tubes. Output is from 600 to 3110 v at currents up to 15 ma. Regulation is  $\pm 0.01$  percent for a 20-percent change in line voltage and  $\pm 0.005$  percent for a load change of 10 ma. Stability is 0.005 percent per hour and 0.05 percent per day. A 1.02-v sample of the output is available at the front panel for monitoring. (John Fluke Manufacturing Co., Inc., Dept. S403)

■ **PULSE GENERATOR** provides repetition rates from 10 cy to 100 kcy/sec, variable advance or delay operation, 0 to 100  $\mu$ sec, variable pulse width from less than 0.1 to 100  $\mu$ sec, and variable-amplitude, low-impedance output. (Electro-Pulse, Inc., Dept. S404)

■ **AIR-SAMPLING KIT** permits detection of toluene diisocyanate and toluene diisocyanate urea vapors in manufacture of polyurethane plastics. Concentrations less than 0.1 ppm are detected. The vapors are detected by hydrolysis to amine and conversion to a diazo amine compound. (Mine Safety Appliance Company, Dept. S395)

■ **PAPER-CHROMATOGRAM SCANNER** is a windowless model suitable for counting  $C^{14}$  and  $S^{35}$ . The chromatogram is mounted on a drum which rotates in front of the detector. Count rate is recorded by a rectilinear-type recording millimeter. The scanner and recorder motions are mechanically related. Chromatograms measuring up to 56 by 3.5 cm are accommodated. (Radiological Service Co., Inc., Dept. S400)

■ **FREQUENCY MULTIPLIER** is designed to reduce the time necessary for measurement of frequency in the range of 390 to 410 cy/sec. Used with electronic counters, the frequency multiplier cuts down by one decade the sampling time required for a given precision. Multipliers for other frequencies can also be supplied. (The Gyrex Corp., Dept. S401)

■ **DIGITAL PRINTER** operates from four-line 1-2-2-4 binary code to print up to 12 digits on standard adding-machine tape. Minimum display time is 0.2 sec. Dimensions are 14 by 8 by 10 in. (Computer Measurements Corp., Dept. S396)

■ **DEMINEERALIZATION UNIT** furnishes water with a resistivity greater than 10 Mohm at rates up to 40 gal/hr. The mixed-bed cation and anion resins are regenerated, seven canisters at a time, in auxiliary equipment. Regeneration requires 1½ hr. (Penfield Manufacturing Co., Inc., Dept. S405)

■ **NEUTRON DETECTOR**, a boron polyester with  $ZnS(Ag)$  activator, measures thermal neutrons in the presence of high gamma flux. Detection efficiency ranges up to 35 percent and can be further increased by the use of enriched boron-10. The detector is supplied in disks 1.2 mm thick and of various diameters. (Nuclear Enterprises, Ltd., Dept. S406)

■ **RECORDING BALANCE** is suitable for a total load of 100 g. For thermal work, the balance is surmounted by a nichrome-wound furnace. Furnace temperatures and loss of weight are recorded, side-by-side, on a twin-pen electronic recorder. A capacitance sensor follows the movement of the balance beam to provide observation of weight. The balance is air damped. Sensitivity may be either 1 mg or 0.1 mg. At the end of each full beam movement, a weight-loading mechanism is actuated. In this way, changes of weight up to 1 g can be followed automatically on the 1-mg sensitivity model. A single-recorder model that records weight against time is also available. (Stanton Instruments Ltd., Dept. S424)

■ **LEVEL SWITCHES** are glass tubing arcs filled with a special electrolyte. One hollow platinum electrode and two solid platinum electrodes make contact with the electrolyte to provide the output signal. The switches can withstand temperatures up to 200°C and operate below -60°C. Level and deviations from level are indicated to within tenths of a degree. (Corning Glass Works, Dept. S413)

■ **TEMPERATURE TRANSDUCERS** for telemetering applications are of resistance type, giving outputs up to 5 v for change of 150°F. Standard units cover the range from -320° to +500°F, with  $\pm 2$ -percent linearity. Special units can be had for use up to 1600°F. Resistances of the units range from 100 to 20,000 ohm. (Arnoux Corporation, Dept. S409)

■ **POWER ABSORBER**, operating at 13,500 w, continuous duty, has a weight of 1 lb per kilowatt absorbed. Air, drawn through circumferential slots by a fan, flows over V-section resistors to dissipate the heat produced. Overload protection is provided. (Sun Electric Corp., Dept. S412)

JOSHUA STERN  
National Bureau of Standards

**SCIENCE** | The weekly magazine of research

June 28, 1957

TO RESEARCH DIRECTORS

It is a source of great encouragement to us that more and more companies are beginning to consult their research departments in regard to advertising. For many years, we have felt that the Research Director could contribute substantially to the promotional activities of industry.

Industry's growing dependence on research has played a decisive role in bringing about this change. Most companies now realize that their futures depend on new applications for their existing products. Because of this, they are anxious to make sure that news of their activities gets to the research scientist.

If you have a voice in your company's advertising policies, you will certainly want to know more about SCIENCE MAGAZINE. Let us show you how SCIENCE can do an effective job of carrying information about your products to research workers in every phase of industry and government.

"Facts about SCIENCE," a new booklet, gives detailed information on circulation and readership. To get your copy, just drop us a line.

SCIENCE  
Room 740  
11 West 42nd Street  
New York 36, New York

Sincerely yours,

*Earl J. Scherago*


Earl J. Scherago  
Advertising Manager

MADE BY



IN WEST GERMANY

# REVOLVER MICRO PROJECTOR

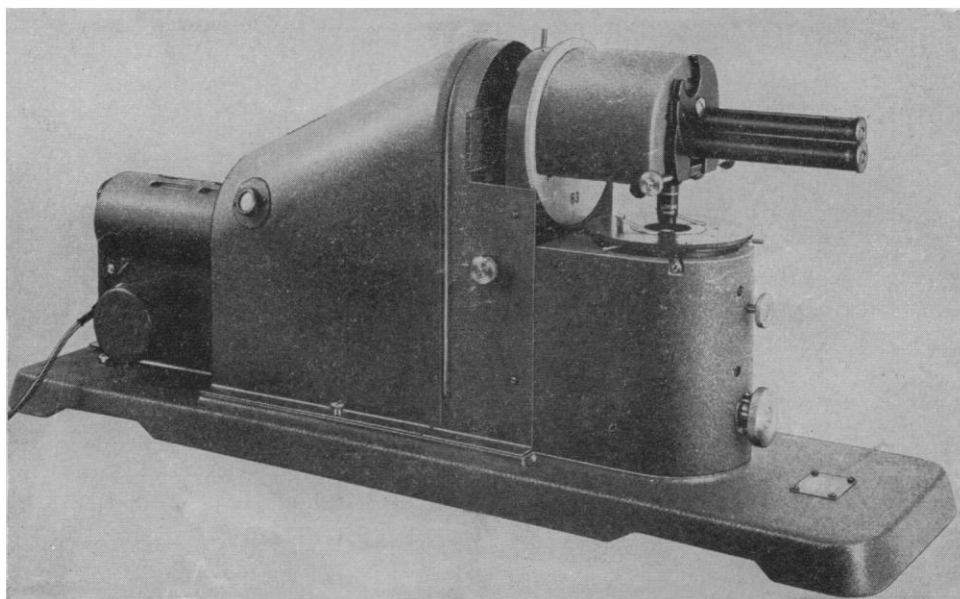

The advantages of micro-projection . . . permitting the showing of microscope slides to a group of scientists or students as well as pointing out specific details in the projected object . . . have not been fully utilized because of the complicated handling of micro-projectors that were thus far available.

With the new Carl Zeiss Revolver Micro Projector apparatus, these difficulties are completely eliminated. Six objectives coupled mechanically to suitable condensers together with special projection eyepieces instantly project an image on the screen from low (macro) up to high magnifications. All objectives are parfocal and the matched condensers provide illumination by the Koehler principle. Thereby best resolution and greatest brightness of images are assured.

Special projection eyepieces guarantee favorable fields of view, even at long projection distances. A fully automatic carbon arc lamp eliminates frequent manual adjustment, so that even untrained operators can easily handle this projector.

The Revolver Micro Projector can be quickly converted into a lantern slide projector for 2 x 2-in. slides by merely swinging a reflecting mirror, a condenser and a projection lens into the path of rays.

*Write for free detailed literature*

**CARL ZEISS, INC.,** 485 FIFTH AVENUE, NEW YORK 17, N.Y.

*Guaranteed uninterrupted repair service*