

New Products

The information reported here is obtained from manufacturers and from other sources considered to be reliable. Neither Science nor the writer assumes responsibility for the accuracy of the information. A coupon for use in mailing inquiries concerning the items listed is included in the post card insert. Circle the department number of the items in which you are interested on this coupon.

■ **GONIOMETER** for calibration of divided circles, polygons, and angle gages, provides direct reading to 0.1 sec of arc. The bearing for the worktable carries a glass-divided circle, and the autocollimating telescope unit also contains an optical system for determining the mean value of the opposite-side circle readings. The table may be rotated relative to the divided circle about an auxiliary center by means of a micrometer spindle engaging a worm wheel. A second autocollimating telescope is mounted on a column carried by the base casting. (Engis Equipment Co., Dept. Sci830, 431 S. Dearborn St., Chicago 5, Ill.)


■ **REGULATED POWER SUPPLY** furnishes independent positive and negative outputs, each capable of being loaded up to 200 ma at 100 volts. The supply uses a Weston cell as voltage reference. Accuracy and stability are said to be better than ± 0.1 percent, long term, for -100 volts. The +100-volt supply can be set to within 1 mv of the negative supply voltage and will remain within 5 mv. Source impedance is less than 0.05 ohm and ripple and noise are less than 15 mv peak-to-peak. (Solartron Electronic Group, Dept. Sci832, Thames Ditton, Surrey, England)

■ **BLOOD FLOW METER** for use during cardiopulmonary bypass is based on the electromagnetic induction principle. The meter is a refinement of the manufacturer's industrial magnetic flow meter. An indicator provides continuous flow indication, an integrator totalizes liters of blood flow during bypass, and a chart record permits postoperative evaluation. Standard range is 0 to 5 lit./min. Accuracy is said to be ± 1 percent of full scale over the entire scale and repeatability ± 0.5 percent of full scale. The flow tube is removable from the meter for sterilization. (Foxboro Co., Dept. Sci838, Foxboro, Mass.)

■ **SEMICONDUCTOR DEVICE TESTER** will test transistors for breakdown voltage, gain over the complete dynamic range, voltage and current saturation characteristics, and leakage current at up to 80 volts. Zener diodes can be tested for breakdown voltage, dynamic impedance at any current up to 1 amp, and drift with temperature or current. Rectifiers can be tested for leakage up to 80 volts and forward-current char-

NOW YOU CAN BUY APPROVED ANTON TRANSISTORIZED SURVEY METERS FOR LABORATORY OR FIELD USE

... Anton instruments assure accurate surveys. The Anton 700 meets the rigid federal OCDM Specification for CDV-700. Ranges .5, 5, 50 MR/HR. Only five (5) conventional flashlight (type D) batteries power its economical, rugged, reliable, experience-tested transistorized circuit. More than 100 continuous hours of life without battery change. Over 50,000 units manufactured to date by quality-controlled "line" producing one unit per minute. New model equipped with easy-to-read $3\frac{1}{2}$ " meter... aural monitoring through headphone. Equipped with long-lived Anton halogen quenched detectors. **ANTON ELECTRONIC LABORATORIES INC.** 1226 Flushing Ave., B'klyn 37, N. Y.

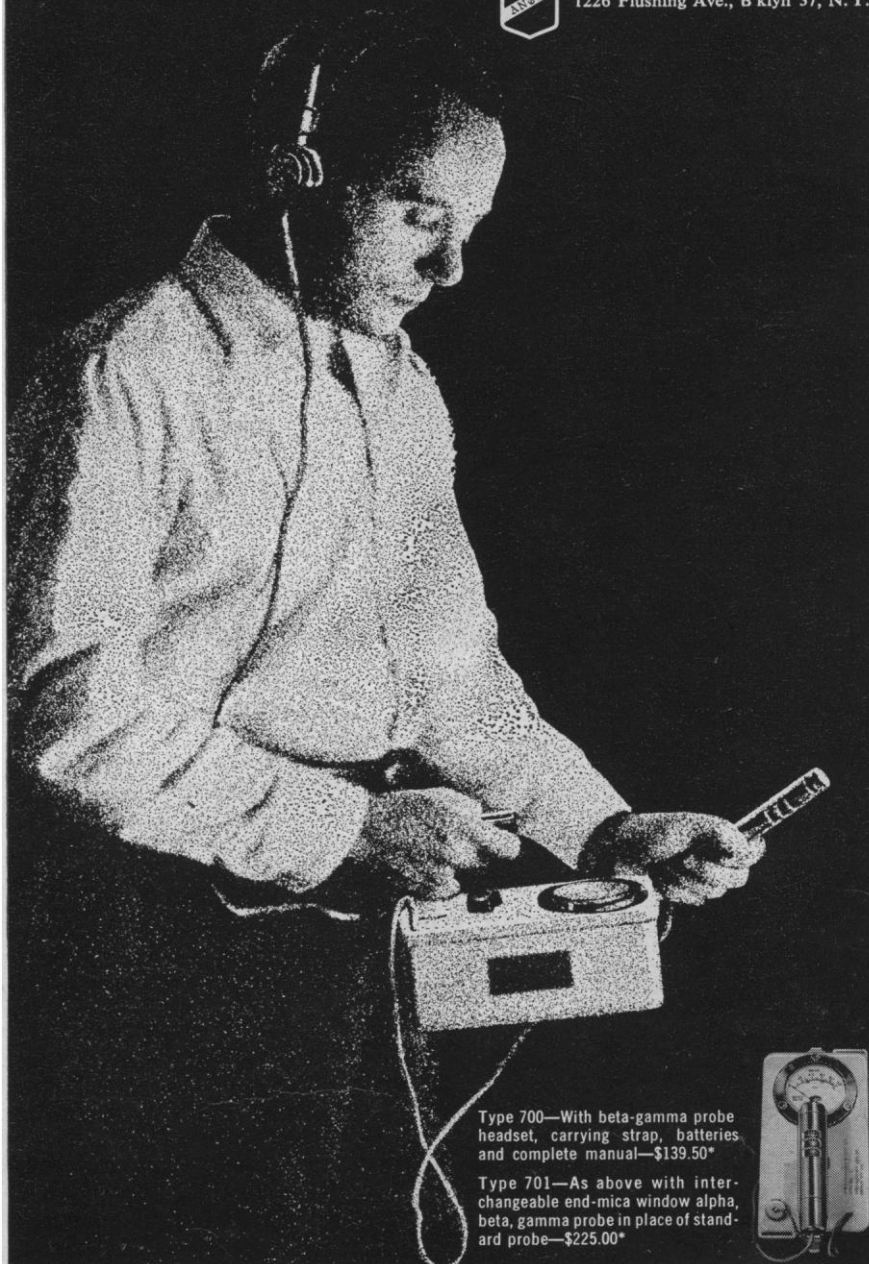

Type 700—With beta-gamma probe headset, carrying strap, batteries and complete manual—\$139.50*

Type 701—As above with interchangeable end-mica window alpha, beta, gamma probe in place of standard probe—\$225.00*

ORDER NOW FOR IMMEDIATE DELIVERY . . . OR SEND FOR ADDITIONAL DATA.
*FOB B'klyn. If payment accompanies order we will ship at our own expense (quantity discounts on request)

acteristics up to 1 amp. Tunnel-diode characteristics of tunneling current, valley current, and forward voltage can be determined. (PRL Corporation, Dept. Sci833, P.O. Box 215, East Brunswick, N.J.)

■ **PRESSURE BALANCE** for calibration of pressure gages provides a pressure range from 1000 to 48,000 lb/in.² in 94 steps of 500 lb/in.², or 50 to 3250 atm in 128 steps of 25 atm. Accuracy is said to be 1 part in 2000. Balance weights are lifted mechanically by a series of levers that permit selection of any combination without stopping the balancing operation. (High Pressure Equipment Co., Dept. Sci843, 1222 Linden Ave., Erie, Pa.)

■ **LEAD SULFIDE PHOTOCONDUCTORS** are Dewar-mounted for operation from room temperature to -196°C . The detecting elements consist of chemically deposited lead-sulfide films with response to $4.5\ \mu$. Specifications quoted are: dark resistance, 0.5 to 5 megohm/square; time constant, 800 to 2000 μsec . A variety of Dewar designs, cell configurations, and immersions is available. All are furnished with fire-sealed, sapphire windows. (Infrared Industries, Inc., Dept. Sci845, P.O. Box 42, Waltham 54, Mass.)

■ **PRECISE LINEAR SCALES** are offered in two types. Type A, available in 150-, 250-, and 500-mm graduated lengths, produced by direct ruling, is said to be accurate to $\pm 0.75\ \mu$. Lines are engraved and etched in glass. Type B, available in 150- and 200-mm graduated lengths, is produced photographically with accuracy said to be $\pm 2.5\ \mu$. English graduations are also available. (David W. Mann Co., Dept. Sci851, Lincoln, Mass.)

■ **RECORDING INSTRUMENT** times short-duration events to milliseconds even at slow chart speeds. Time markings along edge of the chart show time of day any event occurs while sweep of the recording pen across the chart displays duration of the event. Sweep-time scale ranges from 1 sec to 1 hr are available. Standard chart speeds are $\frac{3}{4}$, $1\frac{1}{2}$, 3, 6, and 12 in./hr and in./min. (R. B. Annis Co., Dept. Sci850, 1101 N. Delaware St., Indianapolis 2, Ind.)

■ **COUNT-RATE AND PERIOD METER** is a logarithmic instrument that measures neutron count/min over a six-decade range from 10 to 10^6 count/min. The output reading is available for remote meter and recorder connections. The instrument also provides continuous in-

dication of rate of change of power level during reactor startup and trips an alarm if the reactor period is shorter than a preset interval. (General Electric Co., Dept. Sci852, Schenectady 5, N.Y.)

■ **X-RAY FLUORESCENCE SPECTROMETER** uses an evacuated chamber so that all elements of atomic number above 11 can be analyzed without use of helium atmosphere. Simultaneous analysis of the elements is said to be obtained in about 2 min. Dual sample handling facilities permit sample interchange without breaking vacuum. (Applied Research Laboratory, Dept. Sci853, P.O. Box 1710, Glendale 5, Calif.)

■ **PRESSURE REFERENCE CELL** consists of a pressure storage chamber, a diaphragm, and a sensitive switch. The cell detects equality between an unknown pressure and the reference pressure. Stored pressure ranges from 0.2 to 200 in.-Hg. Cells can be furnished sealed at a given pressure or unsealed. Temperature dependence is about 0.35 percent/ $^{\circ}\text{C}$ and the units must be operated in an ice bath for best performance according to the manufacturer. Precision is said to be $\pm(0.001\ \text{in.-Hg.} + 0.003\ \text{percent of calibrated value})$. Multiple gage calibration is accomplished by unfolding a series of cells and the gages to be calibrated. (Rosemount Engineering Co., Dept. Sci854, 4900 W. 78 St., Minneapolis, Minn.)

■ **SIGNAL GENERATOR** covers the frequency range 1 cy to 1 Mcy/sec. Distortion is said to be 0.2 percent. An output meter and attenuator permit output amplitude to be set to desired value. (Southwestern Industrial Electronics Co., Dept. Sci839, 10201 Westheimer Rd., Houston 27, Tex.)

■ **DECADE RING COUNTER** consists of ten magnetic storage elements connected as a ring counter. Pulses furnished to an input terminal are stored by shifting them along from position to position in the forward mode of operation. Upon receipt of a command signal on a separate "reverse" line, counts are subtracted instead of being added. Decades may be cascaded. Counting rates up to $10^5/\text{sec}$ are accommodated. Reversal time is 10 μsec . (Magnetics Research Co., Dept. Sci855, 255 Grove St., White Plains, N.Y.)

■ **TIME ANALYZER** is an electronic instrument that resolves a time span into up to 40 consecutive intervals and analyzes input events in terms of the number of occurrences within each interval. Duration of the intervals is variable over a wide range. Connection to an appropriate recorder pro-

You are cordially invited to attend

STANDARD'S 2nd PARADE of SCIENTIFIC INSTRUMENTS

*New Laboratory Instruments
New Apparatus and Chemicals
New Techniques—New Ideas*

Demonstrated and displayed by 60 of America's Outstanding Instrument and Apparatus Manufacturers and Chemical Producers . . . and featuring a symposium and lectures by eminent scientists and technicians on instrumentation and methods.

GRAND BALLROOM

HOTEL NEW YORKER

34th Street and 8th Avenue, New York City

Nov. 7, 1960—2 to 9 A. M.

Nov. 8, 1960—11 A. M. to 10 P. M.

Nov. 9, 1960—11 A. M. to 7 P. M.


under the auspices of

STANDARD SCIENTIFIC SUPPLY CORP.

808 Broadway, New York 3, N. Y.

We will gladly furnish tickets upon request

+250° **IN THE LAB--**
use TIME TAPE for best results!

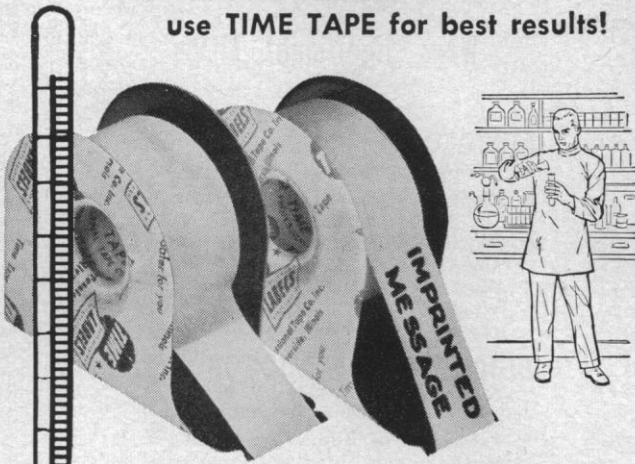

Proven superior by actual use. Here is the toughest, most durable pressure-sensitive tape available. WRITE ON IT! TYPE ON IT! Acid, water, dirt, grease or heat don't affect it! Withstands temperatures from +250° to -70°! A variety of colors available in plain or pre-printed to your specs. Numbers, identification, warning and many other time-saving uses can cut costs and increase efficiency.

For samples and prices write to — Dept. RSL

PROFESSIONAL TAPE CO., INC.
355 Burlington Ave. Riverside, Ill.

TIME LABELS
SELF STICKING
VINYL COATED


new england nuclear

Putrescine-2,3-H³ Dihydrochloride
\$175/5 millicuries

Specific activity:
125 millicuries per millimole

CATALOG ON REQUEST

new england nuclear corp.
575 ALBANY STREET, BOSTON 18, MASS. Liberty 2-5964

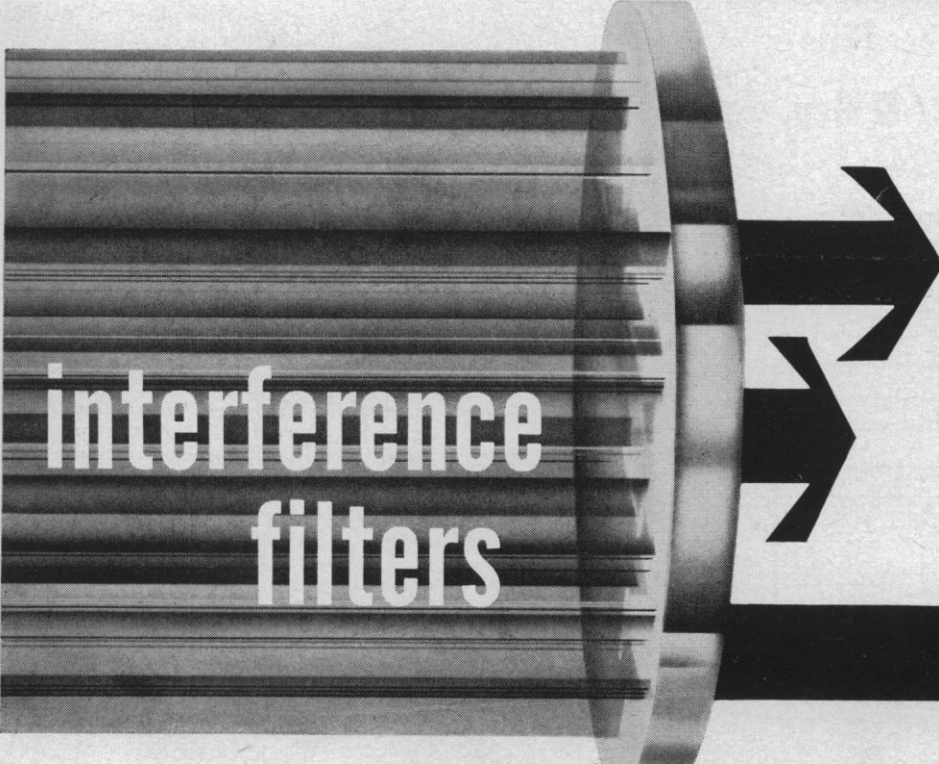

interference filters

Ultraviolet and visible wavelengths.
Finest optical performance available.
Standard sizes 1" x 1" and 2" x 2" —
other sizes and shapes on special order.
Write for brochure X-22.

BA




BAIRD-ATOMIC, INC.

33 university road • cambridge 38, mass.

GLASS ABSORPTION CELLS

made by **KLETT**

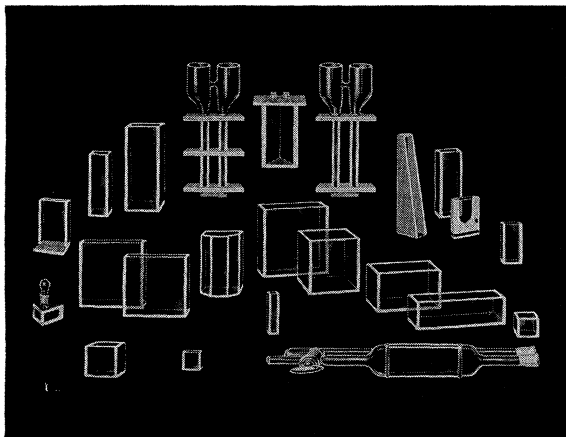

SCIENTIFIC APPARATUS
Klett-Summerson Photoelectric Colorimeters—
Colorimeters — Nephelometers — Fluorimeters—
Bio-Colorimeters — Comparators — Glass Stand-
ards—Klett Reagents.

Klett Manufacturing Co.
179 East 87 Street, New York, New York

LIFE SCIENCE SERIES

New Significant Titles



MYCOLOGY

Consulting Editor: George B. Cummins

- **Illustrated Genera of Imperfect Fungi**
by Barnett, \$4.50
- **Illustrated Genera of Rust Fungi**
by Cummins, \$4.50
- **Illustrated Genera of Wood Decay Fungi**
by Fergus, \$4.00

BIOCHEMISTRY-MICROBIOLOGY

Consulting Editors: Robert H. Burris and
Herman C. Lichstein

- **Principles of Radioisotope Methodology**
by Chase, \$6.00
- **Elementary Biochemistry**
by Mertz, cloth bound \$6.50,
spiral bound \$5.50
- **Nucleic Acid Outlines, Vol. I**
by Potter, \$5.00
- **Behavior of Enzyme Systems**
by Reiner, \$6.50
- **Metabolic Maps, Vol. II**
by Umbreit, \$5.50
- **Manometric Techniques**
by Umbreit-Burris-Stauffer, \$6.50
- **Symposium: Latency and Masking in Viral and Rickettsial Infections**
by Walter-Hanson-Evans, \$4.75

order from
BURGESS PUBLISHING COMPANY

Dept. S1060, 426 S. 6th St., Minneapolis 15, Minn.

Narrow Band Interference Filters

MADE BY


JENAer Glaswerk Schott & Gen.

WEST GERMANY

For the spectral region from 300 to 2,000 m μ .
Transmission up to 60%. Half-value width down to 5 m μ .
Tolerance at peak wave length:
 $\pm 1\%$ for regular quality . . . $\pm 0.5\%$ for precision quality.
—0

AVAILABLE AS

Line Filters • Line Double Filters • Band Filters
Band Double Filters • Wedge Filters • Broad Band Filters

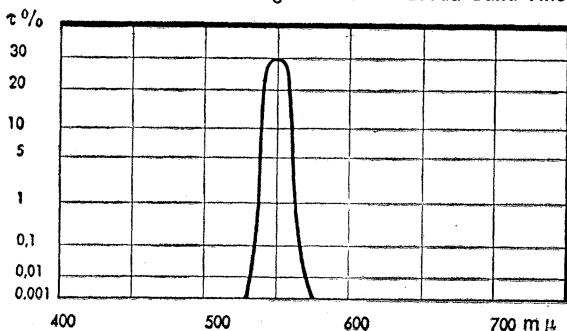

BAND DOUBLE FILTER

Tmax abt. 30%. Half width abt. 16 m μ .

Ratios: Tenth width to half width 1.5, Hundredth width to half width 2, Thousandth width to half width 3.5.

Write for further information

Fish-Schurman Corp., 74 Portman Road, New Rochelle, N.Y.

Fish-Schurman



*no knobs, no wheels,
no tools...*

JUST LIFT SEAT TO DESIRED HEIGHT

What could be simpler or cleaner? Just lift the seat to the desired height. No dirty knobs, wheels or tools to handle. The Ajustrite patented adjusting mechanism is the reason hundreds of thousands of Ajustrite Chairs and Stools are in service today. It's the oldest, the simplest, the fastest. And the most trouble-free—that's why we guarantee it for 10 years!

30-DAY FREE TRIAL No obligation. Prove to yourself the Ajustrite advantages in utility, comfort and economy.

Production TPC-1826

Drafting RUC-2230

AJUSTER
CHAIRS ... STOOLS

AJUSTO EQUIPMENT CO.
Bowling Green, Ohio

vides a distribution of events in time. A total-events counter is also provided. Accuracy depends on the time standard used, either line frequency or external generator. (Grason-Stadler Co., Dept. Sci846, West Concord, Mass.)

■ **PULSE GENERATOR** produces positive or negative pulses of amplitude up to 20 volts. Line changes between 90 and 125 volts change output amplitude less than 0.04 percent. Two pulse shapes are provided, one with 10 μ sec rise and 250 μ sec decay, the other with 0.25 μ sec rise and 2 μ sec decay. Linearity is 0.1 percent. Voltage ranges from 0 to 20, 0 to 10, 0 to 1, 0 to 0.1 and 0.01 can be divided into 1000 increments by means of a ten-turn precision potentiometer. (Interstate Electronics Corp., Dept. Sci847, 707 E. Vermont Ave., Anaheim, Calif.)

■ **VIBRATING-REED CAPACITANCE MODULATOR** is said to permit measurement of currents as low as 10^{-10} amp. The vibrating plate is driven by an alternating magnetic field. Drift is said to be within ± 0.2 mv/day. Models are available with quartz or with ceramic insulation and with 500 or 120 cy/sec drive frequency. (Stevens-Arnold Inc., Dept. Sci844, 7 Elkins St., South Boston 27, Mass.)

■ **NOISE SOURCE** furnishes output frequencies over the range 30 cy to 300 kcy/sec with uniformity to ± 2 db when used with the proper amplifier circuits. No a-c power is used. Output voltage is 0 to 10 mv r.m.s. into a 1000-ohm load. The device is transistorized; its dimensions are 1½ in. square by 3 in. (Raytheon Co., Dept. Sci848, 55 Chapel St., Newton, Mass.)

■ **DOUBLE SCALER** provides two scales of 10^4 each followed by a four-digit electrically reset register. The two sections may be operated individually or simultaneously. Resolving time is said to be 0.8 μ sec. Provision is made for remote control of count and reset operations. (Radiation Instrument Development Laboratory, Dept. Sci856, 61 E. North Ave., Northlake, Ill.)

■ **VELOCITY SERVO** accepts d-c signals varying between ± 10 volts and drives a potentiometer so that speed is directly proportional to the d-c signal. The device contains a solid-state amplifier, a servo motor, a gear train, and a potentiometer-switch combination. The potentiometer has four electrically isolated wipers spaced 90 deg apart and the switch has four wipers riding on an alternately conducting and nonconducting surface. Dimensions are 1½ by 1½ by 3 in. (Spectrol Electronics Corp., Dept. Sci862, 1704 S. Del Mar Ave., San Gabriel, Calif.)

■ **CARDIAC PHONOCATHETERS** are available in two models. Model 191 is a single-lumen phonocatheter, 150 cm long and 2 mm in diameter, for acoustical pickup only. Model 192 is a double-lumen catheter, 150 cm long and 3 mm in diameter, for acoustical and pressure pickup and for fluid samples. Base diameter of the sample lumen is approximately 1 mm. A self-powered preamplifier that will feed standard electrocardiographic equipment is available for use with the catheters. (American Electronic Laboratories, Dept. Sci857, 121 N. 7 St., Philadelphia 6, Pa.)

■ **X-RAY SOURCE** uses an active element, $\text{Sr}^{90}/\text{Y}^{90}$, distributed in a matrix of target material to maximize x-ray production in the desired range. The unit is in the form of a stainless-steel capsule doubly sealed by shielded arc welding. X-rays produced are in the 100-kv range. (U.S. Nuclear Corp., Dept. Sci865, P.O. Box 208, Burbank, Calif.)

■ **TRANSFER-FUNCTION ANALYZER** permits plotting of transfer characteristics of a control system with a conventional X-Y recorder. By turning the dial of the instrument, continuous plotting of

FOR TISSUE CULTURE

NEW! NEWBORN AGAMMA CALF SERUM

An especially processed serum containing exceedingly high content of alpha globulin (37 to 40% of the total protein content) and 7 to 10% beta globulin. Gamma globulin chemically removed by fractionation techniques. Carefully processed to preserve all other proteins and growth components. Every lot biologically tested and rigidly assayed by moving boundary electrophoresis before release. Non-toxic. Recommended as a replacement for Fetal Calf Serum in many tissue culture procedures, including preparation of Puck's media.

Supplied as ready-to-use liquid (sterile) or stable, freeze-dried powder (non-sterile). Liquid product available in 100 cc size. Dried product supplied in 7 gm size (equivalent to 100 cc finished serum) or 42 gm size (equivalent to 600 cc finished serum).

OTHER ADDITIONS

Hyland's rapidly expanding tissue culture line now includes the following components for use in Puck's media: *Puck's Medium N16* (without l-glutamine), 100 cc
Puck's Saline F, 100 cc
NCTC 109 Medium, 100 cc
and *Fetal Calf Serum, Liquid*, 30 cc and 100 cc.

CELL ADHERENCE TO GLASS

Comments continue to be received on the high quality of Hyland's regular Calf Serum. It has unusually high content of alpha globulin (28 to 29% of the total protein content). Alpha globulin contains the fetuin component, which is required for growth, and in its presence most cells adhere to glass and assume a flattened appearance. Hyland Calf Serum is supplied in either liquid or freeze-dried form, in 30 cc and 100 cc sizes.

Write today for a listing of the complete Hyland Tissue Culture line. In addition to the products already mentioned, we offer a wide selection of liquid and dried products in a practical variety of sizes. Our line embraces Serums and Serous Fluids, Embryo Extracts and Ultrafiltrates, Balanced Salt Solutions, Synthetic Media and special formulations.

The Hyland Tissue Culture Laboratory is always at your service and welcomes your inquiries about special formulas or products you would like added to our line.



HYLAND LABORATORIES
4501 Colorado Blvd.,
Los Angeles 39,
California

FREE ^{S&S} Reference Sheets on Selectacel ION EXCHANGE CELLULOSES

for use in chromatographic columns

New Selectacel Ion Exchange Celluloses have remarkable properties when used with ionic and colloidal materials of high molecular weight.

Such applications include—

- ENZYMES
- LIPIDS
- PROTEINS
- NUCLEIC ACIDS
- HORMONES

These materials produce separations that far exceed what usually can be accomplished alone by ion exchange resins, chromatography, electrochromatography, or electrophoresis.

There are several kinds of Selectacel Ion Exchange Celluloses:

ANION EXCHANGERS

Type	Grade	Capacity meq/g
DEAE (Diethylaminoethyl Cellulose)	Standard 20 40	0.9

Separation and purification of proteins, peptides, enzymes, hormones and related materials.

Type	Grade	Capacity meq/g
ECTEOLA (Epichlorohydrin triethanolamine)	Standard 20 40	0.3

Separation and purification of viruses.

CATION EXCHANGERS

Type	Grade	Capacity meq/g
CM (Carboxymethyl Cellulose)	Standard 20 40	0.7

Weakly acidic—most effective at pH's slightly above 4.

Type	Grade	Capacity meq/g
P (Cellulose Phosphate)	Standard	0.9

Bifunctional—containing both strongly acidic and weakly acidic groups. Relatively high exchange capacities.

Send for these new free Selectacel Reference Sheets today—no obligation of course.

Carl Schleicher & Schuell Co.
Keene, New Hampshire
Department S-10

Send FREE Selectacel Reference Sheets.

NAME _____

COMPANY _____

ADDRESS _____

CITY _____ STATE _____

Selectacel is manufactured by Brown Company and exclusively packaged and distributed for laboratory use by S & S.

Nyquist diagram can be achieved from 0.3 cy to 3 key/sec in type 308A and from 30 cy to 300 key/sec in type 308B. Both the in-phase and the quadrature components of an unknown signal, either servo frequency or modulated carrier, are indicated simultaneously by two center-zero meters. Input impedance is 3 megohms shunted with 20 pf. Sensitivity is 0.3 volt r.m.s. full scale. Accuracy is said to be ± 3 percent of full scale. Output signal for the recorder is ± 0.25 volt maximum. (Ad-Yu Electronics Lab., Dept. Sci858, 249-259 Terhune Ave., Passaic, N.J.)

■ PULSE POWER CALIBRATOR for the X-band covers the frequency range 8500 to 9600 Mcy/sec. Power is measured above the level of 0.5 mw with accuracy said to be ± 0.5 db. A reference level is established each time the equipment is used and power is read directly. (General Communication Co., Dept. Sci841, 667 Beacon St., Boston 15, Mass.)

■ DIFFERENTIAL VACUUM-TUBE VOLT-METER is said to be capable of ± 1 percent accuracy throughout the scale. Full-scale ranges of the center-zero instrument are ± 0.3 , 1.0, 3.0, 10, 30, and 100 volts d-c. Input impedance is 20 megohms for single input and 40 megohms for differential input. The instrument can also be used as a cathode follower with open circuit gain of 0.85 and output impedance 1000 ohms. (Decker Corp., Dept. Sci-859, 45 Monument Rd., Bala-Cynwyd, Pa.)

■ ABSORBERS FOR MOSSBAUER EFFECT, specifically for the 14-kv photon from Fe^{57} , consist of a metallic iron film, 2 to 4 mg/cm² thick, enriched approximately 78 percent in stable Fe^{57} , electrodeposited on one side of a beryllium disk 1 to 3 in. in diameter and 0.02 to 0.03 in. thick. An acrylic coating protects the iron film from oxidation. Dimensions and enrichment can be varied to individual requirements. (Nuclear Metals, Inc., Dept. Sci861, Concord, Mass.)

■ STEREOSCOPIC TELEVISION SYSTEM consists of two closed-circuit television cameras, two monitors, two camera control units, and a polarized optical system. The optical system presents the overlapping images from each camera on a single viewing plane with one image polarized horizontally and the other polarized vertically. Observation through glasses or a viewing hood provides three-dimensional picture presentation. The standard system employs 14-in. monitors but other sizes from 8 to 27 in. can be supplied. (Cohu Electronics, Inc., Dept. Sci867, 5725 Kearny Villa Rd., San Diego 11, Calif.)

New Pergamon Books THE RELAY PROTECTION OF HIGH VOLTAGE NETWORKS

G. I. Atabekov

This is a theoretical monograph covering electrical protective gear. It is an exposition of the methods of theoretical analysis, which will enable the reader to apply and develop these methods by himself in practice, and is the essence of a lifetime's study in this field. Two adjacent disciplines are combined in this work—namely, the technique of relay protection and the theory of the calculation of short circuits—which are treated separately. A unique work, invaluable to western scientists. 564pp. \$14.00

MECHANICAL WAVE GUIDES

M. R. Redwood

The author's aim is to present a thorough theoretical treatment of the fundamental physics describing the propagation of mechanical waves in solid cylinders and plates. Such an account is not available in the scientific literature at present; on the contrary much confusion exists and many of the most recently published papers only add to that confusion. 250pp. \$9.00

ADVANCES IN VACUUM SCIENCE AND TECHNOLOGY

Proceedings of the First International Congress on Vacuum Techniques, Namur, Belgium Edited by E. Thomas

VOL. 1. FUNDAMENTAL PROBLEMS IN VACUUM TECHNIQUES: ULTRA-HIGH VACUUM

VOL. 2. VACUUM SYSTEMS APPLICATIONS IN VARIOUS SCIENCES AND TECHNIQUES.

The authoritative proceedings, which form a valuable record of the 156 papers presented by specialists of world-renown on a wide range of subjects in the field. 824pp. Set, \$30.00

PROBLEMS OF LOW TEMPERATURE PHYSICS AND THERMODYNAMICS

The proceedings of the meeting held at Delft, of Commission 1 of the International Institute of Refrigeration, at which 48 papers were presented. The general subjects covered were: Cryogenic apparatus, thermometry, the disturbed crystal lattice, transport phenomena in liquids and gases. 344pp. \$11.50

MILLIMICROSECOND PULSE TECHNIQUES (Second Revised Edition)

International Series of Monographs on Electronics and Instrumentation I. A. D. Lewis and F. H. Wells

The book is devoted to a consideration of basic circuit elements and pieces of equipment of universal application. Details of specific applications, mostly in the field of nuclear physics instrumentation, are also given. 417pp. \$8.50

catalog sent on request



PERGAMON PRESS

122 East 55th St.

New York 22, N. Y.

■ **ELECTRONIC VOLTMETER** features accuracy said to be ± 1 percent of measured value from 1 mv to 250 volts and from 20 cy to 20 kcy/sec. Accuracy over the wider range to 1000 volts and from 10 cy to 250 kcy/sec is said to be ± 2 percent. Indication is logarithmic. Input impedance is 2 megohms shunted by 15 pf, except on the lowest scale, when the shunting capacitance is 25 pf. (Ballantine Laboratories, Dept. Sci863, Boonton, N.J.)

■ **PAPER-TAPE TO MAGNETIC-TAPE CONVERTER** operates at a speed of 150 characters per second. Components are a photoelectric reader and a magnetic-tape writing unit. Input tape may be 11/16, 7/8, or 1 in. wide. Paper tape codes whose information content does not exceed six bits per character position may be converted. Output is 7-track, 200-character-per-inch magnetic tape. (International Business Machines Corp., Dept. Sci864, 112 E. Post Rd., White Plains, N.Y.)

■ **RECORDER** of potentiometer type has full-scale sensitivity of 1.0 mv and response time less than 0.6 sec for full travel of chart 9.5 in. wide. Chart speeds 1/2, 1, 2, 4, or 8 in./min are selected by gear-shift levers, and a switch changes set speed from inches per minute to inches per hour. Electrical zero can be set anywhere on the chart. (Fisher Scientific Co., Dept. Sci 868, 711 Forbes Ave., Pittsburgh, Pa.)

■ **AEROSOL-PARTICLE COUNTER** detects particles in a suitably defined stream by light scattering. Scattered light from individual particles is detected by a multiplier phototube whose pulse output is sent to a pulse-height analyzer. The pulse signals are analyzed into 15 channels. Particle count in each channel is indicated visually on decade counters. The channels may be examined for 0.3-, 1-, 3-, or 10-min intervals with automatic scan cycle in all channels. Any of the channels may be included or excluded. (Royco Instruments, Dept. Sci869, 365 San Antonio Rd., Mountain View, Calif.)

■ **DIGITAL CLOCKS** indicate time to 23 hr, 59 min, 59 sec. Twelve-hour clocks are also available. Two modes of operation are provided. In one, external equipment, such as digital counters, controls the print rate, time being printed simultaneously with other data. In the second mode, the digital clocks control the timing of readings. Selectable rates are 1 reading per second, 6 or 1 reading per minute, or 6 or 1 reading per hour. (Hewlett-Packard Co., Dept. Sci866, Palo Alto, Calif.)

JOSHUA STERN

National Bureau of Standards,
Washington, D.C.

21 OCTOBER 1960

Lourdes

VACU-FUGE

FIRST...

to **SPIN**

- 1500 ml. at 60,000xG
- 3300 ml. at 33,000xG

with **AUTOMATICALLY**
CONTROLLED TEMPERATURES
down to **-20°C**

Also spins
800 ml. at 61,500xG



- Temperature range -20°C to 40°C
- Patented "Roto-Air" refrigeration system
- 1-HP Universal motor
- High-Vacuum pump—evacuates chamber in only two minutes
- 800 ml. (16 x 50 ml.) at 61,500 x G
- Slant-O-Matic control panel
- Fully Automated with push-button operation
- Electro-dynamic brake
- Automatic self-centering drive
- Exclusive Flex-O-Matic rotor support system
- One year warranty



**ULTRA
SUPERSPEED
REFRIGERATED
VACU-FUGE***

with exclusive
SLANT-O-MATIC KEYBOARD

Model
VA-2

*Vacu-Fuge... a coined name by Lourdes Instrument Corp., denoting superspeed centrifuges operating under vacuum.

The most versatile, superspeed vacuum centrifuge ever offered. Accommodates six interchangeable rotors. Designed for large or small volume, high or low force centrifugation. New patented refrigeration design and other exclusive

features give performance that far exceeds anything previously available. Write today for Bulletin VA-2.

VA-2 speeds your work safely and dependably. Built for years of rugged service.

MAIL COUPON TODAY

LOURDES INSTRUMENT CORP., Div. of Labline, Inc., 53rd St. & First Ave., Brooklyn 32, N.Y.

Please send me VACU-FUGE Bulletin VA-2 Dept. SC-10A

Name

Title

Activity

Address


City Zone State



The "FINGERPRINT" Apparatus


Consisting of

Large Tank Paper Electrophoresis

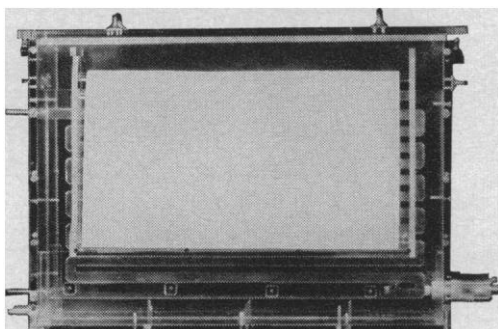

- Internal radiator for circulating cold water
- Includes 2 platinum electrodes
- Baffle plates prevent bubbling under paper
- Safety switches to turn off power when cover is removed
- Dimensions: 24" L, 17" H, 12" W.

High Voltage Power Supply

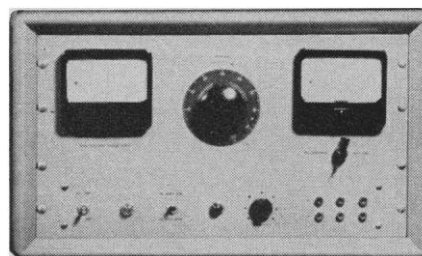

- Output Voltage 0-2000 Volts DC continuous-ly variable
- Output Current 150 milliamperes
- 2 DC Meters 0-2000 V. and 0-150 ma
- Output Termination 3 voltage outputs available from front of unit—positive and negative terminals . . . each output individually monitored for current.

also available . . . Nuclear Accessories Catalog

SERVONUCLEAR CORP.


28-21 Astoria Blvd.

YE. 2-3353

Long Island City 2, N.Y.

Ten years from now you'll be glad you bought Graf-Apsco

THE ORIGINAL "SAFETY FEATURE" MICROSCOPE

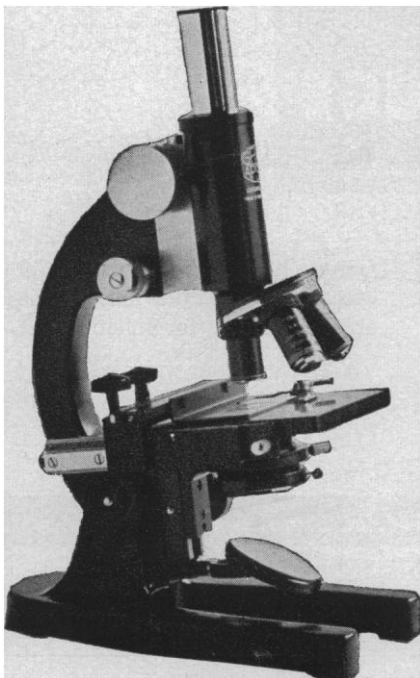

For Bacteriology and Medicine
Model GKM3

\$231.30 each.

in quantities of 5 or more
\$257 each list price

SHIPPED ON TWO WEEKS APPROVAL

If you do not agree that Graf-Apsco microscopes represent the greatest value and highest quality

RETURN AT OUR EXPENSE—
NO OBLIGATION

EXACTLY the same OBJECTIVES on all models

EXACTLY the same FINE ADJUSTMENT on all models

EXACTLY the same STAND on all models

EXACTLY the same NOSE PIECE and HIGH QUALITY WORKMANSHIP on all models

We have only ONE quality—the HIGHEST on ALL Graf-Apsco Microscopes.

Write for our complete catalog showing all Graf-Apsco models as well as popular ZEISS microscopes, and

MAGNIFIERS
DISECTING INSTRUMENTS
MICRO SLIDES — COVER GLASSES
INSECT PINS


Microscope Repair Service

THE GRAF-APSCO CO.

5868 BROADWAY
CHICAGO 40, ILL.



CHICAGO U.S.A.

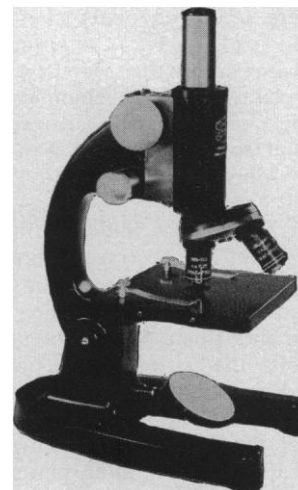

For General Biology
Model GB2A

\$105.30 each.

in quantities of 5 or more
\$117 each, list price

DIRECTORY OF ADVERTISED PRODUCTS

Classified in the following pages are the products advertised in *Science* in the issues from 2 October 1959 through 7 October 1960. This list is intended to aid laboratory workers in finding the manufacturers of all types of laboratory equipment and supplies. On page 1202 there is a list of companies that advertised in "The Market Place" section during the period 2 October 1959 through 7 October 1960. An index of advertisers in this issue appears on page 1204.

ABSORPTION CELLS

Beckman Instruments, Inc., Scientific and Process Instruments Div.

1960: 4 Mar., 628; 15 Apr., 1068; 29 July, 305

Klett Manufacturing Co.

1959: 2 Oct., 867; 9 Oct., 931; 16 Oct., 988; 30 Oct., 1202; 6 Nov., 1269; 13 Nov., 1347; 27 Nov., 1486; 11 Dec., 1665

1960: 8 Jan., 115; 15 Jan., 165; 22 Jan., 243; 5 Feb., 368; 12 Feb., 425; 19 Feb., 545; 26 Feb., 618; 4 Mar., 676; 18 Mar., 843; 1 Apr., 997; 29 Apr., 1325; 13 May, 1452; 20 May, 1552; 27 May, 1626; 10 June, 1746; 24 June, 1896; 1 July, 47; 15 July, 159; 22 July, 254; 29 July, 305; 5 Aug., 369; 19 Aug., 477; 9 Sept., 686; 16 Sept., 747; 23 Sept., 850; 30 Sept., 905

ACCELERATORS, VAN DE GRAFF

High Voltage Engineering Corp.

1960: 29 Apr., 1284; 20 May, 1490

AIR POLLUTION DETECTION UNIT

Central Scientific Co.

1960: 9 Sept., 684

AMPLIFIERS

American Electronic Laboratories, Inc.

1959: 4 Dec., 1581

1960: 22 Jan., 233; 18 Mar., 778; 22 Apr., 1226

Beckman Instruments, Inc., Scientific and Process Instruments Div.

1960: 9 Sept., 683

Sanborn Co., Medical Div.

1960: 5 Feb., 371

Radiation Instrument Development Laboratory, Inc.

1960: 23 Sept., 847

Technical Associates

1960: 22 July, 247

ANALYZERS

Beckman Instruments, Inc., Scientific and Process Instruments Div.

1959: 6 Nov., 1212

1960: 1 Jan., 4; 19 Feb., 453; 18 Mar., 785; 20 May, 1471

Central Scientific Co.

1960: 27 May, 1626; 7 Oct., 973

Coleman Instruments, Inc.

1960: 19 Feb., 462; 18 Mar., 765; 29 Apr., 1281; 23 Sept., 766

Fisher Scientific Co.

1959: 13 Nov., 1350

Harvard Apparatus Co., Inc.

1959: 4 Dec., 1605

Packard Instrument Co., Inc.

1959: 23 Oct., 1041; 11 Dec., 1628

1960: 22 Jan., 196; 19 Feb., 478

Philips Electronics, Inc.

1959: 9 Oct., 884

Scientific Glass Apparatus Co., Inc.

1960: 24 June, 1895

ANALYZERS, PULSE HEIGHT

Pickering X-Ray Corp.

1960: 22 Apr., 1151; 15 July, 107; 23 Sept., 775

Radiation Instrument Development Laboratory, Inc.

1960: 19 Feb., 473; 23 Sept., 847; 7 Oct., 964

Technical Associates

1960: 18 Mar., 865; 20 May, 1563; 22 July, 247

Technical Measurement Corp.

1959: 9 Oct., 894; 23 Oct., 1048; 20 Nov., 1380; 4 Dec., 1532

1960: 8 Jan., 70; 4 Mar., 632; 22 Apr., 1162; 17 June, 1778; 15 July, 112; 26 Aug., 516; 7 Oct., 922

Victoreen Instrument Co.

1960: 17 June, 1755

ANIMALS, EXPERIMENTAL

Charles River Breeding Laboratories, Inc.

1960: 7 Oct., 973, 974

Colorado Serum Co.

1959: 23 Oct., 1132; 13 Nov., 1363; 4 Dec., 1597

1960: 15 Jan., 165; 19 Feb., 537; 18 Mar., 857; 22 Apr., 1226; 9 Sept., 681

AUTOCLAVES

American Sterilizer Co.

1960: 19 Feb., 443

Wilmot Castle Co.

1960: 22 Apr., 1134; 17 June, 1762

BALANCES, ANALYTICAL

Brinkmann Instruments, Inc.

1959: 23 Oct., 1141

1960: 16 Sept., 751; 23 Sept., 770; 30 Sept., 905; 7 Oct., 917

Central Scientific Co.

1960: 22 Jan., 532; 29 Apr., 1325; 19 Aug., 489; 9 Sept., 680

Exact Weight Scale Co.

1959: 23 Oct., 1111

1960: 19 Feb., 535; 18 Mar., 841; 22 Apr., 1233; 17 June, 1817; 26 Aug., 566

Harshaw Chemical Co.

1960: 29 Apr., 1326; 8 July, 96; 16 Sept., 746

Mettler Instrument Corp.

1959: 23 Oct., 1022; 4 Dec., 1586

1960: 19 Feb., 456; 18 Mar., 779; 20 May, 1484; 23 Sept., 776

Microtech Services Co.

1959: 2 Oct., 872

New York Laboratory Supply Co., Inc.

1960: 22 Apr., 1241

NEW SHARP FLAME SURFACE-MIXED GAS-OXYGEN HAND TORCH



Flame range—hard glass, 3mm to 45mm. Operates on low pressure city gas—natural, mixed, propane, hydrogen. For hard glass (Borosilicate), quartz, silver soldering.

Hotter and lighter than conventional hand torches, the surface-mixing SHARP FLAME has phenomenal range—from tiny flame to a wide, long fire. One tip for all flame sizes—can be rotated—silent burning. Won't blow out—can't even be shaken out—and can't flash back. Overall length 11"—weight 7½ oz.

Price
\$35.00



● At your laboratory dealer or write:

Cut-away shows how gas and oxygen are separated up to burner face, producing flame performance impossible with premixed fuels. (Not illustrated, but also available: hand torch holder—insert and remove with a twist of the wrist.)



BETHLEHEM

Apparatus Company, Inc.
HELLERTOWN, PENNSYLVANIA

Books on Science from Philosophical Library

ANALOGUE AND DIGITAL COMPUTERS

by A.C.D. Haley and W.E. Scott. This basic survey for electrical engineers covers number representation, circuit elements, input and output equipment, programming and machines. Illustrated. \$15.00

MODERN ELECTRONIC COMPONENTS

by G.W.A. Dummer. A comprehensive summary of the characteristics of the more commonly used electronic components and their behavior under normal stress conditions. \$15.00

ELECTRONIC BUSINESS MACHINES

Edited by J.H. Leveson. Experts in design, installation and application discuss the practical aspects of these machines, including descriptions of latest equipment, punched cards and tapes. \$15.00

ELECTRONIC COMPUTERS: Revised Edition

by T.E. Ivali. Extensively revised, the emphasis is on digital and analogue computers, their circuitry, construction and application, with special emphasis on automation and control systems. \$12.00

DICTIONARY OF AERONAUTICAL ENGINEERING

by J.L. Nayler. Defines the latest terminology in aerodynamics, aero engines, electrical and electronic engineering, helicopters, jets, propellers, rockets and V.T.O.L. aircraft. Illustrated. \$10.00

AEROSPACE DICTIONARY

by Frank Gaynor. Introduction by Wernher von Braun. Up-to-the-minute information on the many phases of rocketry and astronautics. Includes all abbreviations for missiles and various vehicles, plus descriptions of U.S. and U.S.S.R. missiles. \$6.00

THE UPPER ATMOSPHERE

by H.S.W. Massey and R.L.F. Boyd. An authoritative account of the phenomena studied during the International Geophysical Year, including aurorae, cosmic rays, meteors, ionization, radio absorption, spectographic devices and balloons. 27 plates; line drawings; index. \$17.50

CLASSICS IN SCIENCE

Edited by E.N. da C. Andrade. A cohesive presentation of scientific ideas from the writings of Aristotle, Newton, Lavoisier, Darwin and many others. \$6.00

CLASSICS IN BIOLOGY

Edited by Sir S. Zuckerman. Concerned with the process of evolution, this volume presents writings by Huxley, Pasteur, Darwin, Mendel, Lister, Fleming and others. Biographical notes, glossary and index. \$6.00

DICTIONARY OF MECHANICAL ENGINEERING

by Alfred del Vecchio. Prime definitions in architecture, automatic controls, engineering mechanics, electricity, heat treatment of metals, welding, etc. Illustrated. \$6.00

TRANSFORMERS AND GENERATORS FOR POWER SYSTEMS: THEIR BEHAVIOR, CAPABILITIES AND RATING

by R. Langlois-Berthelot. A detailed examination of the great progress now being made in this field in America, France and Britain. \$12.00

ENGINEERING MATHEMATICS

by J. Blakey and M. Hutton. Ample covers the pure mathematics required for a degree in engineering—also providing invaluable aid to engineers and advanced students. Illustrated. \$10.00

MATHEMATICS REFRESHER

by Kurt Wolter. An indispensable review book for all practising engineers and students. Illustrated. \$3.75

CHEMISTRY OF NUCLEAR POWER

by J. K. Dawson and G. Long. An account of the extensive part played by chemists in the development of nuclear power. \$10.00

NUCLEAR POWER PLANT

by E. Oppenshaw Taylor. A survey of the fundamental ideas underlying nuclear power generation. \$7.50

NEUTRON DETECTION

by W. D. Allen. A comprehensive study of principles and standards, instruments and applications of neutron detection. Extensive bibliography. \$10.00

PROPERTIES OF MATTER

by F. C. Champion and N. Davy. An enlarged edition of a standard text; the subject re-orientated from a philosophical point of view to atomic interpretations. \$10.00

ATOMIC TERMINOLOGY

English—German—French—Italian

Edited by Lore Lettenmeyer. A dictionary of essential terms in atomic and nuclear physics, and associated fields. \$6.00

You can expedite shipment by enclosing remittance

PHILOSOPHICAL LIBRARY

15 East 40th Street, New York 16, N.Y.

Sauter, August, of New York, Inc.

1959: 23 Oct., 1134; 13 Nov., 1348
1960: 19 Feb., 540; 18 Mar., 882; 22 Apr., 1247; 17 June, 1826; 26 Aug., 554
Standard Scientific Supply Corp.

1959: 23 Oct., 1128

Stoelting, C. H., Co.

1960: 22 July, 245; 26 Aug., 563

Torsion Balance Co.

1959: 23 Oct., 1019

1960: 19 Feb., 463; 22 Apr., 1143; 20 May, 1474; 22 July, 181; 26 Aug., 515

Welch, W. M., Manufacturing Co.

1960: 5 Feb., 367

BALANCES, ANIMAL

Exact Weight Scale Co.

1959: 23 Oct., 1111

1960: 19 Feb., 535; 18 Mar., 841; 22 Apr., 1233; 17 June, 1817; 26 Aug., 566

BEAKERS

LaPine, Arthur S., and Co.,

1960: 20 May, 1550

Nalge Co., Inc.

1960: 20 May, 1564; 17 June, 1824; 22 July, 248

BOOKS AND JOURNALS

Academic Press

1960: 22 Apr., 1230

Addison-Wesley Publishing Co., Inc.

1960: 22 Apr., 1240

Annual Reviews, Inc.

1959: 2 Oct., 872; 23 Oct., 1121; 6 Nov., 1271; 4 Dec., 1589

1960: 8 Jan., 117; 19 Feb., 531; 18 Mar., 844; 22 Apr., 1243; 13 May, 1457; 17 June, 1823; 22 July, 233; 5 Aug., 369; 2 Sept., 627; 7 Oct., 972

ARTIA, Prague, Czechoslovakia

1960: 15 July, 159

Baker, J. T., Chemical Co.

1960: 12 Feb., 428

Basic Books

1959: 16 Oct., 985

1960: 19 Feb., 528; 22 Apr., 1246; 7 Oct., 916

British Information Services

1959: 23 Oct., 1126; 4 Dec., 1594

1960: 19 Feb., 552

Burgess Publishing Co.

1960: 22 Apr., 1226; 22 July, 254; 26 Aug., 571

California Academy of Sciences

1960: 19 Feb., 533

Cambridge University Press

1960: 22 Apr., 1222

Cattell, Jaques, Press, Inc.

1960: 25 Mar., 943

Consultants Bureau Enterprises, Inc.

1960: 22 Apr., 1123; 15 July, 157

Daedalus

1960: 23 Sept., 836; 7 Oct., 971

Doubleday & Co., Inc.

1960: 5 Feb., 326; 19 Feb., 447; 3 June, 1683

Dover Publications, Inc.

1959: 30 Oct., 1160

1960: 29 Jan., 262; 29 Apr., 1280

Dutton, E. P., & Co.

1960: 2 Sept., 626

Eaton-Dikeman Co.

1960: 20 May, 1562

Edmund Scientific Co.

1960: 26 Aug., 508; 23 Sept., 855



**Instant Controlled
Thorough Mixing**
*In Tubes of Many Sizes
With the*
VORTEX MIXER

4 Tube Model Showing Use
With Different Size Tubes

- SIMPLE TO OPERATE
- ELIMINATES HAND MIXING
- SAVES TIME
- INCREASES ACCURACY

Individual 3-speed control for each tube. Simple one-hand insertion or removal of tubes. Eliminates stoppers, rods, or finger capping. Accommodates tubes up to 25 mm. diameter, up to 200 mm. long.

ADAPTABLE TO ANY MIXING PROCEDURE
IN TEST TUBES
OR CENTRIFUGE TUBES

Ask your laboratory supply
dealer for details, or write
directly to:
**Scientific
Industries, Inc.**
Dept. S-1010, 15 Park St.
Springfield 3, Mass.

SPRAGUE-DAWLEY, INC.

Pioneers in the development

of the

STANDARD LABORATORY RAT.

We are completing another new modern colony which will double our present production.

The new colony building contains every device to insure continuous production and shipment of guaranteed Sprague-Dawley strain albino rats.

Increased orders from our present customers and orders from new customers will be accepted as production builds up.

OUR PLEDGE: Our insistence on the highest possible quality will never be sacrificed to quantity.

Price list will be mailed upon request.

SPRAGUE-DAWLEY, INC.

P.O. Box 2071

Madison, Wisconsin

Fisher Verlag
1960: 22 Apr., 1221

Greiner, Emil, Co.
1960: 22 Jan., 249; 26 Aug., 568

Grune & Stratton
1959: 27 Nov., 1485

Harvard University Press
1959: 20 Nov., 1434
1960: 5 Feb., 366; 22 Apr., 1266; 26 Aug., 565

Holt, Henry, and Co., Inc.
1960: 22 Apr., 1224

Interscience Publishers, Inc.
1959: 13 Nov., 1357

Johns Hopkins Press
1960: 22 Apr., 1251

Kling Photo Corp.
1960: 23 Sept., 834

Lea & Febiger
1959: 4 Dec., 1585
1960: 22 Apr., 1161

Library of Science
1959: 13 Nov., 1289
1960: 11 Mar., 691

Lippincott, J. B., Co.
1960: 22 Jan., 234; 22 Apr., 1252

Long Island Biological Assoc.
1959: 13 Nov., 1361

Macmillan Co.
1960: 22 Apr., 1264; 10 June, 1744

Macy, Josiah, Jr., Foundation
1959: 16 Oct., 993

Martineau, Paul
1960: 13 May, 1455

McGraw-Hill Book Co., Inc.
1960: 22 Apr., 1132, 1133; 26 Aug., 495

Merck & Co., Inc.
1959: 13 Nov., 1348
1960: 17 June, 1820

Mistaire Laboratories
1959: 27 Nov., 1489; 4 Dec., 1608; 11 Dec., 1660; 18 Dec., 1714

Mosby, C. V., Co.
1960: 22 Apr., 1157

Oxford University Press
1959: 4 Dec., 1598
1960: 19 Feb., 546; 8 Apr., 1053; 9 Sept., 682; 7 Oct., 968

Pergamon Press, Inc.
1959: 23 Oct., 1149
1960: 18 Mar., 877; 22 Apr., 1139

Philosophical Library
1959: 2 Oct., 871; 20 Nov., 1433; 27 Nov., 1487
1960: 22 Apr., 1239

Pioneer Scientific Corp.
1960: 16 Sept., 703

Prentice-Hall, Inc.
1960: 22 Apr., 1127, 1141

Princeton University Press
1960: 22 Apr., 1248

Putnam's, G. P., Sons
1960: 4 Mar., 677

Random House
1960: 25 Mar., 940


Reinhold College Textbook Department
1960: 22 Apr., 1129

Rockefeller Institute Press
1959: 4 Dec., 1595

Ronald Press Co.
1960: 8 Jan., 66; 19 Feb., 548; 22 Apr., 1232; 19 Aug., 483

Saunders, W. B., Co.
1959: 9 Oct., 879; 6 Nov., 1211; 4 Dec., 1495
1960: 1 Jan., 3; 12 Feb., 375; 11 Mar., 685; 1 Apr., 955; 8 Apr., 1003; 15 Apr., 1070; 22 Apr., 1115; 29 Apr., 1283; 6 May, 1335; 13 May, 1398; 20 May, 1463;

21 OCTOBER 1960

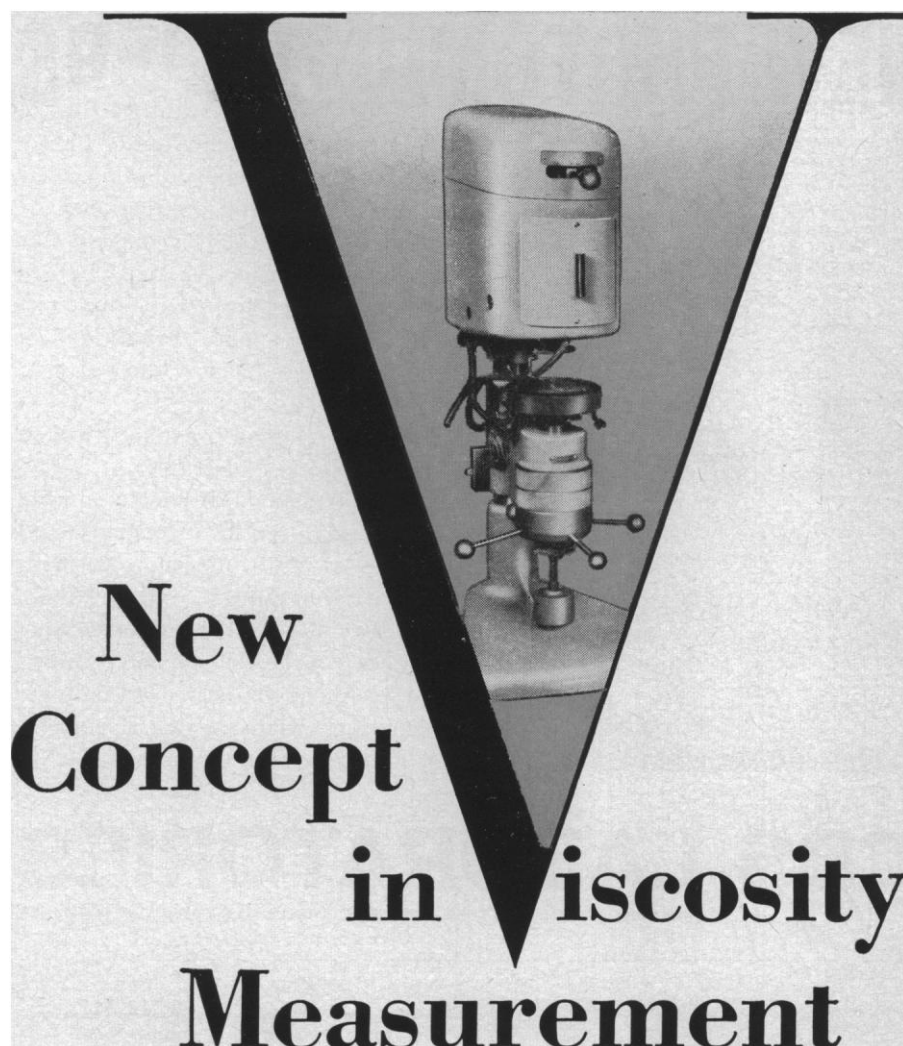

THE FERRANTI-SHIRLEY CONE-PLATE VISCOMETER

This advanced instrument enables the flow behavior of simple or complex fluids to be examined and evaluated with totally new standards of accuracy and precision. The instrument is particularly useful in handling the complex non-Newtonian fluids. Methods long used for characterizing these fluids have been subject to error. The cone-plate principle affords a constant rate of shear, speed accuracy within 0.2%; cone speeds continuously variable so as to give a shear rate range from 2 to 20,000 sec.⁻¹; direct reading of speed, full torque at all speeds, five sensitivities by selector switch.

A programmed control unit for use in conjunction with an X-Y recorder to permit automatic plotting of characteristics is also available.


Investigate this advanced viscometer and the new principle that brings a greater degree of accuracy to the examination of fluids under today's more critical and exacting requirements, both in laboratory and production control applications.

Write for literature.



FERRANTI ELECTRIC, INC.
ELECTRONICS DIVISION
INDUSTRIAL PARK PLAINVIEW, N. Y.

NEW PHOTOMULTIPLIERS

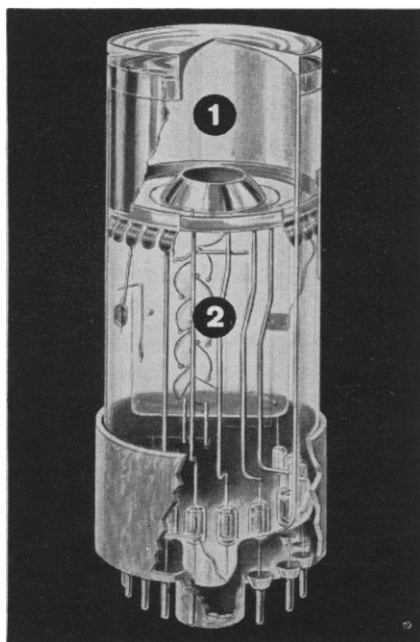


CBS LABORATORIES new line of photomultipliers are specially designed for counting or scanning applications.

Unique photocathode geometry (1) and improved linear dynode structure (2) are combined to provide excellent uniformity of response across the face of the tube and extremely short transit time spread.


The new, rugged photomultipliers are available as illustrated in 2", 3" and 5" diam. cathodes with visible (S-11) or infra-red (S-1) response and 10 stages of multiplication; or with quartz windows in 2" and 3" diam. with ultraviolet (S-13) response. Special types can be developed to order.

For technical bulletins or complete information, write: CBS LABORATORIES, Electron Tube Department.



LABORATORIES

HIGH RIDGE RD. STAMFORD, CONN. • A DIVISION OF COLUMBIA BROADCASTING SYSTEM, INC.

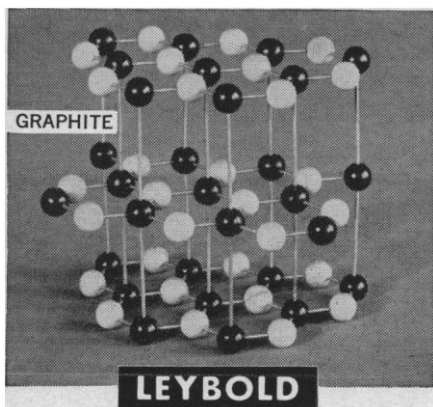

CRYSTAL LATTICE MODELS FOR THE LABORATORY • FOR TEACHING

Three-dimensional models provide the true representation so valuable for both laboratory and teaching.

Angles and dimensions are based on X-ray and electron diffraction data. Linear magnification 250 million times. Spheres have a 20-mm diameter, are painted in various colors, and are permanently joined by metal rods.

The structure of the space lattice of compounds, arrangement of components, formation of planes and characteristic symmetry functions become clearly recognizable.

Write for bulletin describing the many models available.



ARTHUR S. LAPINE AND COMPANY
6001 South Knox Avenue • Chicago 29, Ill.

LANCO LOZENGES®

The **Molded-in-Teflon** Magnetic Stirring Bars with **NO SEAMS, JOINTS, OR PLUGS**

Guaranteed not to corrode or contaminate solutions
*®Trade-Mark Registered—Patent Pending

ACTUAL
SIZE



Lanco LOZENGES® resist practically all chemicals (except molten alkali metals) resist adhesion, have zero moisture absorption and withstand temperatures to 500° F. Powerful Alnico V magnetic bars. Every Lanco LOZENGE® is tested with high frequency spark to assure you perfect quality.

Used for stirring in closed systems and in small capacity vessels.

Lanco Magnetic Stirrers are available with built-in support rod clamp and rheostat. Write for Bulletin 2C58 for complete stirrer information. **Order Direct Today!**

No. 5384-03 Teflon-Covered Stirring Bars

	Length	Each	Lots of 12* ea.
Small	7/8"	\$2.50	\$2.25
Medium	1 1/2"	2.75	2.47
Large	2"	3.00	2.70

*May be Assorted



ARTHUR S. LAPINE AND COMPANY
6001 S. KNOX AVE. • CHICAGO 29, ILLINOIS
LABORATORY SUPPLIES, EQUIPMENT, REAGENT & INDUSTRIAL CHEMICALS

3 June, 1635; 1 July, 3; 12 Aug., 375;
9 Sept., 635; 7 Oct., 911

Schaar and Co.

1960: 20 May, 1557

Science Book Club, Inc.

1959: 9 Oct., 885

Society for General Systems Research

1960: 19 Feb., 539

Springer Verlag

1960: 29 Apr., 1278; 1 July, 4; 22 July, 245; 30 Sept., 905

United Nations

1960: 22 Apr., 1228

University of California Press

1960: 23 Sept., 827

University of Chicago Press

1959: 4 Dec., 1524

1960: 6 May, 1387; 8 July, 99

University of Michigan Press

1960: 29 Jan., 311; 22 Apr., 1131

University of Wisconsin Press

1959: 23 Oct., 1132

1960: 22 Apr., 1145

Van Nostrand, D., Co., Inc.

1959: 23 Oct., 1151

1960: 22 Apr., 1135; 7 Oct., 921

Welch, W. M., Manufacturing Co.

1960: 1 Jan., 51

Wiley, John, & Sons, Inc.

1959: 9 Oct., 888; 4 Dec., 1516, 1517

1960: 12 Feb., 431; 11 Mar., 688; 22

Apr., 1118, 1119

Williams & Wilkins Co.

1960: 22 Apr., 1153

Yale University Press

1960: 1 July, 47

Year Book Publishers, Inc.

1960: 11 Mar., 693; 22 Apr., 1235

BORESCOPIES

American Cystoscope Makers, Inc.

1960: 23 Sept., 821

BRAIN STIMULATION EQUIPMENT

Foringer & Co., Inc.

1960: 7 Oct., 971

BURNERS

Standard Scientific Supply Corp.

1959: 13 Nov., 1360

1960: 19 Feb., 538

CAGES, ANIMAL

Brunswick Corp., Aloe Scientific Div.

1960: 26 Aug., 553; 23 Sept., 835

Kirschner Manufacturing Co.

1960: 19 Feb., 531; 22 Apr., 1231; 23

Sept., 830

Labline, Inc.

1959: 4 Dec., 1599

Maryland Plastics, Inc., Econo-Cage Div.

1959: 23 Oct., 1147

1960: 22 Jan., 239; 19 Feb., 543; 22

Apr., 1249; 29 Apr., 1328; 17 June, 1831;

23 Sept., 764

Will Corp.

1959: 4 Dec., 1513

CALORIMETERS

Parr Instrument Co.

1960: 18 Mar., 870

CAMERAS AND ACCESSORIES

Aloe, A. S., Co., Aloe Scientific Div.

1959: 6 Nov., 1271

American Optical Co.

1959: 6 Nov., 1276

1960: 15 Jan., 172; 22 Apr., 1272; 15 July, 164

Avco Corp., Research and Advanced Development Div.

1959: 23 Oct., 1017

Beckman & Whitley

1959: 23 Oct., 1011

1960: 19 Feb., 569

Kling Photo Corp.

1960: 17 June, 1820; 22 July, 230; 26 Aug., 556

Philips Electronics, Inc.

1959: 13 Nov., 1284, 1285

Rosenthal, Paul

1960: June, 1744; 23 Sept., 822

United Scientific Co.

1959: 23 Oct., 1076, 1077

1960: 19 Feb., 436; 27 May, 1576; 19 Aug., 436

CATALOGS

Ace Glass, Inc.

1960: 22 Jan., 247; 20 May, 1547; 22 July, 237

Baird-Atomic Inc.

1960: 19 Feb., 468

Baker, J. T., Chemical Co.

1959: 4 Dec., 1503

1960: 8 Jan., 65; 18 Mar., 767

Bausch & Lomb Optical Co.

1959: 9 Oct., 896; 6 Nov., 1224; 20 Nov., 1382; 4 Dec., 1534

1960: 29 Jan., 268; 11 Mar., 698; 18 Mar., 772, 773; 25 Mar., 896; 8 Apr., 1014; 22 Apr., 1164; 6 May, 1340; 13 May, 1453; 20 May, 1492; 3 June, 1640; 17 June, 1780; 1 July, 8; 12 Aug., 386; 19 Aug., 479; 23 Sept., 784; 7 Oct., 924

Beckman Instruments, Inc., Scientific and Process Instruments Div.

1960: 4 Mar., 628; 15 Apr., 1068; 29 July, 305

Bel-Art Products

1960: 19 Feb., 555

Brinkmann, C. A., & Co.

1960: 22 Jan., 216, 217, 218; 5 Feb., 361; 26 Feb., 613; 8 Apr., 1004; 20 May, 1549; 3 June, 1685

Corning Glass Works

1959: 9 Oct., 891

1960: 22 Jan., 249; 5 Feb., 323; 11 Mar., 745; 8 Apr., 1011; 13 May, 1450; 3 June, 1636

Colorado Serum Co.

1959: 13 Nov., 1363

1960: 19 Feb., 537; 18 Mar., 857; 22 Apr., 1226

Duralab Equipment Corp.

1960: 18 Mar., 881

Edmund Scientific Co.

1959: 6 Nov., 1221

1960: 18 Mar., 791; 27 May, 1631; 17 June, 1764

Esterline-Angus Co.

1960: 22 July, 250

Falcon Plastics Co.

1959: 23 Oct., 1035

Fisher Scientific Co.

1960: 22 Jan., 189

Greiner, Emil, Co.

1960: 22 Jan., 249


Harvard Apparatus Co., Inc.

1959: 4 Dec., 1605

1960: 22 Apr., 1261

Industrial Instruments, Inc.

1960: 22 Jan., 244; 18 Mar., 846; 22 Apr., 1232; 17 June, 1816

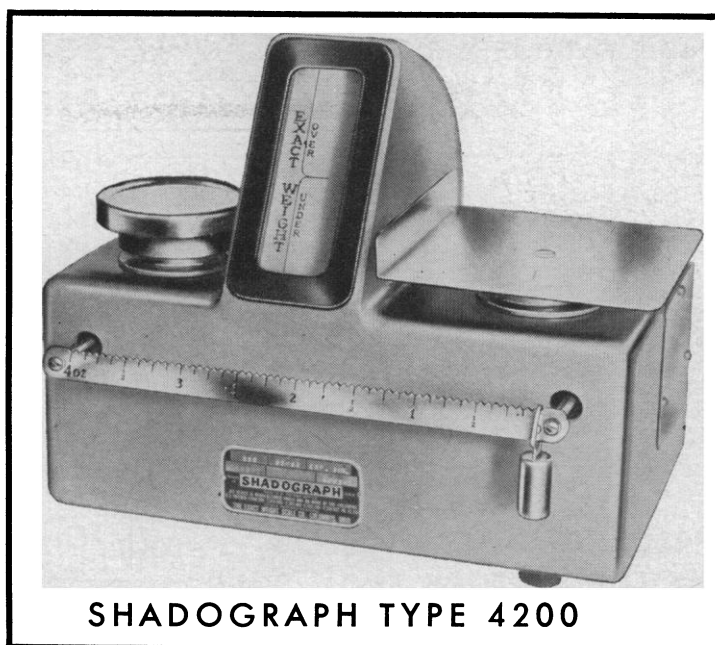

SHADOGRAPH TYPE 4200

Unequalled for versatility,
speed and visible accuracy . . .

SHADOGRAPH® BALANCE SAVES TIME IN COUNTLESS LABORATORY USES

FAST — The Shadograph comes to rest almost immediately.


EASY TO READ — Light-beam projection indication provides a sharp shadow-edge reading on a frosted glass dial. Parallax reading is eliminated.

WEIGHS OUT-OF-LEVEL — The Shadograph is easily moved from one location to another; it weighs accurately without leveling; and is unaffected by normal vibration.


RUGGED — The Shadograph is a precision instrument, sturdily constructed and designed for utmost dependability in day-in-day-out laboratory use.

Models are available with visible sensitivity from one milligram (2000 milligrams capacity) to two grams (35 kilos capacity). We will be glad to demonstrate the time-saving advantages of the Shadograph in your laboratory. No obligation, of course. Write for our laboratory catalog.

OTHER SHADOGRAPH MODELS

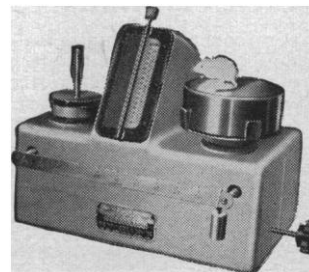

MODEL 4203B-TC-SA,
SMALL ANIMAL BALANCE



MODEL 4142, TISSUE
AND TUMOR BALANCE



THE EXACT WEIGHT SCALE CO.
901 W. FIFTH AVE., COLUMBUS 8, OHIO
In Canada: 5 Six Points Road, Toronto 18, Ont.

Sales and Service Coast to Coast



Instruments for Research and Industry

1960: 18 Mar., 878

Kimble Glass Co.

1960: 15 Jan., 123; 22 Jan., 183; 12 Feb., 381; 11 Mar., 689; 15 Apr., 1072; 13 May, 1399

Kewaunee Scientific Equipment

1960: 19 Feb., 536

Lafayette Radio

1959: 23 Oct., 1013

Lourdes Instrument Corp.

1960: 18 Mar., 783

Matheson Co., Matheson Coleman & Bell Div.

1960: 20 May, 1565

Microchemical Specialties Co.

1960: 22 Apr., 1222

Nalge Co., Inc.

1960: 19 Feb., 532; 18 Mar., 872; 1 Apr., 995; 22 Apr., 1227; 20 May, 1564; 17 June, 1824; 22 July, 248; 26 Aug., 570; 23 Sept., 824

National Appliance Co.

1959: 23 Oct., 1118

1960: 8 Jan., 111; 4 Mar., 674

New Brunswick Scientific Co., Inc.

1960: 15 Jan., 165; 22 Jan., 255; 19 Feb., 559; 26 Feb., 619; 18 Mar., 877; 25 Mar., 943; 22 Apr., 1235; 27 May, 1626; 10 June, 1747; 17 June, 1838; 24 June, 1896

Nuclear-Chicago Corp.

1959: 16 Oct., 996

1960: 1 Apr., 1000

Nuclear Corporation of America,**Isotopes Specialties Co.**

1960: 26 Aug., 577

Nutritional Biochemicals Corp.

1959: 30 Oct., 1159; 13 Nov., 1279; 27 Nov., 1443; 11 Dec., 1615

1960: 8 Jan., 55; 22 Jan., 175; 5 Feb., 315; 19 Feb., 435; 4 Mar., 625; 18 Mar., 753; 1 Apr., 951; 15 Apr., 1063; 29 Apr., 1275; 13 May, 1395; 27 May, 1575; 10 June, 1695; 24 June, 1851; 8 July, 55; 22 July, 167; 5 Aug., 315; 19 Aug., 435; 2 Sept., 583; 16 Sept., 695; 30 Sept., 859

Pioneer Scientific Corp., subsidiary of**Bausch & Lomb Optical Co.**

1960: 16 Sept., 703

Radiochemical Centre

1960: 8 Jan., 115; 5 Feb., 361; 29 Apr., 1325; 24 June, 1893; 22 July, 249

Sanborn Co., Medical Div.

1959: 16 Oct., 983; 11 Dec., 1623

Schueler & Co., Schuco Scientific Div.

1960: 23 Sept., 814

Sorensen & Co. Inc.

1960: 22 Apr., 1223; 20 May, 1468; 23 Sept., 841

Sorvall, Ivan, Inc.

1960: 17 June, 1760, 1761; 23 Sept., 773

Technical Associates

1960: 18 Mar., 865

United Scientific Co.1959: 2 Oct., 871; 30 Oct., 1201; 6 Nov., 1266; 27 Nov., 1484; 4 Dec., 1584
1960: 8 Jan., 114; 15 Jan., 168; 29 Jan., 304; 26 Feb., 616; 4 Mar., 677; 25 Mar., 940; 1 Apr., 996; 8 Apr., 1054; 22 Apr., 1246; 6 May, 1388; 13 May, 1454; 20 May, 1562; 27 May, 1576; 3 June, 1688; 17 June, 1840; 24 June, 1852; 8 July, 98; 15 July, 156; 5 Aug., 364; 12 Aug., 427; 2 Sept., 626; 9 Sept., 683; 16 Sept., 748; 30 Sept., 902; 7 Oct., 970**Welch, W. M., Manufacturing Co.**

1960: 4 Mar., 675; 7 Oct., 967

Will Corp.

1959: 23 Oct., 1127

CELLS**Beckman Instruments, Inc., Scientific and Instruments Process Div.**

1960: 4 Mar., 628; 15 Apr., 1068; 29 July, 305

CENTRIFUGES AND ACCESSORIES**Beckman Instruments, Inc., Spinco Div.**

1959: 9 Oct., 878; 23 Oct., 999; 25 Dec., 1727

1960: 26 Feb., 572; 25 Mar., 890; 27 May, 1574; 24 June, 1850; 26 Aug., 494; 23 Sept., 754

Corning Glass Works

1960: 8 Apr., 1011

Custom Scientific Instruments, Inc.

1959: 23 Oct., 1142

1960: 22 Jan., 234; 22 July, 236; 23 Sept., 834

Doerr Glass Co.

1959: 13 Nov., 1283; 4 Dec., 1499

International Equipment Co.

1959: 2 Oct., 875; 16 Oct., 940; 23 Oct., 1007; 13 Nov., 1299; 27 Nov., 1483; 4 Dec., 1510; 25 Dec., 1730, 1731



1960: 8 Jan., 67; 5 Feb., 318, 319; 19 Feb., 471; 4 Mar., 626; 18 Mar., 797; 8 Apr., 1009; 22 Apr., 1154, 1155; 13 May, 1401; 27 May, 1579; 10 June, 1751; 24 June, 1855; 8 July, 103; 22 July, 175; 5

**FINEST PRECISION INSTRUMENTS
FOR THE LABORATORY FROM****SM XX (citoplast)**

This stereoscopic dissecting microscope is an unsurpassed instrument embodying every known advance in microscopy. Brilliantly-resolved, erect, three-dimensional image. Rotable magnification changer has five built-in parfocal objectives. Magnification range: 4X to 100X at 100 mm working distance.

**SLIDING
MICROMANIPULATOR**

A new conception in the technique of micromanipulation. Ideal for colloidal chemistry, physics, microchemistry, medicine and textiles etc. Allows simple precise manipulation and reliable measurement. Affords free movement in all directions.

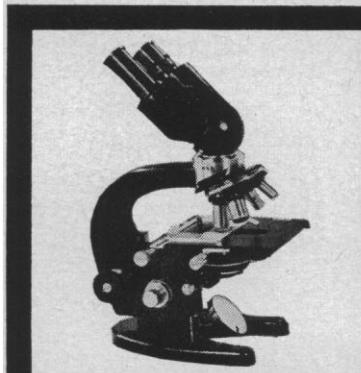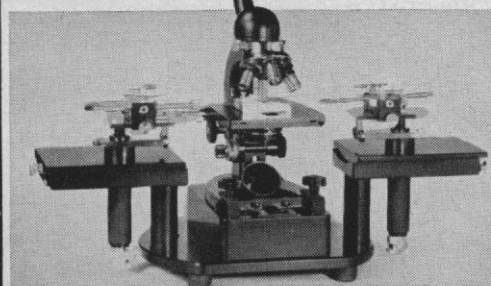**LGOG MICROSCOPES**


The perfect laboratory and research microscope featuring extreme versatility, low positioned course and fine adjustments, or apochromat, quartz or reflecting objectives. Accessories for phase contrast, polarizing, dark field and photomicrographic application.

For complete information on Carl Zeiss Jena precision instruments write:

**Scientific Instrument Division****ERCONA CORPORATION**

16 West 46th Street, New York 36, N.Y.

In Canada: **JENA SCIENTIFIC INSTRUMENTS LTD.**
1437 Mackay Street, Montreal 25, Quebec

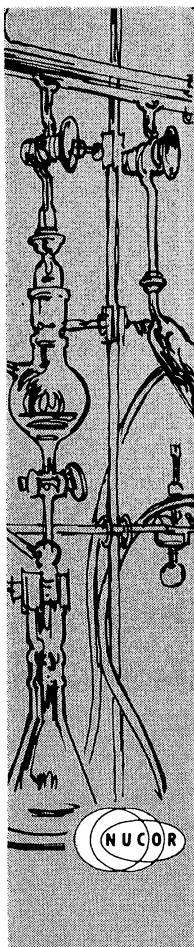

These LABELED COMPOUNDS can increase your research efficiency

I^{131} Iodobenzene Cl^{36} Chlorobenzene

S^{35} Dodecylbenzene Sulphonate

P^{32} Tri-N-Butyl Phosphate H^3 Water

C^{14} Allyl Alcohol H^2 Polyethylene

Whether you require any of the above or others, you are assured of getting labeled compounds of the highest chemical and radio chemical purity.

Should you require a special compound, Isotopes Specialties' skilled personnel can produce it to your exacting requirements.

Write to Dept. S-10 and ask for our Catalog #587 which lists all labeled compounds available for immediate delivery.



ISOTOPES SPECIALTIES CO.

Division of Nuclear Corporation of America
BOX 688 • BURBANK, CALIFORNIA

the modern slant

MORTON stainless steel CULTURE TUBE CLOSURE*

THE PROVEN REPLACEMENT
FOR COTTON PLUGS

Grip culture tubes with patented pressure fingers
 ● Assure reduced evaporation of culture media
 ● Provide adequate aeration for culture ● Resist corrosion and retain resilience ● Reliably prevent contamination.

*U. S. Pat. No. 2,287,746

WRITE TODAY FOR BROCHURE C-3
 "research deserves the best" **BELCO GLASS INC.**
 VINELAND, NEW JERSEY

THE NEW BRUNSWICK 6-UNIT

Batch Fermentor


- For Aerobic and Anaerobic Fermentations
- For Tissue Culture and Metabolic Studies
- Completely Autoclavable

Six stainless steel fermentors, with Pyrex jars of 5, 7.5, or 14 liter capacity, are removable for autoclaving. The non-freezing agitators are in stainless steel, ball-bearing housings which incorporate leakproof seals for repeated autoclaving. Performance is cool, quiet, and dependable even under continuous operation.

Temperature, agitation-speed, air volume and pressure are measured and precisely regulated. The stainless steel water baths, with a temperature range up to 60°C. are thermostatically controlled within $\pm 0.5^\circ\text{C}$.

Twin anti-friction drives provide a wide range of agitation rates. The apparatus can be equipped with automatic pH control and electronic anti-foam system.

Models with Single
and 3-Fermentor Drive
Assemblies Also Available.

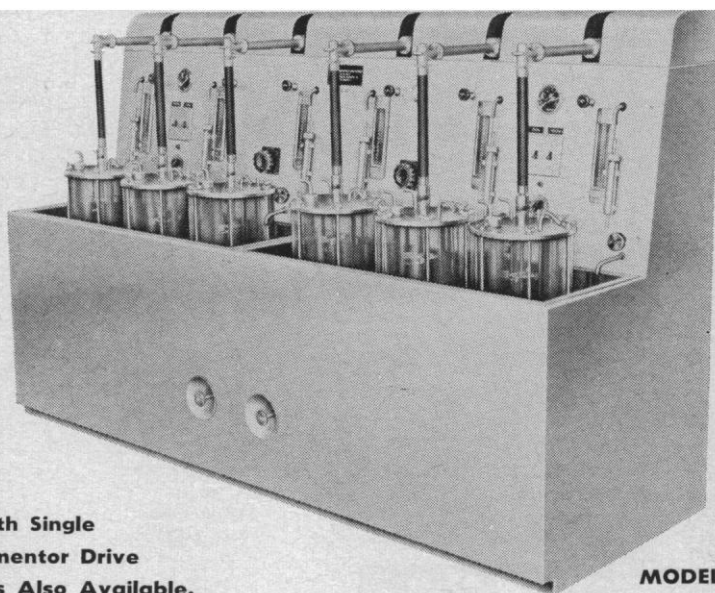

MODEL
FS-614

UNCONDITIONAL ONE-YEAR WARRANTY

WRITE FOR
CATALOG
FS-0215



NEW BRUNSWICK SCIENTIFIC CO., INC.
PRECISION LABORATORY APPARATUS
P.O. BOX 606, NEW BRUNSWICK, NEW JERSEY

EXACTING CONSTANT TEMPERATURE TASKS

such as

- ✓ Semiconductor Testing
- ✓ Critical Incubations
- ✓ Guidance Components Testing
- ✓ Plastics Conditioning

REQUIRE A

Treas

CONSTANT TEMPERATURE CABINET WITH

guaranteed temperature uniformity as close as $\pm 0.90^{\circ}\text{C}$... Long lasting stainless steel interiors... Electronic control.



You can choose from 60 models...all sizes...all temperature ranges...all guaranteed for 5 years and backed by 56 years of proved performance...

Write for Bulletin 302

Treas
Built By

SINCE 1920

PRECISION
SCIENTIFIC CO.



3735 West Cortland St., Chicago 47, Ill.

Local Offices in
Chicago • Cleveland • Houston
New York • Philadelphia • San Francisco

Aug., 319; 19 Aug., 438; 2 Sept., 587; 30 Sept., 860

Lourdes Instrument Corp.

1959: 23 Oct., 1014

1960: 22 Jan., 182; 19 Feb., 441; 18 Mar., 783; 22 Apr., 1149; 23 Sept., 819; 7 Oct., 969

Sorvall, Ivan, Inc.

1959: 23 Oct., 1024, 1025; 13 Nov., 1371; 4 Dec., 1509

1960: 19 Feb., 444, 445; 18 Mar., 756, 757; 20 May, 1561; 17 June, 1760, 1761; 22 July, 231; 26 Aug., 567; 23 Sept., 773

CHEMICALS, BIOLOGICAL

Borden Chemical Co.

1959: 23 Oct., 1142

Difco Laboratories

1959: 13 Nov., 1351

1960: 22 Apr., 1221; 26 Aug., 563

Matheson Co., Inc., Matheson Coleman & Bell Div.

1960: 20 May, 1565

Merck & Co., Inc.

1959: 13 Nov., 1348

New England Nuclear Corp.

1959: 20 Nov., 1432

Nutritional Biochemicals Corp.

1959: 2 Oct., 819; 16 Oct., 939; 30 Oct., 1159; 13 Nov., 1279; 27 Nov., 1443; 11 Dec., 1615; 25 Dec., 1727

1960: 8 Jan., 55; 22 Jan., 175; 5 Feb., 315; 19 Feb., 435; 4 Mar., 625; 18 Mar., 753; 1 Apr., 951; 15 Apr., 1063; 29 Apr., 1275; 13 May, 1395; 27 May, 1575; 10 June, 1695; 24 June, 1851; 8 July, 55; 22 July, 167; 5 Aug., 315; 19 Aug., 435; 2 Sept., 583; 16 Sept., 695; 30 Sept., 859

Schwarz BioResearch, Inc.

1959: 9 Oct., 880; 13 Nov., 1300

1960: 22 Jan., 179; 5 Feb., 363; 18 Mar., 786; 20 May, 1482; 10 June, 1745; 22 July, 172; 29 July, 307; 23 Sept., 779

Sigma Chemical Co.

1959: 6 Nov., 1269; 4 Dec., 1591

1960: 1 Jan., 47; 29 Jan., 305; 26 Feb., 617; 25 Mar., 941; 20 May, 1545; 17 June, 1823; 15 July, 159; 23 Sept., 843

Will Corp.

1960: 20 May, 1516, 1517

Winthrop Laboratories

1959: 23 Oct., 1116

1960: 12 Feb., 425; 18 Mar., 843; 22 Apr., 1251; 27 May, 1628; 16 Sept., 749

Worthington Biochemical Corp.

1960: 1 Jan., 48; 5 Feb., 364; 4 Mar., 630; 1 Apr., 994; 20 May, 1543; 3 June, 1682; 1 July, 49; 5 Aug., 365; 2 Sept., 625; 23 Sept., 844

CHEMICALS, GENERAL

Allied Chemical Co., General Chemical Div.

1960: 22 Jan., 240; 18 Mar., 845; 22 July, 244

Eastern Chemical Corp.

1960: 7 Oct., 971

Harshaw Chemical Co.

1959: 13 Nov., 1346

1960: 8 Jan., 112; 29 Jan., 306

Mallinckrodt Chemical Works

1960: 18 Mar., 795; 20 May, 1473

Matheson Co., Inc., Matheson


Coleman & Bell Div.

1960: 17 June, 1827; 22 July, 168

Pilot Chemicals, Inc.

1959: 23 Oct., 1146

ISOTOPES for Your Development Work

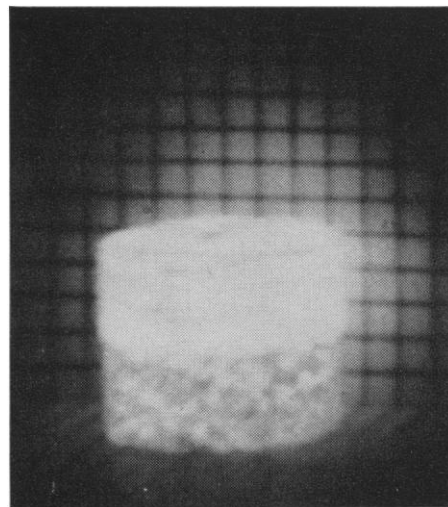

Oak Ridge National Laboratory offers more than 300 radioactive and stable isotope products.

RADIOISOTOPES


Processed Solutions—90 processed radioisotopes may be obtained, including many carrier-free and high specific activity products.

Now Available—Iridium-192 gamma sources with specific activity up to 100 curies per gram, and cobalt-60 radiography sources 1/8 and 1/16-inch in diameter with specific activity greater than 100 curies per gram. At a reduced price, carbon-14 barium carbonate is available at \$9.50 per millicurie.

STABLE ISOTOPES

More than 200 stable isotopes available from 50 elements.... Chemical processing and target fabrication services also offered.... Ultra-high isotopic purity in a number of isotopes.

For information or literature, write to: Isotopes Division, Oak Ridge National Laboratory, P. O. Box X, Oak Ridge, Tennessee.



OAK RIDGE NATIONAL LABORATORY

Operated by
UNION CARBIDE CORPORATION
for the
U.S. ATOMIC ENERGY COMMISSION



Standard Scientific Supply Corp.

1960: 7 Oct., 966

Winthrop Laboratories

1959: 27 Nov., 1485

1960: 12 Feb., 425; 18 Mar., 843

CHEMICALS, ORGANIC

Allied Chemical Co.

1960: 18 Mar., 845

Eastern Chemical Corp.

1960: 7 Oct., 971

Matheson Co., Inc.

1960: 19 Aug., 484

CHEMICALS, TRACER

Baird-Atomic, Inc.

1960: 22 Apr., 1121; 20 May, 1515

New England Nuclear Corp.

1959: 9 Oct., 929; 23 Oct., 1129; 6 Nov., 1267; 20 Nov., 1432; 4 Dec., 1603; 18 Dec., 1717

1960: 1 Jan., 51; 15 Jan., 164; 29 Jan., 308; 12 Feb., 426; 26 Feb., 613; 11 Mar., 744; 25 Mar., 938; 8 Apr., 1053; 22 Apr., 1255; 6 May, 1385; 20 May, 1568; 3 June, 1684; 17 June, 1838; 1 July, 51; 15 July, 161; 29 July, 311; 12 Aug., 425; 26 Aug., 571; 9 Sept., 684; 23 Sept., 814; 7 Oct., 972

Nuclear-Chicago Corp.

1960: 29 Apr., 1332; 30 Sept., 908

Nuclear Corporation of America,

Isotopes Specialties Co.

1960: 26 Aug., 577

Oak Ridge National Laboratory

1960: 19 Feb., 528; 18 Mar., 854; 22 Apr., 1224; 10 June, 1742; 23 Sept., 818

Picker X-Ray Corp.

1960: 20 May, 1489; 15 July, 107

Radiochemical Centre

1959: 13 Nov., 1347

1960: 8 Jan., 115; 5 Feb., 361; 29 Apr., 1325; 24 June, 1893; 22 July, 249; 16 Sept., 747

Schwarz BioResearch, Inc.

1959: 13 Nov., 1300; 18 Dec., 1715

1960: 18 Mar., 786; 15 Apr., 1107; 22 July, 172; 29 July, 307

Tracerlab, Inc.

1959: 23 Oct., 1141; 27 Nov., 1486

1960: 22 Apr., 1130

**CHROMATOGRAPHY EQUIPMENT
AND ACCESSORIES**

American Instrument Co., Inc.

1959: 4 Dec., 1590

Atomic Accessories, Inc.

1959: 23 Oct., 1004

1960: 17 June, 1826

Barber-Colman Co., Wheelco

Instruments Div.

1960: 22 Apr., 1156; 17 June, 1758; 22 July, 176; 26 Aug., 514

Beckman Instruments, Inc.

1959: 2 Oct., 825; 6 Nov., 1212; 20 Nov., 1379; 27 Nov., 1442

1960: 12 Feb., 374; 4 Mar., 629; 1 Apr., 956; 8 Apr., 1002; 10 June, 1694; 22 July, 166

California Laboratory Equipment Co.

1959: 23 Oct., 1116; 13 Nov., 1347; 4 Dec., 1601; 25 Dec., 1767

Central Scientific Co.


1960: 29 Jan., 308; 27 May, 1626; 7 Oct., 973

Corning Glass Works

1960: 22 Jan., 249

21 OCTOBER 1960

New WILD*

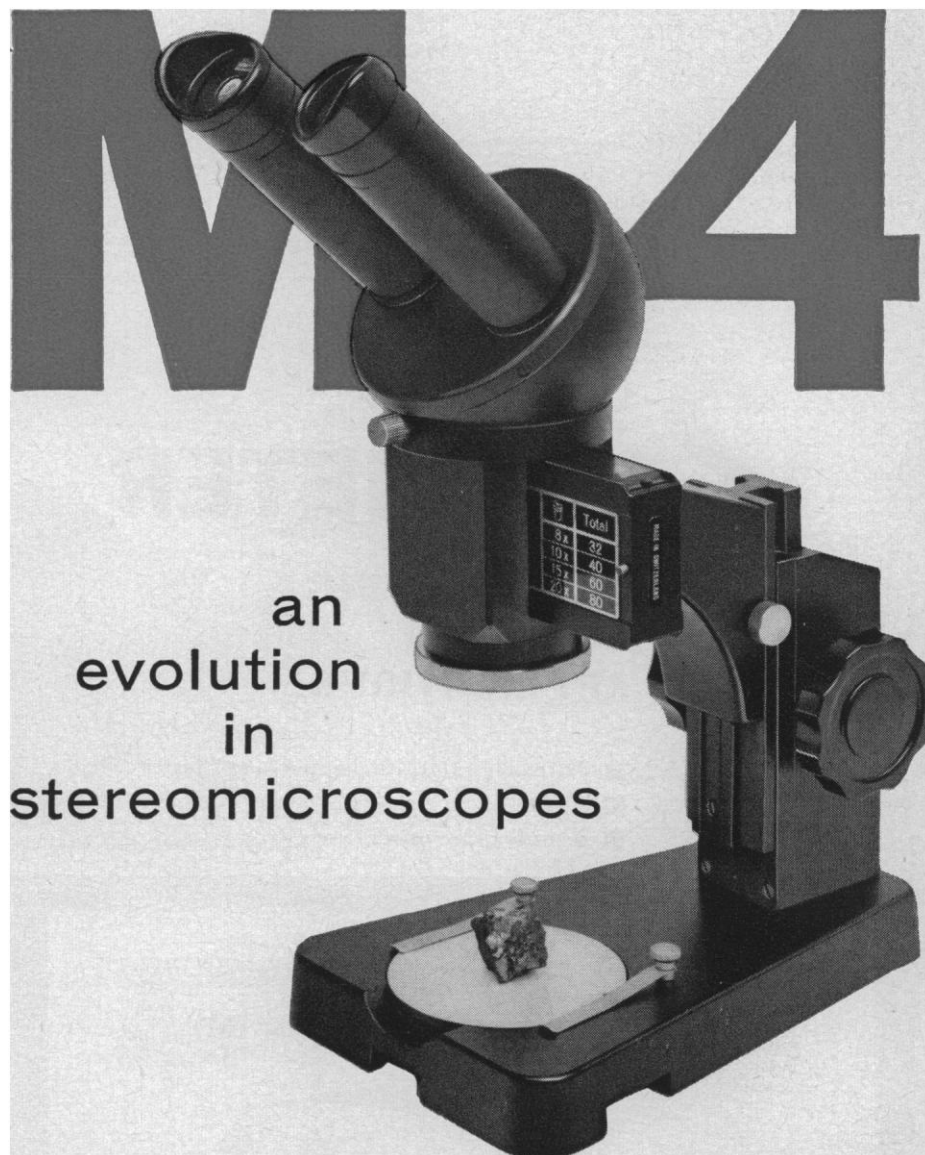

Did you ever see such simplicity in a multi-purpose stereomicroscope?

Yet here is an instrument with all the efficiency and versatility for educational and industrial laboratory use. The M-4 is available with either fixed magnification or variable by means of power cartridge...providing a total range of from 5x to 160x with interchangeable eyepieces and attachment objectives.

This new simplified design concept, carried through a complete range of accessories for photomicrography, results in lower acquisition cost.

The Wild M-4 is the stereomicroscope you must investigate. Write for Booklet M-4.

*The FIRST name in a complete line of Surveying Instruments, Photogrammetric Equipment and Microscopes.

WILD
HEERBRUGG

WILD HEERBRUGG INSTRUMENTS, INC.
PORT WASHINGTON, NEW YORK

In Canada: Wild of Canada Ltd.,
157 Maclearen St., Ottawa, Ontario

F & M Scientific Corp.
 1960: 18 Mar., 766; 20 May, 1486; 26 Aug., 562; 23 Sept., 769
Greiner, Emil, Co.
 1960: 22 Jan., 249
Hamilton Co., Inc.
 1960: 26 Aug., 513; 23 Sept., 831
Kontes Glass Co.
 1959: 2 Oct., 826
Labline, Inc.
 1960: 22 Jan., 233
Microchemical Specialties Co.
 1960: 19 Feb., 530
New Brunswick Scientific Co., Inc.
 1959: 23 Oct., 1123; 11 Dec., 1666
 1960: 5 Feb., 367; 13 May, 1452; 24 June, 1896; 23 Sept., 849


Packard Instrument Co., Inc.
 1959: 23 Oct., 1041; 11 Dec., 1628
 1960: 22 Jan., 196; 19 Feb., 478; 1 Apr., 958; 27 May, 1582; 22 July, 190; 2 Sept., 590
Perkin-Elmer Corp., Instrument Div.
 1960: 12 Feb., 376; 22 Apr., 1116; 15 July, 108; 26 Aug., 496
Phoenix Precision Instrument Co.
 1959: 23 Oct., 1006
 1960: 19 Feb., 550; 20 May, 1546; 23 Sept., 845
Photovolt Corp.
 1959: 13 Nov., 1361; 18 Dec., 1717
 1960: 19 Feb., 527; 18 Mar., 857; 22 Apr., 1231; 20 May, 1559; 17 June, 1825; 22 July, 245; 26 Aug., 563; 23 Sept., 839

Reeve Angel
 1960: 19 Feb., 454; 20 May, 1481
Research Specialties Co.
 1959: 23 Oct., 1043
 1960: 23 Sept., 816
Schaar and Co.
 1960: 20 May, 1557
Schleicher, Carl, & Schuell Co.
 1960: 16 Sept., 745
Schueler and Co., Schuco Scientific Div.
 1960: 19 Feb., 565; 23 Sept., 814
Scientific Glass Apparatus Co., Inc.
 1959: 23 Oct., 1026
Sigma Chemical Co.
 1960: 26 Aug., 575
Technicon Chromatography Corp.
 1960: 22 Apr., 1247; 17 June, 1837; 23 Sept., 853
Ultra-Violet Products, Inc.
 1959: 13 Nov., 1364
Vanguard Instrument Co.
 1959: 4 Dec., 1531
 1960: 26 Aug., 506

2 CHANNEL pH METER

FOR EXACTING RESEARCH APPLICATIONS

- readable & sensitive to changes of 0.001 pH
- extremely low drift chopper-amplifier circuitry
- hum rejection circuitry
- recording provisions

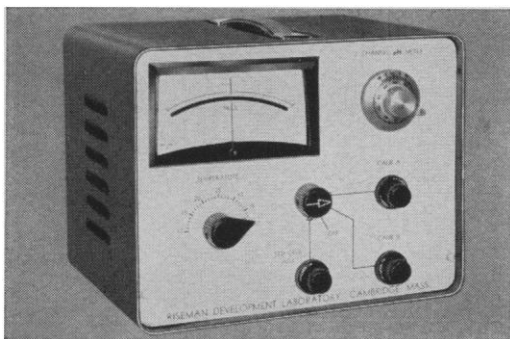

size: 8 x 10 x 8" wt: 10 1/4 lbs.

- for measuring small pH changes accurately
- for use with Severinghaus pCO₂ electrodes
- for use with sodium or potassium sensitive glass electrodes
- models available with millivolt scales and combination null-balance & direct reading

RISEMAN DEVELOPMENT LABORATORY
 18 MOUNT AUBURN STREET • CAMBRIDGE 38, MASS.

CLAMPS

LaPine, Arthur S., and Co.
 1960: 22 Jan., 250; 22 July, 246

CLASSROOM CHARTS

Welch, W. M., Manufacturing Co.
 1959: 2 Oct., 867
 1960: 1 Jan., 51; 3 June, 1685
Central Scientific Co.
 1960: 22 Jan., 255; 18 Mar., 857; 13 May, 1452

CLEANSERS

Alconox, Inc.
 1959: 6 Nov., 1269
 1960: 22 Apr., 1245; 22 July, 240
Greiner, Emil, Co.
 1960: 22 Apr., 1246; 17 June, 1820
Meinecke & Co., Inc.
 1959: 23 Oct., 1114; 4 Dec., 1580
 1960: 19 Feb., 474; 18 Mar., 868; 22 Apr., 1263; 17 June, 1834; 23 Sept., 828
Ultrasonic Industries, Inc.
 1960: 22 Apr., 1238

COBALT-60 IRRADIATORS

Atomic Energy of Canada Limited
 1960: 23 Sept., 781
Budd Co., Nuclear Systems Div.
 1959: 9 Oct., 935

COLONY COUNTERS

American Optical Co.
 1960: 3 June, 1692
New Brunswick Scientific Co., Inc.
 1959: 23 Oct., 1123
 1960: 8 Jan., 116; 26 Feb., 619; 3 June, 1687

COLORIMETERS AND ACCESSORIES

Bausch & Lomb Optical Co.
 1959: 9 Oct., 896
 1960: 1 Jan., 8; 9 Sept., 642
Beckman Instruments, Inc., Scientific and Process Instruments Div.
 1960: 4 Mar., 628; 15 Apr., 1068; 29 July, 305
Fisher Scientific Co.
 1960: 22 July, 174

NOW
A LOW COST METERING
PUMP
FOR
SULPHURIC ACID
AND OTHER
STRONG OXIDIZING AGENTS

Now a special formulation of Hypalon makes the dependable SIGMAMOTOR Pump applicable for metering sulphuric acid or other strong oxidizing agents. Liquid is forced through Hypalon tubing by wave-like action of steel fingers. Never contacts metal.



Model T6SH opens to permit change of tubing easily — quickly.

SIGMAMOTOR Inc.
 68 NORTH MAIN STREET • MIDDLEPORT, NEW YORK

DIFCO

Dehydrated
Culture Media
DIFCO


The utmost in efficiency and economy in the bacteriological laboratory is realized through use of Dehydrated Culture Media, Difco.

Convenience—any medium can be instantly prepared.
 Stability—media can be kept without deterioration.
 Availability—each medium is instantly available.
 Completeness—no additional ingredients are required.
 Uniformity—successive lots are identical.
 Comparability—dependable, comparative studies are possible in widely separated laboratories over long periods of time when standardized Difco Products are employed.

Specify "DIFCO"


DIFCO LABORATORIES
DETROIT 1, MICHIGAN

COUNTERCURRENT
FRACTIONATOR

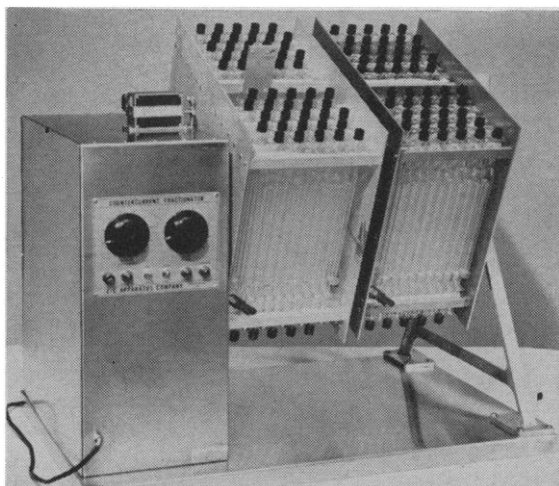

▲ EC520 COUNTERCURRENT FRACTIONATOR with automatic drive; two racks of 100 20-ml tubes on base 24" x 34".

NEW VERTICAL GEL ELECTROPHORESIS

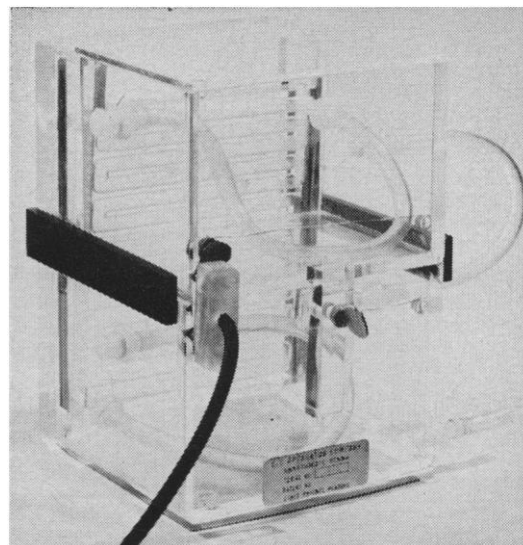

EC470 VERTICAL GEL ELECTROPHORESIS APPARATUS, WATER-COOLED PRESSURE PLATES

SEND FOR FURTHER INFORMATION AND DETAILED SPECIFICATIONS

E-C APPARATUS COMPANY

538 WALNUT LANE
 SWARTHMORE, PENNA.

BARNSTEAD DEMINERALIZERS FOR ALL INDUSTRIAL APPLICATIONS



DESCRIBED IN NEW CATALOG #160

This NEW 36-page Catalog features the complete line of Barnstead Mixed-Bed, Two-Bed, and Four-Bed Demineralizers with capacities of up to 2500 gallons per hour and more . . . built to your specifications. A special section of interest to Nucleonic and Electronic engineers is devoted to Barnstead "Train" equipment which produces ultra pure water of 18,000,000 ohms resistance at 25° C. This Pure Water equipment connected in series also removes organics, inorganics, bacteria, gases, and submicroscopic particles down to 0.45 micron. Other sections are devoted to Barnstead Tin-Lined Piping, Fittings, Faucets, Purity Meters, Storage Tanks, Sand and Carbon Filters, Submicron® Filters, and other auxiliary equipment.

Installation case histories of Barnstead "Pure Water Specials" are also described and illustrated. Charts, specification drawings and actual on-job installations are detailed. Write for your copy of Catalog #160 Today!

Barnstead®
STILL AND STERILIZER CO.
00 Lanesville Terrace, Boston 31, Mass.

BOSTON Jamaica 2-8490	NEW YORK Kingsbridge 8-1557	CLEVELAND ACademy 6-6622
CHICAGO Rogers Park 1-6173	PHILADELPHIA Broadway 9-3146	WASHINGTON, D.C. District 7-1142
LOS ANGELES Ryan 1-6663	SAN FRANCISCO TEmplebar 2-5391	DETROIT ENTERprise 7422

FIRST IN WATER PURIFICATION
SINCE 1878

Instrumentation Associates

1960: 29 Jan., 304; 17 June, 1840

Klett Manufacturing Co.

1959: 2 Oct., 867; 16 Oct., 988; 23 Oct., 1132; 30 Oct., 1202; 13 Nov., 1347; 20 Nov., 1432; 27 Nov., 1486; 4 Dec., 1597; 18 Dec., 1717; 25 Dec., 1767

1960: 22 Jan., 243; 5 Feb., 368; 19 Feb., 545; 4 Mar., 676; 18 Mar., 843; 1 Apr., 997; 15 Apr., 1106; 6 May, 1384; 27 May, 1626; 8 July, 94; 15 July, 159; 29 July, 311; 5 Aug., 369; 2 Sept., 628; 16 Sept., 747; 7 Oct., 973

Photovolt Corp.

1959: 9 Oct., 929; 11 Dec., 1663

1960: 8 Jan., 116; 22 Jan., 251; 11 Mar., 747; 8 Apr., 1055; 15 Apr., 1109; 27 May, 1628; 24 June, 1896; 1 July, 47; 15 July, 160; 19 Aug., 477

Thomas, Arthur H., Co.

1960: 8 Jan., 120

COMPUTERS

American Bosch Arma Corp.

1960: 10 June, 1698

Burroughs Corp., ElectroData Div.

1960: 18 Mar., 762, 763; 20 May, 1466, 1467

Donner Scientific Co.

1960: 18 Mar., 776

General Motors Research Laboratories

1960: 10 June, 1702

Royal McBee Corp.

1959: 2 Oct., 824; 6 Nov., 1216

1960: 25 Mar., 891; 29 July, 263

CONDUCTIVITY EQUIPMENT

Industrial Instruments, Inc.

1959: 13 Nov., 1365

1960: 22 Jan., 244; 18 Mar., 846; 22 Apr., 1232; 17 June, 1816; 26 Aug., 573

CONE, TAPER

Burdick & Jackson Laboratories

1960: 22 Apr., 1259

CONNECTORS, ELECTRICAL

Superior Electric Co.

1959: 13 Nov., 1349

CONTROLLERS

Smith, Arthur F., Inc.

1960: 7 Oct., 968

CRUCIBLES, PLATINUM-CLAD

Fisher Scientific Co.

1960: 20 May, 1571; 23 Sept., 777

CURRENT INTEGRATOR

Eldorado Electronics

1959: 23 Oct., 1150

DECAPITATORS

Harvard Apparatus Co., Inc.

1960: 18 Mar., 843

DEMINERALIZERS

Barnstead Still and Sterilizer Co.

1959: 23 Oct., 1042

1960: 22 Apr., 1248; 20 May, 1566

Outstanding RONALD Books

DEVELOPING CELL SYSTEMS AND THEIR CONTROL

Edited by Dorothy Rudnick,
Albertus Magnus College
and Yale University



Just published! 18th Growth Symposium. This new book presents and describes advances in the knowledge of cell differentiation and its control within the organism, from both the biological and biochemical points of view. The ten internationally known contributors discuss a diversity of organisms in the plant, animal, and micro-biological kingdoms. 1960. 240 pp., 125 ills. \$8

The 16th and 17th Symposia of the Society for the Study of Development and Growth—

Developmental Cytology. Dorothea Rudnick, Editor, with 10 Contributors. 1959. 215 pp.; 118 ills., tables. \$7

Cell, Organism, and Milieu. Dorothea Rudnick, Editor, with 12 Contributors. 1959. 326 pp.; 136 ills., tables. \$8

SUBCELLULAR PARTICLES

Edited by Teru Hayashi,
Columbia University

The Fifth Annual Symposium Publication of the Society of General Physiologists. A comprehensive review of research on cell inclusions. Emphasis is on the structural aspects of subcellular particles as related to their function, especially with regard to the heterogeneous system created by the very presence of the particulate material within the cell. 20 Contributors. 1959. 213 pp.; 122 ills., tables. \$6

Other S.G.P. Symposia—

Physiological Adaptation. C. Ladd Prosser, Editor, with 14 Contributors. 1958. 185 pp.; 90 ills., tables. \$4

Influence of Temperature on Biological Systems. Frank H. Johnson, Editor, with 24 Contributors. 1957. 275 pp.; 133 ills., tables. \$4.50

Physiological Triggers and Discontinuous Rate Processes. Theodore H. Bullock, Editor, with 16 Contributors. 1957. 179 pp.; 55 ills., tables. \$4

Electrolytes in Biological Systems. Abraham M. Shanes, Editor, with 11 Contributors. 1955. 243 pp.; 123 ills., tables. \$4

INTRODUCTION TO QUANTITATIVE GENETICS

D. S. Falconer,
University of Edinburgh

A valuable synthesis of material on the inheritance of quantitative differences between individuals. The basic theory of quantitative variations is developed, showing what variations can be attributed to genetic and non-genetic causes. Many examples illustrate the theoretical discussions. 1960. 348 pp.; 98 ills., tables. \$6

PRINCIPLES OF PALEOBOTANY

William C. Darrah,
Gettysburg College

Second Edition of this textbook presents the conceptual scheme of paleobotany through the explanation and use of the assumptions and techniques employed in the interpretation of the fossil record. A Chronica Botanica Publication. 2nd Ed., 1960. 295 pp.; 75 ills., tables. \$6.50

Publishers of the Chronica Botanica Books

Order direct from:

THE RONALD PRESS COMPANY
15 East 26th St., New York 10

DENSITOMETERS

Photovolt Corp.

1959: 9 Oct., 929; 13 Nov., 1361; 18 Dec., 1717

1960: 8 Jan., 116; 12 Feb., 425; 19 Feb., 527; 18 Mar., 857; 15 Apr., 1109; 22 Apr., 1231; 20 May, 1559; 17 June, 1825; 24 June, 1896; 22 July, 245; 19 Aug., 477; 26 Aug., 563; 16 Sept., 749; 23 Sept., 839

Welch, W. M. Manufacturing Co.

1959: 23 Oct., 1113

1960: 4 Mar., 675; 7 Oct., 967

DESICCATORS

New York Laboratory Supply Co., Inc.

1960: 17 June, 1819

Precision Scientific Co.

1960: 19 Feb., 537; 22 Apr., 1244; 20 May, 1552

DISINTEGRATORS

Instrumentation Associates

1959: 23 Oct., 1152

1960: 20 May, 1554

DOSIMETERS

Bausch & Lomb Optical Co.

1960: 1 Jan., 8

Cambridge Instrument Co., Inc.

1960: 18 Mar., 844

DRY BOXES

American Sterilizer Co.

1960: 22 July, 177; 23 Sept., 761

Blickman, S., Inc.

1960: 20 May, 1557

Greiner, Emil, Co.

1960: 19 Feb., 550

Kewaunee Scientific Equipment

1960: 19 Feb., 536

EGG PUNCH

Tri-R Instruments

1960: 22 Apr., 1258

ELECTROMAGNETS

Harvey-Wells Electronics, Inc.

1960: 18 Mar., 875; 22 Apr., 1225; 17 June, 1825; 22 July, 249

ELECTROMETERS

Applied Physics Corp.

1959: 6 Nov., 1266

1960: 22 Jan., 235; 22 July, 236

Nuclear-Chicago Corp.

1960: 1 Apr., 1000

Victoreen Instrument Co.

1960: 22 Jan., 252

ELECTROPHORESIS APPARATUS

American Instrument Co., Inc.

1959: 4 Dec., 1512

Beckman Instruments, Inc., Spinco Div.

1959: 13 Nov., 1278; 11 Dec., 1614

1960: 8 Jan., 54; 22 Jan., 174; 11 Mar., 684; 22 Apr., 1114; 13 May, 1394; 17 June, 1776; 12 Aug., 374

Brinkman, C. A., & Co., Inc.

1959: 6 Nov., 1219

21 OCTOBER 1960

NOW AVAILABLE FROM YEDA
RESEARCH AND DEVELOPMENT
COMPANY, LTD. (AT THE
WEIZMANN INSTITUTE OF SCIENCE)
IN THE WESTERN HEMISPHERE...

Exclusively through

SCHWARZ BIORESEARCH

A GROUP OF HIGHLY SPECIALIZED
AMINO ACID COMPOUNDS* PRODUCED BY
THE YEDA RESEARCH AND DEVELOPMENT
COMPANY, LTD. AT THE
WEIZMANN INSTITUTE

This unique group of over 80 compounds includes amino acid derivatives, peptides, polypeptides and O^{18} labelled amino acids, many of which are available in a choice of three grades of purity. Yeda is equipped to make to your order a host of specialized compounds. Inquiries are invited for quotations on any special requirements of amino acid derivatives and peptides. All material is made in Israel and shipped to Schwarz by air. We assure *prompt delivery* to all parts of the world.

*Among others: Carbobenzoxy Chloride (glacial) • p-Nitro Cbz Chloride (crystalline) • L-Lysine Ethyl Ester Dihydrochloride • N-Cbz-L-Arginine • S-Cbz-L-Cysteine • N-Cbz-L-Tryptophan • Cbz-L-Leucyl Hydrazide • ε-Cbz-L-Lysyl Benzyl Ester Hydrochloride • α-Phthaloyl-ε-Cbz-L-Lysine • Cbz-L-Proline • Cbz-L-Glutamic Acid Anhydride • Poly-L-Aspartic Acid • Poly-L-Glutamic Acid • Poly-L-Lysine Hydrobromide

*Send us your requirements and write for our new, free catalog and price list.
If in a rush, wire us at BIORE or call Mount Vernon 4-1100.*



SCHWARZ BIORESEARCH, INC. • Department JB, Mount Vernon, New York
BIOCHEMICALS • RADIOCHEMICALS • PHARMACEUTICALS for research, for medicine, for industry

"HOT OFF THE PRESS"
**"THE INSIDE DOPE" WITH
 THE LATEST WORD ON
 SAFETY ENCLOSURES**



Our Hero displays, with justifiable pride, the catalog which is truly "the last word" on Safety Enclosures . . . glove, vacuum and dry boxes; dust free enclosures; and controlled atmosphere systems.

"The inside dope" is now a part of our service . . . try some.

Write for your
 copy today → **K·S·E** KEWAUNEE SCIENTIFIC EQUIPMENT ADRIAN, MICHIGAN

4004 Logan Street

NATIONAL APPLIANCE

**32 CUBIC FOOT
 INCUBATOR**



An economical investment for large volume incubation of tube and plate cultures. Excellent for classroom, incubators can be placed side by side. Will accommodate large containers such as 5-gal. carboys. 30 square feet of adjustable nickel-plated shelves. Additional shelves can be installed any time.

Blower convects air through side wall ducts from bottom heating chamber to top and downward over work area. Fully instrumented. Temperature controlled by hydraulic thermostat and limited by safety thermostat. Temperature—room to 65° C. Max. temp. differential 1° C.

Interior white baked enamel—exterior durable light beige enamel over steel. Outside: 36" w., 30" d., 90" h. Inside: 31" w., 24½" d., 74" h. 2" fiberglass insulation. 1500 watts, 115, 208, or 230 volts AC.

Write for bulletin or catalog of complete N. A. line.

na
 NATIONAL APPLIANCE COMPANY
 CONTROLLED ENVIRONMENT

National Appliance Co.
 7634 S.W. Capitol Hy. • Portland 19, Ore.

Eastern Sales:
 H. Reeve Angel & Co., Inc.
 9 Bride Well Pl. • Clifton, N. J.

NATIONAL APPLIANCE

E-C Apparatus Co.

1959: 2 Oct., 869; 4 Dec., 1605
 1960: 22 Apr., 1255

Kern Co.

1959: 23 Oct., 1126; 4 Dec., 1594
 1960: 7 Oct., 964

Microchemical Specialties Co.

1960: 15 Jan., 169; 18 Mar., 851; 20 May, 1551; 17 June, 1841

National Instrument Laboratories, Inc.

1959: 23 Oct., 1032
 1960: 18 Mar., 760

Perkin-Elmer Corp.

1959: 23 Oct., 1000

Photovolt Corp.

1959: 13 Nov., 1361; 20 Nov., 1431; 18 Dec., 1717

1960: 29 Jan., 307; 12 Feb., 425; 19 Feb., 527; 18 Mar., 857; 22 Apr., 1231; 20 May, 1559; 17 June, 1825; 22 July, 245; 26 Aug., 563; 23 Sept., 839

Schuler and Co., Schuco Scientific Div.

1960: 19 Feb., 565; 23 Sept., 814

EVAPORATORS

**Buchler Instruments, Inc., formerly
 Laboratory Glass & Instrument Corp.**

1959: 23 Oct., 1115
 1960: 22 Jan., 180; 19 Feb., 460; 22 Apr., 1244; 20 May, 1565

Instrumentation Associates

1960: 18 Mar., 846

EXTRACTORS

VirTis Co., Inc.

1960: 22 July, 180

FERMENTOR DRIVE ASSEMBLY

New Brunswick Scientific Co., Inc.

1959: 2 Oct., 873; 6 Nov., 1268
 1960: 15 Jan., 165; 25 Mar., 943

FILM, INTERFERENCE

Fish-Schurman Corp.

1960: 20 May, 1542

FILM, BADGES

**Nuclear Corporation of America,
 Isotopes Specialties Co.**

1960: 26 Aug., 577

FILTERS

Custom Scientific Instruments, Inc.

1960: 22 Jan., 234; 22 July, 236; 23 Sept., 834

Millipore Filter Corp.

1959: 23 Oct., 1140; 13 Nov., 1362; 20 Nov., 1430; 4 Dec., 1602

1960: 22 Apr., 1257

Reeve Angel

1960: 23 Sept., 768

Schleicher, Carl, & Schuell. Co.

1960: 22 Apr., 1264

FILTERS, INTERFERENCE

Baird-Atomic, Inc.

1959: 4 Dec., 1603
 1960: 19 Feb., 531; 18 Mar., 792; 23 Sept., 765

Bausch & Lomb Optical Co.

1960: 12 Feb., 384

Fish-Schurman Corp.

1959: 23 Oct., 1141

1960: 19 Feb., 545; 22 Apr., 1236; 20 May, 1542

Photovolt Corp.

1959: 30 Oct., 1203; 4 Dec., 1589

1960: 1 Apr., 993; 8 July, 97; 2 Sept., 627

FILTER PAPER

New York Laboratory Supply Co., Inc.

1959: 20 Nov., 1431

1960: 18 Mar., 863

Reeve Angel

1960: 19 Feb., 454; 20 May, 1481

Schleicher, Carl, & Schuell Co.

1959: 23 Oct., 1133; 13 Nov., 1357; 4 Dec., 1598

1960: 22 Apr., 1264; 13 May, 1402; 17 June, 1816

FLASKS

Belco Glass, Inc.

1959: 4 Dec., 1507; 18 Dec., 1713

1960: 8 Jan., 113; 22 Jan., 255; 5 Feb., 368; 19 Feb., 539; 3 June, 1689; 17 June, 1842; 8 July, 94; 9 Sept., 684; 7 Oct., 970

Corning Glass Works

1960: 11 Mar., 745; 8 Apr., 1011; 8 July, 100

Doerr Glass Co.

1959: 13 Nov., 1283

F & M Scientific Corp.

1960: 18 Mar., 766; 20 May, 1486; 23 Sept., 827

Falcon Plastics Co.

1960: 1 July, 5

Kimble Glass Co.

1960: 15 Jan., 123; 22 Jan., 183; 11 Mar., 689

Kontes Glass Co.

1959: 23 Oct., 1120

1960: 22 Jan., 253; 19 Feb., 558; 18 Mar., 859; 22 Apr., 1228

FLOWMETERS, GAS

Matheson Co., Inc.

1959: 23 Oct., 1125

FLUOROMETERS

Coleman Instruments, Inc.

1959: 23 Oct., 1047

Farrand Optical Co., Inc.

1959: 23 Oct., 1116; 13 Nov., 1361; 4 Dec., 1607

1960: 18 Mar., 844; 22 Apr., 1251; 22 July, 235; 26 Aug., 571; 23 Sept., 821

Klett Manufacturing Co.

1959: 9 Oct., 931; 23 Oct., 1132; 20 Nov., 1432; 18 Dec., 1717; 25 Dec., 1767

1960: 1 Jan., 47; 29 Jan., 305; 11 Mar., 747; 25 Mar., 945; 22 Apr., 1236; 10 June, 1746; 17 June, 1833; 26 Aug., 575; 9 Sept., 686

Perkin-Elmer Corp., Instrument Div.

1960: 15 Jan., 124

Photovolt Corp.

1959: 6 Nov., 1271

1960: 15 Jan., 165; 26 Feb., 613; 11 Mar., 747; 15 Apr., 1109; 13 May, 1457; 27 May, 1628; 24 June, 1896; 1 July, 47; 19 Aug., 477; 16 Sept., 749

Thomas, Arthur H., Co.


1960: 18 Mar., 888; 22 July, 260; 16 Sept., 752

Will Corp.

1960: 19 Feb., 561

21 OCTOBER 1960

CANALCO ANALYZERS TAKE THE LABOR OUT OF LABORATORY

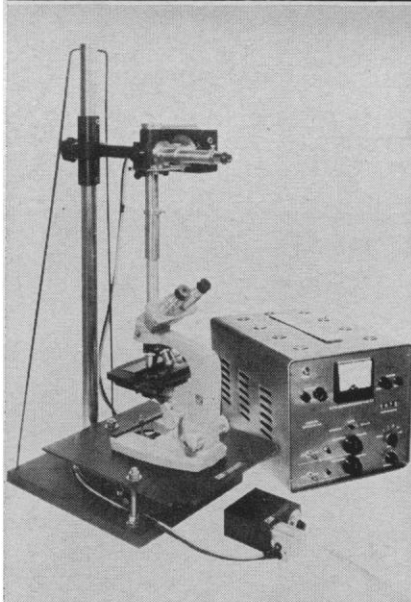

IN MICRO-CHEMISTRY

the new


Ultra-Microspectrophotometer

Ultra-Microspectrophotometer gives fully automated quantitation, in both the visible and the U.V. for

- cell components
- tissue extracts
- fluorescence
- micro-liquids (10-50 ul)
- interference microscopy
- autoradiographs
- micro-chromatography (10 ul flow cuvettes)

Two Models

1. Digital Ratio Reporter, for one and two wavelength analysis
2. Absorption Curve Computer, for spectral curve recording

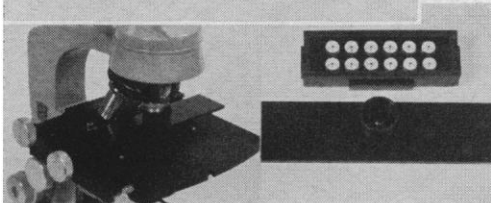

Micro-chemical Cuvettes


... IN FRACTION ANALYZING

Base Compensating U.V. Flow Analyzer

For automatic location and measurement of ultraviolet-absorbing materials in flow, with flat base line and full sensitivity maintained in the presence of U.V.-absorbing solvents. For use in column chromatography and other flow systems.

FIVE MODELS for . . .

- broadly absorbing materials
- specific wavelengths
- monochromatic density studies
- 260/280 ratios
- simultaneous monitoring of one to eight columns at one or more wavelengths.

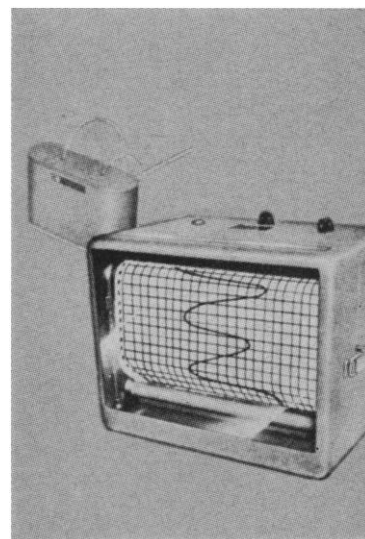

**CANAL
INDUSTRIAL
CORPORATION**

Dept. SO/4940 St. Elmo Avenue, Bethesda 14, Maryland

Freeing the Scientist for Science

FRACTIONATORS

E-C Apparatus Co.

1959: 2 Oct., 869; 4 Dec., 1605

Gilson Medical Electronics

1959: 13 Nov., 1367

1960: 18 Mar., 849

FRACTION COLLECTORS AND ACCESSORIES

Buchler Instruments, Inc., formerly Laboratory Glass & Instrument Corp.

1960: 22 Jan., 180; 19 Feb. 460; 22 Apr., 1221; 9 Sept., 684

Gilson Medical Electronics

1959: 13 Nov., 1367

1960: 12 Feb., 427; 18 Mar., 849

Hamilton Co., Inc.

1959: 13 Nov., 1358

1960: 19 Feb., 544; 24 June, 1897

Microchemical Specialties Co.

1959: 4 Dec., 1608

National Instrument Laboratories, Inc.

1960: 22 Jan., 251; 22 Apr., 1255

Packard Instrument Co., Inc.

1960: 1 Apr., 958; 27 May, 1582; 22

July, 190; 2 Sept., 590

Schaar and Co.

1960: 20 May, 1557

FREEZE-DRYING EQUIPMENT

American Hospital Supply Corp.,

Scientific Products Div.

1959: 4 Dec., 1521

American Sterilizer Co.

1960: 22 July, 177; 26 Aug., 509; 23 Sept., 761

Buchler Instruments, Inc., formerly Laboratory Glass & Instrument Corp.

1960: 18 Mar., 875; 22 Apr., 1231

Repp Industries, Inc.

1960: 19 Feb., 446; 22 Apr., 1122; 26 Aug., 501

Scientific Glass Apparatus Co., Inc.

1960: 25 Mar., 942

VirTis Co., Inc.

1959: 23 Oct., 1038

1960: 22 Jan., 184; 18 Mar., 771; 23 Sept., 762

FUME HOODS

Aloe, A. S., Co., Aloe Scientific Div.

1960: 18 Mar., 879

Blickman, S., Inc.

1960: 20 May, 1557

FUNNELS

Nalge Co., Inc.

1960: 1 Apr., 995

VirTis Co., Inc.

1960: 22 July, 180

Will Corp.

1960: 22 Apr., 1267; 27 May, 1625

FURNACES

Hevi-Duty Electric Co.

1959: 23 Oct., 1124; 4 Dec., 1592

1960: 19 Feb., 542; 15 July, 156

Lindberg Engineering Co.

1960: 22 Apr., 1236; 20 May, 1565

New York Laboratory Supply Co., Inc.

1959: 20 Nov., 1431

Thermo Electric Manufacturing Co.

1959: 23 Oct., 1121; 4 Dec., 1585

FURNITURE, LABORATORY

Ajusto Equipment Co.

1960: 23 Sept., 846

Aloe, A. S., Co., Aloe Scientific Div.

1960: 18 Mar., 879

Blickman, S., Inc.

1960: 23 Sept., 830

Brinkmann Instruments, Inc.

1959: 27 Nov., 1486; 25 Dec., 1767

Brunswick-Balke-Collender Co.

1960: 17 June, 1835

Central Scientific Co.

1960: 12 Aug., 425

Duralab Equipment Corp.

1960: 18 Mar., 881; 17 June, 1827; 23 Sept., 840

Fisher Scientific Co.

1959: 16 Oct., 992

1960: 22 Jan., 189

Graphic Systems

1959: 13 Nov., 1354

1960: 22 Jan., 242; 18 Mar., 870; 20 May, 1554; 22 July, 242; 23 Sept., 845

Harshaw Chemical Co.

1959: 23 Oct., 1112; 13 Nov., 1346

1960: 8 Jan., 112; 29 Jan., 306

Johns-Manville

1959: 9 Oct., 887; 6 Nov., 1215; 4 Dec., 1523

Kewaunee Scientific Equipment


1960: 19 Feb., 536

LABASCO

1960: 17 June, 1818; 23 Sept., 820

Laboratory Construction Co.

1960: 23 Sept., 814

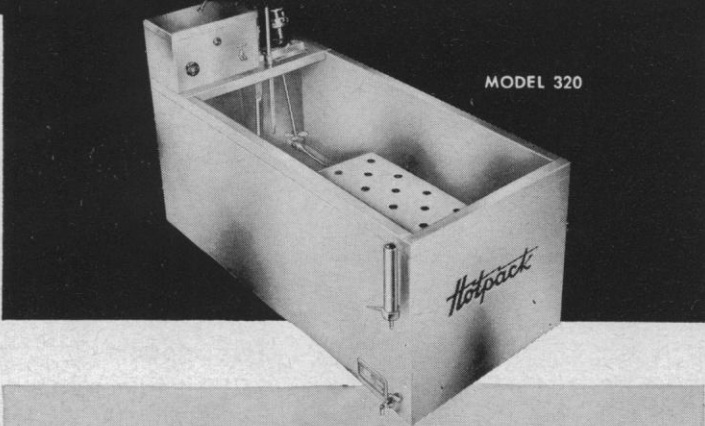


**HOTPACK'S LABORATORY BATH
GIVES YOU ABSOLUTE CONTROL**


... ACCURATE, ADJUSTABLE THERMOSTAT
AUTOMATICALLY REGULATES BATH
TEMPERATURES FROM AMBIENT TO
125°C OR 0° TO 60°C (REFRIG)
WITHIN $\pm 0.2^\circ\text{C}$

Hotpack's quality engineered
baths offer precisely-controlled, uniform
temperatures for many laboratory cooling, heating
and mixing requirements! A unique double-bank of
heaters — individually controlled — bring operating
temperatures quickly ... eliminate excessive differentials.
Override, too, is prevented. Optional, built-in copper
cooling coils lower fluid temperatures rapidly
below ambient ... ideally suited for low temperature
processing! And a specially mounted motor stirrer
agitates fluids evenly throughout open bath
area ... you get optimum liquid uniformity.
Every Hotpack bath is constructed of heavy duty
stainless steel, and equipped with s/s tray, thermometer
and mercurial thermostat ... tailor made for economy
and protection in many tough applications!


For complete bath information write to:



ENVIRONMENTAL ROOM



HUMIDITY OVEN




INCUBATOR

5086 COTTMAN AVENUE • PHILADELPHIA 35, PA.

ATOMIC ABSORPTION INSTRUMENTATION provides greater scope than flame photometry

This new Hilger & Watts equipment now offers an analytical method virtually free from inter-element interference. Its accuracy is largely unaffected by flame temperature—the technique generally needs only one working curve per element.

Atomic absorption spectroscopy approaches the ideal more closely than any other method and has been tested effectively in many diverse fields.

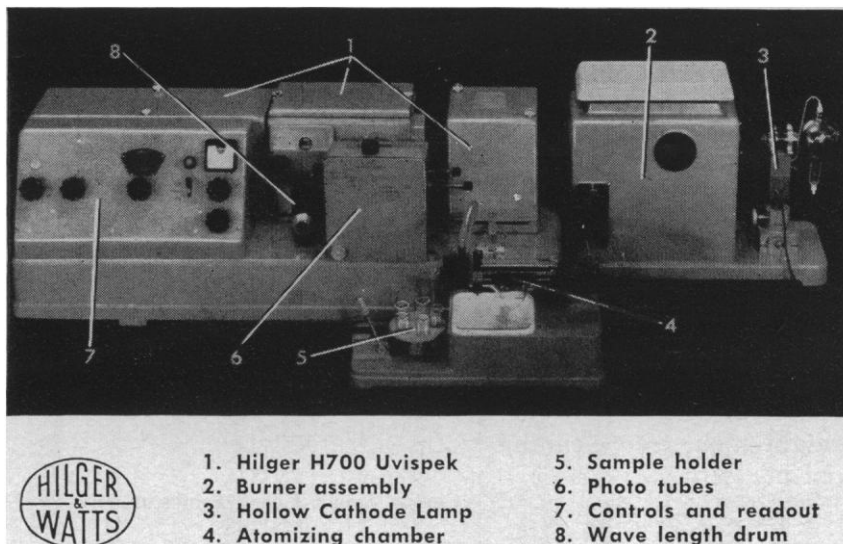


For additional information concerning this new equipment, ask for Catalog CH 407

ENGIS EQUIPMENT COMPANY

AFFILIATED WITH HILGER & WATTS, INC.

431 SOUTH DEARBORN STREET CHICAGO 5, ILLINOIS TELEPHONE: HARRISON 7-3223

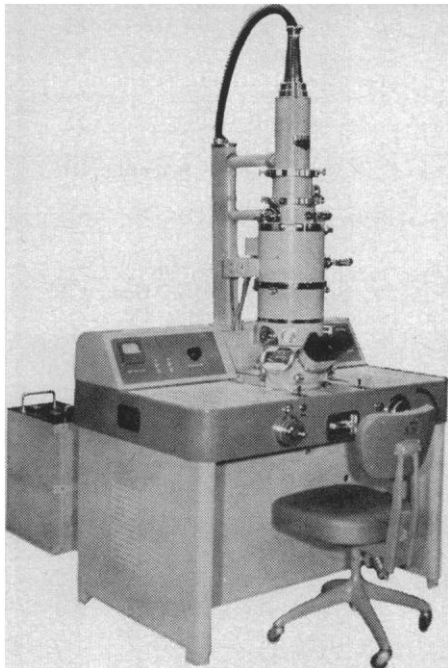

the HITACHI HS-6 ELECTRON MICROSCOPE

The Hitachi HS-6 permanent magnet Electron Microscope provides a continuously variable magnification range of 200x to 28,000x. Focusing is achieved by altering the magnetic flux of the objective lens leaving the accelerating voltage unchanged.

One of the outstanding features of the Hitachi HS-6 is the guaranteed resolution of 20 Angstrom Units or better. The simplicity of operation, mechanics and circuitry makes the HS-6 an ideal Electron Microscope for the researcher in medical and biological fields.


Your inquiries are invited at either our West Coast or East Coast offices, where competent sales personnel will answer your questions, and arrange a demonstration.

ERB & GRAY SCIENTIFIC, Inc.

Exclusive Hitachi Distributors for the U. S.

854 S. Figueroa St., Los Angeles 17, Calif.

501 Fifth Ave., New York 17, N.Y.

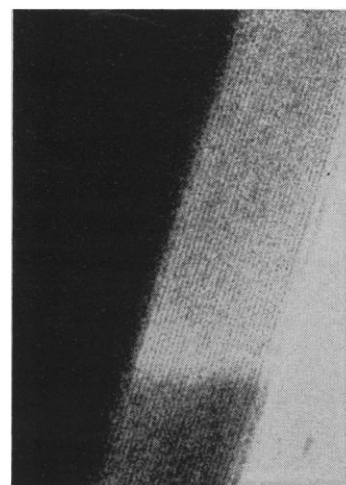

Illustrated is a microphotograph of Cu-phthalocyanine, taken at 30,000X electronic magnification with the HS-6!



TOO MANY VARIABLES?

It's time to draw a line.
Straighten out your cleaning problems with

HAEMO-SOL

There's nothing like Haemo-Sol's unique cleansing power and positive rinsing . . . it's completely safe! No etching! No corroding of metal parts! Immediate Haemo-Sol bath for valuable volumetric and optical equipment prevents soil etching!

Haemo-Sol guarantees clean laboratory glassware and apparatus—

- removes the full range of laboratory soils
- effectively digests protenoid materials . . . other types of polymeric materials
- assures free draining pipets . . . burets
- gives sparkling clear surfaces for quartz and glass absorption cells
- provides chemically clean reaction and titration flasks
- leaves the clean surfaces that are a must for the smooth operation of fractionating columns and other pieces of laboratory equipment.

And, just as important as its unique cleaning power, is Haemo-Sol's *high solubility* and powerful solubilizing action. Haemo-Sol washed glassware *rinses completely clean . . . nothing remains behind* but a chemically clean, free draining glass surface.



Write
**TODAY for
Sample and
Literature.**

Distributed by

MEINECKE & CO., INC.

225 Varick Street
New York 14



Lab-Tek Plastics Co.
1959: 23 Oct., 1122; 4 Dec., 1582
Metalab Equipment Co.
1960: 19 Feb., 547
Will Corp.
1960: 20 May, 1516, 1517

GALVANOMETERS

Cambridge Instrument Co., Inc.
1960: 23 Sept., 830
Photovolt Corp.
1959: 27 Nov., 1486; 25 Dec., 1767
1960: 22 Jan., 251; 8 Apr., 1055; 13 May, 1457; 15 July, 160
Texas Instruments, Inc.
1960: 18 Mar., 887

GAMMA IRRADIATORS

Atomic Energy of Canada Limited
1959: 23 Oct., 1008; 4 Dec., 1520
1960: 22 Jan., 178; 18 Mar., 782; 22 Apr., 1150; 20 May, 1488
Budd Co.
1960: 9 Oct., 935
Curtiss-Wright Corp., Princeton Div.
1959: 23 Oct., 1143
Victoreen Instrument Co.
1959: 23 Oct., 1131
1960: 22 Jan., 252; 19 Feb., 557; 29 Apr., 1284; 20 May, 1490

GAS CONTAINERS

Union Carbide Corp., Linde Co. Div.
1959: 18 Dec., 1718
1960: 22 Apr., 1262; 12 Aug., 426; 7 Oct., 962

GAS FLOW CONTROL DEVICES

Granville-Phillips Co.
1960: 7 Oct., 970

GAS METERS

Thomas, Arthur H., Co.
1959: 2 Oct., 876

GAUGES, VACUUM

Ace Glass, Inc.
1960: 22 July, 237
Central Scientific Co.
1959: 27 Nov., 1485
Greiner, Emil, Co.
1960: 23 Sept., 853
New York Air Brake Co., Kinney Vacuum Div.
1960: 19 Feb., 533; 18 Mar., 849; 22 Apr., 1225; 17 June, 1819; 19 Aug., 483
Smith, Arthur F., Inc.
1960: 17 June, 1844; 7 Oct., 968

GAUSSMETERS

Harvey-Wells Electronics, Inc.
1960: 17 June, 1825

GLASS, PLASTIC COATED

Ace Glass, Inc.
1960: 19 Feb., 529

GLASS CUTTERS

Standard Scientific Supply Corp.
1960: 18 Mar., 862

THE NEXT TIME YOU ORDER ORGANICS

We hope, the next time you order organics, you'll specify MC&B. We think there are some pretty fair advantages in specifying our chemicals. For example—
Convenience—the best Distributor Network in the business
Dependable Purity—Each lot checked to maintain purity
Complete Line—Over 4400 laboratory chemicals. Write for Catalog.
Will you specify MC&B the next time? We'll appreciate the business, and so will our good distributors.



Matheson Coleman & Bell
Division of The Matheson
Company, Norwood
(Cincinnati), Ohio;
East Rutherford,
New Jersey

Welch, W. M., Manufacturing Co.
1960: 1 Apr., 993; 2 Sept., 627

GLASSBLOWING KIT

Bethlehem Apparatus Co., Inc.
1960: 17 June, 1832; 22 July, 234; 26 Aug., 560

GLASSWARE AND ACCESSORIES

Ace Glass, Inc.
1960: 22 Jan., 247; 19 Feb., 529; 18 Mar., 855; 20 May, 1547

Bellco Glass, Inc.
1959: 4 Dec., 1507; 18 Dec., 1713
1960: 8 Jan., 113; 22 Jan., 255; 22 Apr., 1243; 6 May, 1385; 8 July, 94; 5 Aug., 367; 19 Aug., 482; 9 Sept., 684; 23 Sept., 850; 7 Oct., 970

Corning Glass Works
1959: 9 Oct., 891; 6 Nov., 1265; 13 Nov., 1349; 4 Dec., 1527
1960: 5 Feb., 322, 323; 11 Mar., 745; 3 June, 1636; 8 July, 100; 5 Aug., 320; 9 Sept., 687

Doerr Glass Co.
1959: 9 Oct., 883; 13 Nov., 1283; 4 Dec., 1499

1960: 26 Feb., 573; 18 Mar., 759; 15 Apr., 1067; 13 May, 1403; 16 Sept., 700

Fischer & Porter Co.
1959: 13 Nov., 1287
1960: 22 Jan., 194; 19 Feb., 457

Harshaw Chemical Co.
1959: 23 Oct., 1112; 13 Nov., 1346
1960: 8 Jan., 112; 29 Jan., 306

Kimble Glass Co.
1959: 2 Oct., 823; 30 Oct., 1164; 6 Nov., 1222; 20 Nov., 1375; 4 Dec., 1519; 18 Dec., 1675

1960: 15 Jan., 123; 22 Jan., 183; 11 Mar., 689; 15 Apr., 1072; 10 June, 1701; 8 July, 58; 9 Sept., 639

Klett Manufacturing Co.
1959: 2 Oct., 867; 16 Oct., 988; 23 Oct., 1132; 6 Nov., 1269; 13 Nov., 1347; 20 Nov., 1432; 27 Nov., 1486; 4 Dec., 1597; 11 Dec., 1665; 18 Dec., 1717

1960: 1 Jan., 47; 8 Jan., 115; 15 Jan., 165; 22 Jan., 243; 29 Jan., 305; 5 Feb., 368; 12 Feb., 425; 4 Mar., 676; 11 Mar., 747; 1 Apr., 997; 8 Apr., 1051; 15 Apr., 1106; 22 Apr., 1236; 29 Apr., 1325; 13 May, 1452; 20 May, 1552; 27 May, 1626; 3 June, 1687; 10 June, 1746; 17 June, 1833; 24 June, 1896; 1 July, 47; 15 July, 159; 22 July, 254; 29 July, 311; 12 Aug., 429; 19 Aug., 477; 26 Aug., 575; 2 Sept., 628; 9 Sept., 686; 16 Sept., 747; 23 Sept., 850; 30 Sept., 905

Kontes Glass Co.
1959: 2 Oct., 826; 16 Oct., 985; 23 Oct., 1120; 30 Oct., 1204; 6 Nov., 1220; 13 Nov., 1366; 4 Dec., 1588

1960: 22 Jan., 253; 19 Feb., 558; 22 Apr., 1228

Microchemical Specialties Co.

1960: 22 Apr., 1222

Scientific Glass Apparatus Co., Inc.

1959: 23 Oct., 1026

1960: 19 Feb., 466


Thomas, Arthur H., Co.

1960: 15 Apr., 1112

GLOVES, DRY BOX

Charleston Rubber Co.
1960: 19 Feb., 534

HR-92 X-Y RECORDER

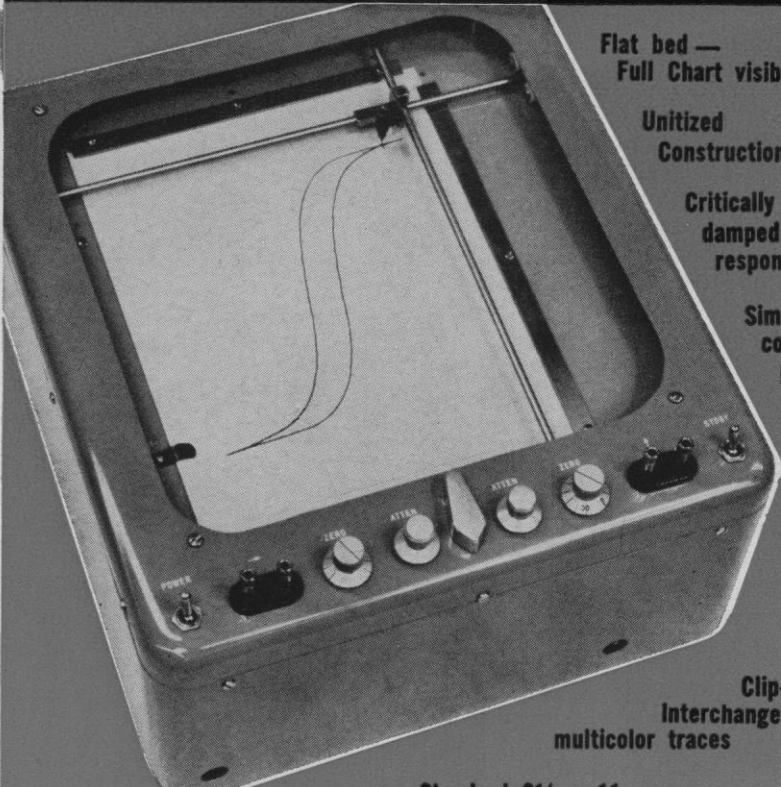

Flat bed —
Full Chart visibility

Unitized
Construction

Critically
damped
response

Simplified
control
panel

Clip-on pen —
Interchangeable for
multicolor traces

Standard 8½ x 11 paper


Unconditionally guaranteed for one year.

RUGGED "All Purpose" X-Y RECORDER

The HR-92 is a null-seeking servo-type plotter designed to draw curves in Cartesian coordinates on regular 8½ x 11 graph paper. It employs conventional chopper amplifiers, 2-phase motors and a potentiometer rebalance. Reference voltages are furnished by mercury cells. Control panel has zero set and continuously-variable attenuator for each axis. Separate standby and power switches are provided. The two axes are electrically and mechanically independent. By moving an internal jumper lead, a high impedance potentiometer input can be made available.

SPECIAL FEATURES:

- Amplifiers easily removed if servicing ever becomes necessary. Electrical connections all contained in two plugs for each amplifier.
- Each amplifier channel (including transformer power supply) independent of rest of system.



houston instrument corporation
4950 TERMINAL AVE., HOUSTON 27, TEXAS
MOhawk 7-7405

GLOVES, POLYETHYLENE

Research Associates, Inc.
1960: 20 May, 1568

GONIOMETERS

LaPine, Arthur S., and Co.
1690: 22 Apr., 1229

GROWTH CHAMBERS

American Sterilizer Co.
1960: 22 July, 177; 23 Sept., 761
Delmar Scientific Laboratories
1959: 23 Oct., 1028
Labline, Inc.
1960: 20 May, 1545

National Appliance Co.

1960: 20 May, 1539

GYROSCOPES

Central Scientific Co.
1959: 30 Oct., 1203; 4 Dec., 1581

HAND TORCHES

Bethlehem Apparatus Co., Inc.
1960: 20 May, 1556

HEATERS

Research Specialties Co.
1959: 16 Oct., 986

Scientific Glass Apparatus Co., Inc.

1960: 25 Mar., 942

Thermo Electric Manufacturing Co.

1959: 23 Oct., 1121

HEATING TAPES

Standard Scientific Supply Corp.
1960: 22 July, 256

HOMOGENIZERS

Instrumentation Associates
1960: 22 Apr., 1248
Sorvall, Ivan, Inc.
1960: 20 May, 1561; 22 July, 231; 26 Aug., 567
Tri-R Instruments
1959: 23 Oct., 1137
1960: 19 Feb., 555
VirTis Co., Inc.
1959: 23 Oct., 1038
1960: 20 May, 1476; 17 June, 1773

HOT PLATES

Central Scientific Co.
1960: 26 Feb., 619; 17 June, 1838
Lindberg Engineering Co., Laboratory Equipment Div.
1960: 22 Jan., 237
Precision Scientific Co.
1960: 19 Feb., 527
Thermo Electric Manufacturing Co.
1959: 23 Oct., 1121

ILLUMINATORS

American Optical Co.
1960: 26 Feb., 622; 23 Sept., 856
Bausch & Lomb Optical Co.
1960: 26 Feb., 578
Burton Manufacturing Co.
1959: 23 Oct., 1152
1960: 19 Feb., 552; 22 Apr., 1224
Hacker, William J., & Co., Inc.
1960: 22 Apr., 1126

INCINERATORS

Phipps & Bird, Inc.
1960: 26 Aug., 575

INCUBATORS

National Appliance Co.
1959: 23 Oct., 1118
1960: 5 Feb., 362; 6 May, 1388; 26 Aug., 556; 23 Sept., 847
Precision Scientific Co.
1959: 4 Dec., 1588
1960: 18 Mar., 846; 20 May, 1540; 26 Aug., 568

INFUSION APPARATUS

Will Corp., Bronwill Scientific Div.
1960: 10 June, 1749; 23 Sept., 849

INJECTORS

Foringer & Co., Inc.
1960: 7 Oct., 971

INTERFEROMETERS

Central Scientific Co.
1959: 11 Dec., 1666
1960: 15 Jan., 164; 17 June, 1833

GAS CHROMATOGRAPHY SYSTEMS

Flexible and expandable to fit your needs

FOR TODAY'S EXACTING ANALYSES

RSCo Modular Systems are employed for their outstanding versatility and operational convenience in numerous government, university and industrial laboratories.

There is a high quality module for every major function in gas chromatography. Start with ones for your present needs and add to the system as other needs arise.

FOR TOMORROW'S IMPROVED METHODS

RSCo Modular Systems give unequaled ease of expansion with space for internal accessories, connections of external modules.

You buy progress, not obsolescence, with RSCo Modular Systems.

Send for your key to complete flexibility in gas chromatography — our 69-page catalog of Gas Chromatography Equipment.




RESEARCH SPECIALTIES CO.

200 South Garrard Boulevard, Richmond, California


22 types of SAFETY ENCLOSURES for handling hazardous substances

VACUUM DRY BOX

for work in controlled atmosphere
• sloping front •
round autoclave-type air lock.

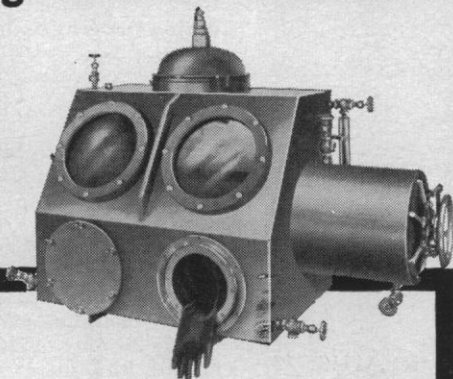

Safety is the first consideration in this newly-designed stainless steel laboratory equipment. These enclosures make it safer—and easier—for the technician to work with contaminants, micro-organisms, live viruses, infected animals, poisonous and radioactive substances. Stainless steel constructed with crevice-free surfaces, generously rounded corners, for easy cleaning and decontamination. Write for illustrated folder describing 22 different kinds of enclosures. S. BLICKMAN, INC., 6910 GREGORY AVENUE, WEEHAWKEN, N. J.


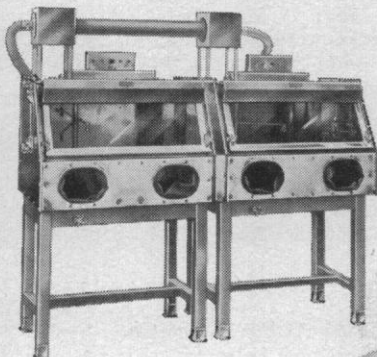


UNITIZED ENCLOSURES

Low in cost •
Stainless steel •
Modular
construction
adapts to many
uses.

CALIFORNIA-TYPE FUME HOOD

For handling radioactive materials • dual-sided for double operation.

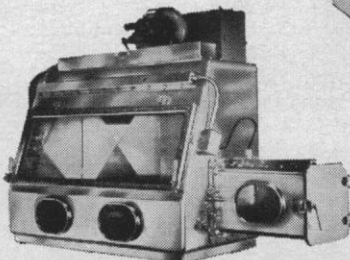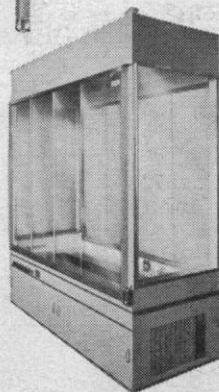

MICRO-BIOLOGICAL SAFETY CABINET

Back or top mounting of biological filter canister • air lock if wanted.

BLICKMAN SAFETY ENCLOSURES

Look for this symbol of quality

Blickman-Built



Kinney®
PRESENTS
A NEW AND
BETTER
MCLEOD
GAGE

READS
EASIER



USES LESS
MERCURY



PANEL OR
PORTABLE
MOUNT



SEPARATE
CAPILLARIES



2 SCALES
150 mm to 2 mm
2,000 μ to 1 μ



ACCURATE
LIGHT IN WEIGHT
COMPACT

The KINNEY McLeod Gage answers the many objections to other gages now in use. Its advanced design compacts superior performance into a rugged, versatile instrument that may be permanently mounted on bracket, tank, panel or pipe or, by affixing demountable legs, used as a portable unit.

The KINNEY McLeod Gage covers a broad range of pressures . . . accurate readings from 150 mm Hg to 1 Micron Hg. This exceptional range of pressure readings is achieved by incorporating two separate capillaries having separate compression ratios, making available measurements of 150 mm to 2 mm and 2,000 microns to 1 micron. Unlike other McLeod Gages, the reading capillary tubes are completely separate and replaceable—easily detached from the main body at the knurled sealing glands. Because these tubes are reproducible, complete accuracy between each gage is assured.

The KINNEY McLeod Gage requires less mercury and it is supremely simple to add mercury, remove it for cleaning or recharge the gage. Operation requires no special skill . . . readings are achieved quickly, easily and confidently. Write for full information and prices today.

Get all the facts on the NEW KINNEY McLEOD GAGE. Write today!

KINNEY VACUUM DIVISION
THE NEW YORK AIR BRAKE COMPANY

3538K WASHINGTON STREET • BOSTON 30 • MASS.

Please send me Bulletin No. 3821.1 and prices on the KINNEY McLeod Gage.


Name _____

Company _____

Address _____

City _____ State _____

EATON - DIKEMAN FILTER PAPER Used in 7 out of 10 laboratories

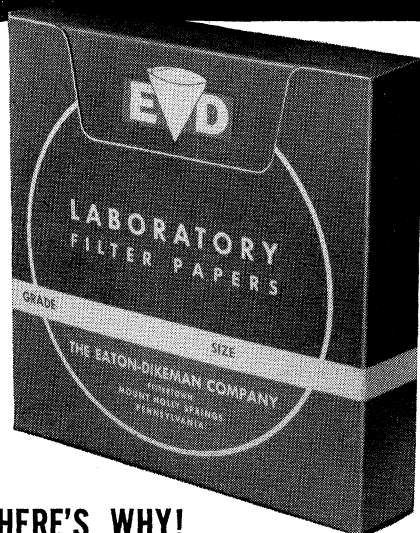

HERE'S WHY!

- **Complete range** — whatever rapidity, and retention characteristics you desire, chances are there's a standard E-D paper available. Made with smooth or creped surfaces, in plain or fluted circles, in strips, or rolls, or cut to your individual requirements.
- **Highest purity** — only the purest pulp available is used.
- **Uniform quality** — every step of the manufacturing process is carefully controlled and checked.
- **Excellent wet strength** — special resins incorporated.
- **Complete technical service** — whatever your filtering problem may be, Eaton-Dikeman with its broad background of more than seventy years of manufacturing filter papers exclusively, can probably solve it.

Also available—papers for chromatography and electrophoresis, as well as bibulous and lens papers. Write for free samples.



EATON-DIKEMAN CO.
Mount Holly Springs, Pennsylvania

KYMOGRAPHS AND ACCESSORIES

Phipps & Bird, Inc.

1959: 23 Oct., 1109; 13 Nov., 1367; 4 Dec., 1607

1960: 4 Mar., 675; 11 Mar., 743; 25 Mar., 943; 1 Apr., 997; 8 Apr., 1051; 10 June, 1743; 17 June, 1842; 24 June, 1893; 1 July, 51; 8 July, 94; 15 July, 161; 7 Oct., 967

LABELS, TIME

Professional Tape Co., Inc.

1960: 4 Mar., 675; 11 Mar., 744; 18 Mar., 873; 25 Mar., 938; 1 Apr., 993; 29 Apr., 1327; 6 May, 1386; 27 May, 1626; 3 June, 1684; 24 June, 1893; 2 Sept., 628; 23 Sept., 846; 7 Oct., 972

LABELS, MICROSCOPIC SLIDE

Professional Tape Co., Inc.

1959: 16 Oct., 987; 23 Oct., 1113; 13 Nov., 1368; 20 Nov., 1437; 4 Dec., 1583; 11 Dec., 1663

1960: 8 Jan., 113; 22 Jan., 243; 5 Feb., 365; 19 Feb., 549; 11 Mar., 743; 25 Mar., 941; 15 Apr., 1106; 20 May, 1537; 17 June, 1823; 16 Sept., 749

LABORATORY EQUIPMENT

Analytical Equipment, Inc.

1959: 23 Oct., 1144

Fisher Scientific Co.

1959: 23 Oct., 1020

1960: 20 May, 1571; 23 Sept., 777

Standard Scientific Supply Corp.

1960: 7 Oct., 966

Will Corp.

1959: 23 Oct., 1127

1960: 20 May, 1516, 1517

LABORATORY EQUIPMENT, PLASTIC

Bel-Art Products

1960: 19 Feb., 555

Burdick & Jackson Laboratories

1960: 22 Apr., 1259

Falcon Plastics Co.

1959: 23 Oct., 1035

1960: 19 Feb., 534; 24 June, 1860; 1 July, 5

Nalge Co., Inc.

1960: 19 Feb., 532; 18 Mar., 872; 22 Apr., 1227; 20 May, 1564; 1 Apr., 995; 17 June, 1824; 22 July, 248; 26 Aug., 570; 23 Sept., 824

Thomas, Arthur H., Co.

1959: 18 Dec., 1714

LABORATORY JACK

Central Scientific Co.

1959: 23 Oct., 1144; 18 Dec., 1713

LAMPS

Aristo Grid Lamp Products, Inc.

1960: 22 Apr., 1252

Ultra-Violet Products, Inc.

1959: 23 Oct., 1151; 4 Dec., 1592

MACHINE TOOLS

American-Edelstaal Unimat Division

1959: 23 Oct., 1118; 13 Nov., 1365; 4 Dec., 1593; 11 Dec., 1667

1960: 22 Jan., 244; 19 Feb., 542; 18 Mar., 874; 17 June, 1840; 22 July, 246; 26 Aug., 562

MACROSCOPES

Bausch & Lomb Optical Co.

1959: 23 Oct., 1050; 4 Dec., 1534

1960: 29 Jan., 268; 1 July, 8

Ednalite Optical Co., Inc.

1959: 4 Dec., 1504

MANIKIN, RADIATION-EQUIVALENT

Atomic Accessories, Inc.

1959: 23 Oct., 1004

MANOMETERS

Ace Glass, Inc.

1960: 22 July, 237

Greiner, Emil, Co.

1960: 20 May, 1556

Phipps & Bird, Inc.

1959: 23 Oct., 1109

MATERIALS TESTING EQUIPMENT

Instron Engineering Corp.

1960: 18 Mar., 839; 22 Apr., 1140; 24 June, 1899

MEASURING EQUIPMENT, PHYSIOLOGICAL

American Hospital Supply Corp.

1960: 18 Mar., 761

Beckman Instruments, Inc., Spinco Div.

1960: 8 July, 54; 9 Sept., 634

Biophysical Electronics

1960: 19 Feb., 556; 22 Apr., 1252; 20 May, 1562

Precision Instrument Co.

1960: 17 June, 1822; 22 July, 255

Riseman Development Laboratory

1960: 26 Aug., 572; 23 Sept., 850

MELTING POINT APPARATUS

LaPine, Arthur S., and Co.

1960: 19 Feb., 560; 22 Apr., 1229; 17 June, 1840

Standard Scientific Supply Corp.

1960: 23 Sept., 842

Thomas, Arthur H., Co.

1959: 23 Oct., 998

MICROANALYSIS EQUIPMENT

Ace Glass, Inc.

1960: 20 May, 1547

Aloe, A. S., Co., Aloe Scientific Div.

1959: 4 Dec., 1600

1960: 5 Feb., 365

Beckman Instruments, Inc., Spinco Div.

1960: 8 July, 54; 9 Sept., 634

Brinkmann Instruments, Inc.

1959: 13 Nov., 1359

1960: 23 Sept., 770

Brunswick Corp., Aloe Scientific Div.

1960: 22 July, 243

Corning Glass Works

1959: 13 Nov., 1349

Hamilton Co., Inc.

1960: 22 Apr., 1234; 22 July, 253

Harvard Apparatus Co., Inc.

1959: 13 Nov., 1368

Kontes Glass Co.

1959: 2 Oct., 826; 4 Dec., 1588

PHOTOVOLT Electronic pH METERS


A complete line of pH meters, incorporating permanently frictionless taut-suspension indicating meters, modern electronic tubes and circuits. Simple in operation and maintenance; featuring sealed amplifier plug-in units.

Two-way pH Meter Model 85

- Single range 0-14, scale length 3", readable to 0.05 pH Unit.
- Available — compact battery pack for field use (\$38.00 addtl.).
- Fully stabilized, simple, usable with all types of electrodes.

Write for Bulletin #195

\$135



High Precision pH Meter Model 110

- Single range 0-14, scale length 7", readable to 0.02 pH unit.
- Temperature control 0-100° C., voltage selector for 80-260 volts.
- Available — carrying cover and baseboard for bottles, beakers.

Write for Bulletin #105

\$235



Standard Laboratory pH Meter Model 115

- Single range 0-14, scale length 4", readable to 0.05 pH unit.
- Temperature control 20-100° C., available with carrying case.
- Additional millivolt scale for redox measurements and titrations.

Write for Bulletin #225

\$175




Portable pH Meter Model 125

- Single range 0-14, scale length 5½", readable to 0.03 pH unit.
- Only 3 batteries, standard radio type, 2,000 hours of service.
- Available — carrying frame for instrument, beakers, bottles.

Write for Bulletin #118

\$195



Tester Model 25 for Checking and Adjusting pH Meters

A compact, inexpensive instrument without batteries; for checking performance of PHOTOVOLT and other pH meters. Requires neither electrodes nor buffers. Write for Bulletin #138

\$68

**PHOTOVOLT
CORPORATION**

95 Madison Avenue, New York 16, N. Y.

PUMPS FOR PHYSIOLOGICAL RESEARCH

Many phases of physiological research require apparatus which will effect the uniform and predictable flow of liquids and gasses. To meet such situations, Harvard Apparatus Co., Inc., makes available, at the lowest possible cost, an extremely wide range of pumping equipment.

In addition to providing the standard pumps described below, Harvard Apparatus Co., Inc., can also manufacture to order special apparatus needed in unusual situations. Inquiries are invited.

All pumps are made with the same fine workmanship and materials that have characterized the Company's equipment for so many years. Each pump will perform exactly as specified and will give years of trouble-free service.

INFUSION-WITHDRAWAL PUMPS

All pumps in this group are operated by synchronous reversing motors and achieve the transfer of liquids by means of motor-driven mechanisms acting on standard Luer-Lok syringes. The syringe piston is attached to a weighted half-nut which rests on a precision-cut lead screw. As the screw turns, a very uniform intake or discharge of liquid takes place. Pre-set limit stops automatically stop pumping action.

Single, dual and multiple syringe models are available, ranging from simple types designed for either infusion or withdrawal to those performing both operations continuously and automatically over extended periods of time.

Both single and multi-speed models are available. The multi-speed pumps are equipped with a transmission which provides 12 separate speeds and 72 pumping rates using syringes from 50 to 2 cc. size. Single speed units deliver one fixed speed and 6 pumping rates using syringes in the same range of sizes. A range of motors from 1 to 1800 R.P.M. is available.

RESPIRATION PUMPS

These are motor-operated, positive displacement pumps for use with small mammals. Air or gas is drawn into a cylinder in one half of the cycle and delivered to the animal in the next half of the cycle. The stroke volume is adjustable mechanically from 30 to 750 cc. per stroke. A motor-operated slide valve provides separate ports for inspiration and expiration. The expired air may be collected or recycled at the slide valve.

Single and multi-speed models are available. In the latter, motor and speed control box produce rates continuously adjustable from 7 to 50 strokes per minute. The single speed model produces a fixed rate of 22 strokes per minute.

PERISTALTIC PUMPS

These are heavy-duty units achieving the continuous flow of liquids by means of peristaltic action on the outside of rubber tubing.

Catalog 1960-61 and Data Sheets are available on request.



HARVARD APPARATUS CO., INC.

(a non-profit organization)

• Dover, Mass., U.S.A.

GILMONT ULTRAMICROBURETS



newly designed!

Write for Gilmont Ultramicroburet
Descriptive Bulletin

100,000 + 1,000,000 ml

The EMIL GREINER Co.
20-26 N. MOORE STREET NEW YORK 13, N.Y.

**NEW PHOENIX MODEL K-5000-A
AMINO ACID ANALYZER**

**Now Available
For Combined
Analytical—
Preparative
Analysis
With the
MODEL 5500
STREAM
SPLITTING
SYSTEM**



PIP I

PHOENIX PRECISION INSTRUMENT COMPANY

*For complete details
write Dept. K for
Bulletin K 5000-A*

3803-05 NORTH FIFTH ST., PHILADELPHIA 40, PENNSYLVANIA

Macalaster Bicknell Co.
1960: 22 Apr., 1261
Microtech Services Co.
1959: 2 Oct., 872
Phipps & Bird, Inc.
1960: 26 Aug., 575
Sauter, August, of New York, Inc.
1960: 26 Aug., 554
Stoelting, C. H., Co.
1960: 20 May, 1568; 23 Sept., 833
VirTis Co., Inc.
1960: 22 July, 180
Will Corp., Bronwill Scientific Div.
1960: 4 Mar., 676; 15 Apr., 1108; 20 May, 1557; 17 June, 1838; 19 Aug., 489

MICROBIOLOGICAL MEDIA

Colorado Serum Co.
1959: 23 Oct., 1132; 13 Nov., 1363; 4 Dec., 1597
1960: 15 Jan., 165; 19 Feb., 537; 18 Mar., 857; 22 Apr., 1226; 9 Sept., 681
Difco Laboratories
1959: 23 Oct., 1113; 13 Nov., 1351; 18 Dec., 1713
1960: 22 Jan., 255; 19 Feb., 527; 18 Mar., 853; 22 Apr., 1221; 20 May, 1537; 17 June, 1833; 22 July, 239; 26 Aug., 563; 23 Sept., 833
Hyland Laboratories
1960: 22 Jan., 236; 19 Feb., 562; 18 Mar., 876; 22 Apr., 1243; 20 May, 1559; 17 June, 1815; 22 July, 232; 26 Aug., 559; 23 Sept., 817


MICROMANIPULATORS

Aloe, A. S., Co., Aloe Scientific Div.
1959: 4 Dec., 1600
1960: 5 Feb., 365
Brinkmann Instruments, Inc.
1959: 13 Nov., 1359
Brunswick Corp., Aloe Scientific Div.
1960: 22 July, 243
Stoelting, C. H., Co.
1960: 20 May, 1568; 23 Sept., 833

MICROSCOPES

American Optical Co.
1959: 20 Nov., 1440
1960: 29 Jan., 312; 11 Mar., 750; 12 Feb., 432; 17 June, 1848; 26 Aug., 580; 7 Oct., 976
Bausch & Lomb Optical Co.
1959: 18 Dec., 1680
1960: 15 July, 114; 26 Aug., 518
Cooke, Troughton & Simms
1960: 18 Mar., 768; 8 Apr., 1012; 29 Apr., 1276; 20 May, 1469; 12 Aug., 384; 9 Sept., 686; 23 Sept., 767; 7 Oct., 972
Elgeet Optical Co., Inc., Scientific Instrument and Apparatus Div.
1959: 23 Oct., 1016; 4 Dec., 1514
1960: 19 Feb., 465; 22 Apr., 1120; 10 June, 1699; 22 July, 185; 5 Aug., 318; 19 Aug., 491; 2 Sept., 631; 16 Sept., 698; 7 Oct., 914
Graf-Apsco Co.
1959: 13 Nov., 1363
1960: 5 Feb., 365; 18 Mar., 879; 16 Sept., 747
Hacker, William J., & Co., Inc.
1959: 23 Oct., 1010
1960: 22 Jan., 185; 19 Feb., 449; 22 Apr., 1126; 26 Aug., 500; 23 Sept., 763
Lafayette Radio
1959: 23 Oct., 1012

**EASIEST TO
OPERATE**

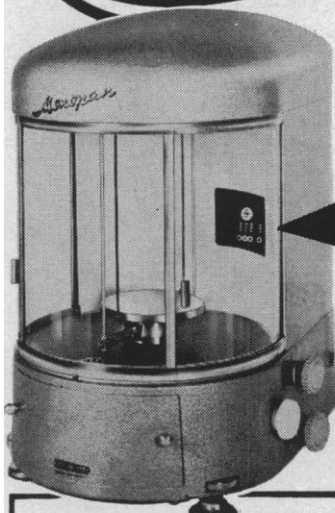


Lowered recessed reading scale eliminates glare. Situated for maximum reading ease in line of vision with load pan.

SAUTER Monopan ANALYTICAL BALANCE

EXCLUSIVE

Monopan weights are in the bottom. Unlike other balances with weights on top, Monopan has no unnecessary swing. With Monopan, all downward force is compensated by equal upward thrust. Since weights are situated within the angle prescribed by pan, oscillation is minimized.

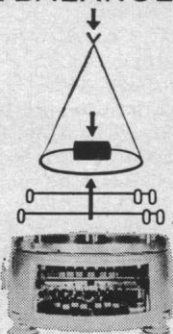

A single pan Analytical Balance making most efficient use of the reliable principle of substitution weighing for the determination of mass.

Very precise • Extremely stable • Remarkably simple.

Several exclusive features:

- Three position arrestment system provides positive locking of weight exchange in "free weighing" position.
- Load pan and substitution weights on separate stirrups minimize oscillation.
- Suspended side sliding doors. No dust-trapping grooves.
- No obstructive front corner posts.
- All controls at base. Operator can rest and steady forearm on table.

Cap.	200 grams
Tare Cap. (add.)	30 grams
Range of opt. scale	110 mg
Readability (per vernier div.)	0.1 mg
Accuracy diff. weighings within opt. range	0.03 mg
Size:	10 1/2" x 18" x 18"
Net Wt.:	45 lbs.
Shipping Wt.:	57 lbs.

Write for Illustrated Literature



AUGUST SAUTER OF N.Y., INC.
866 WILLIS AVENUE
ALBERTSON, L. I., N. Y.
Pioneer 6-0254

Leitz, E., Inc.

1959: 2 Oct., 818; 16 Oct., 938; 6 Nov., 1210; 20 Nov., 1374; 27 Nov., 1444; 18 Dec., 1674

1960: 1 Jan., 2; 15 Jan., 122; 5 Feb., 314; 18 Mar., 752; 1 Apr., 950; 15 Apr., 1062; 6 May, 1334; 17 June, 1754; 1 July, 2; 15 July, 106; 19 Aug., 434; 2 Sept., 582

Lumiscop Co.

1959: 23 Oct., 1129; 4 Dec., 1597

United Scientific Co.

1959: 23 Oct., 1076; 11 Dec., 1616; 18 Dec., 1713

1960: 22 Jan., 176; 29 July, 264

Wild Heerbrugg Instruments, Inc.

1959: 23 Oct., 1046; 6 Nov., 1218; 20 Nov., 1435; 4 Dec., 1530

1960: 8 Jan., 68; 22 Jan., 230; 26 Feb., 614; 11 Mar., 694; 18 Mar., 796; 22 Apr., 1260; 13 May, 1400; 10 June, 1700; 24 June, 1858; 8 July, 95; 22 July, 250; 19 Aug., 486; 26 Aug., 552; 9 Sept., 685; 23 Sept., 828

Zeiss, Carl, Inc.

1959: 9 Oct., 893; 23 Oct., 1023; 13 Nov., 1288

1960: 26 Feb., 621; 18 Mar., 789; 13 May, 1459; 5 Aug., 371

MICROSCOPES, ELECTRON

Bendix Aviation Corp., Cincinnati Div.

1959: 23 Oct., 1123; 4 Dec., 1601

1960: 22 Jan., 243; 22 July, 233

Erb & Gray Scientific, Inc.

1959: 4 Dec., 1522; 11 Dec., 1663

1960: 22 Jan., 188; 19 Feb., 549; 4 Mar., 673; 18 Mar., 853; 27 May, 1629; 8 July, 97; 26 Aug., 565; 23 Sept., 833

Hitachi, Ltd.

1960: 26 Feb., 615; 25 Mar., 939; 15 July, 155

National Instrument Laboratories, Inc.

1960: 23 Sept., 758

Philips Electronics, Inc.

1959: 23 Oct., 1040; 4 Dec., 1526

1960: 18 Mar., 780; 22 Apr., 1136

Siemens New York, Inc.

1959: 23 Oct., 1155; 4 Dec., 1611

MICROSCOPES, POLARIZING

American Optical Co.

1960: 8 Apr., 1060; 12 Aug., 432

Leitz, E., Inc.

1960: 5 Aug., 314

United Scientific Co.

1959: 27 Nov., 1484

1960: 15 Jan., 168; 26 Feb., 616; 8 Apr., 1054; 3 June, 1688; 8 July, 98; 12 Aug., 427; 2 Sept., 626

Zeiss, Carl, Inc.

1960: 8 July, 56

MICROSCOPES, STEREO

American Optical Co.

1959: 23 Oct., 1156

1960: 1 Jan., 52; 25 Mar., 948; 6 May, 1392; 23 Sept., 856

Bausch & Lomb Optical Co.

1959: 23 Oct., 1050; 20 Nov., 1382; 4 Dec., 1534

1960: 29 Jan., 268; 26 Feb., 578; 6 May, 1340; 1 July, 8; 12 Aug., 386; 23 Sept., 784

Cooke, Troughton & Simms, Inc.

1960: 29 Apr., 1276; 20 May, 1469

TECHNICON®

AUTOMATIC VARIABLE GRADIENT DEVICE*

produces any buffer requirement in pH or concentration for chromatography

Eliminates
DISCRETE BUFFER CHANGEOVERS
as an example . . .


to pH 5.28

to pH 4.25

from pH 3.25

. . . usual in


AMINO ACID CHROMATOGRAPHY
instead the Autograd automatically supplies a buffer gradient in a continuous, uninterrupted flow.**

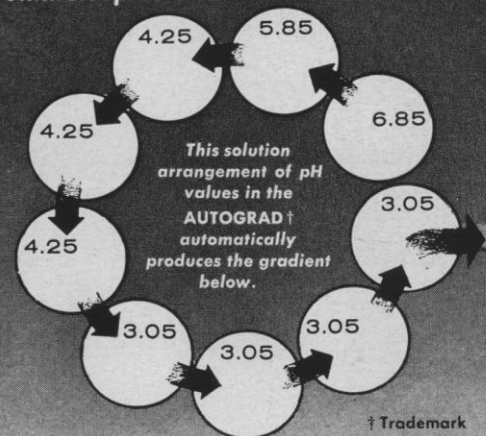

† Trademark

Produces higher Resolution

The Autograd† starts the column elution delivery at pH 3.05, as shown above, and progressively in a continuous flow, increases to pH 6.85. Not only is each discrete buffer value systematically produced, but the resulting gradient includes all of the intermediate values as graphed below.

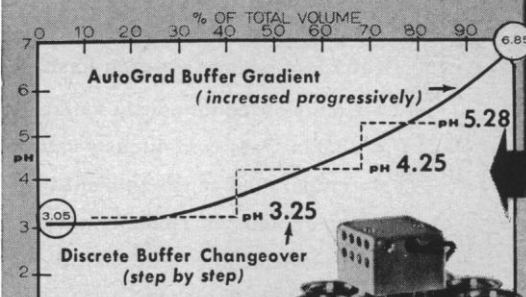

Developed at the National Cancer Institute, National Institutes of Health, U. S. Department of Health, Education, and Welfare, Public Health Service, Bethesda, Maryland.

**Procedure developed by Karl A. Piez, National Institute of Dental Research, National Institute of Health.

*Reference: "Variable Gradient Device for Chromatography", E. A. Peterson and H. A. Sober, Anal. Chem., Vol. 31, No. 34, May 1959.

Send for Brochure No. AG1, and further Data, to:

Technicon Chromatography Corp.
Research Park • Chauncey, New York

Edmund Scientific Co.

1959: 9 Oct., 886; 6 Nov., 1221
 1960: 8 Jan., 69; 19 Feb., 459; 27 May, 1631; 17 June, 1764; 22 July, 259; 26 Aug., 508; 23 Sept., 855

Sobotka, Eric, Co.

1960: 13 May, 1450; 20 May, 1540; 3 June, 1686; 9 Sept., 688; 23 Sept., 845; 7 Oct., 964

United Scientific Co.

1959: 2 Oct., 871; 20 Nov., 1432
 1960: 22 Jan., 176; 12 Feb., 425; 11 Mar., 744; 18 Mar., 754; 15 Apr., 1064; 29 Apr., 1327; 10 June, 1747; 22 July, 233; 26 Aug., 572; 23 Sept., 756; 7 Oct., 970

Wild Heerbrugg Instruments, Inc.

1959: 9 Oct., 890

1960: 29 Jan., 263; 12 Feb., 380; 27 May, 1627; 12 Aug., 378

MICROSCOPES, STUDENT**Bausch & Lomb Optical Co.**

1960: 22 Apr., 1164; 3 June, 1640; 23 Sept., 784

Edmund Scientific Co.

1959: 27 Nov., 1446; 4 Dec., 1506
 1960: 19 Feb., 459

Elgeet Optical Co., Inc., Scientific Instrument and Apparatus Div.

1959: 13 Nov., 1301
 1960: 22 Jan., 186; 18 Mar., 793; 20 May, 1487; 10 June, 1699; 22 July, 185; 5 Aug., 318; 19 Aug., 491; 2 Sept., 631; 16 Sept., 698; 7 Oct., 914

Graf-Apsco Co.

1959: 23 Oct., 1121; 4 Dec., 1595
 1960: 22 Jan., 237; 19 Feb., 563; 22 Apr., 1244; 20 May, 1549; 9 Sept., 686; 23 Sept., 816

Leitz, E. Inc.

1959: 23 Oct., 1033; 18 Dec., 1674

Science Materials Center

1959: 6 Nov., 1217

United Scientific Co.

1959: 23 Oct., 1076, 1077; 13 Nov., 1280
 1960: 19 Feb., 436; 4 Mar., 677; 1 Apr., 996; 18 Mar., 754; 15 Apr., 1064; 22 Apr., 1246; 13 May, 1454; 20 May, 1562; 27 May, 1576; 24 June, 1852; 15 July, 156; 29 July, 264; 19 Aug., 436; 16 Sept., 748; 30 Sept., 902

MICROSCOPES, TELEVISION**Brinkmann Instruments, Inc.**

1960: 19 Feb., 467; 18 Mar., 774

MICROSCOPE ACCESSORIES**American Hospital Supply Corp.**

1960: 19 Feb., 458

American Optical Co.

1959: 20 Nov., 1440
 1960: 12 Feb., 432; 26 Feb., 622; 8 Apr., 1060; 6 May, 1392; 17 June, 1848; 1 July, 52; 26 Aug., 580; 23 Sept., 856; 7 Oct., 976

Burton Manufacturing Co.

1959: 23 Oct., 1152

Hacker, William J., & Co., Inc.

1960: 22 Apr., 1126

Lafayette Radio

1959: 23 Oct., 1012

Leitz, E., Inc.

1959: 16 Oct., 938

Sobotka, Eric, Co.

1960: 26 Feb., 616; 18 Mar., 842; 8 Apr., 1054

United Scientific Co.

1959: 23 Oct., 1076; 13 Nov., 1280; 11 Dec., 1616

1960: 12 Feb., 425; 19 Feb., 436; 11 Mar., 744; 18 Mar., 754; 15 Apr., 1064; 29 Apr., 1327; 27 May, 1576; 24 June, 1852; 29 July, 264; 19 Aug., 436; 26 Aug., 572; 23 Sept., 756; 7 Oct., 970

Wild Heerbrugg Instruments, Inc.

1959: 23 Oct., 1046; 18 Dec., 1678
 1960: 8 Jan., 68; 22 Apr., 1260; 13 May, 1400; 8 July, 95; 22 July, 250; 19 Aug., 486; 9 Sept., 685; 23 Sept., 828

Zeiss, Carl, Inc.

1960: 15 Jan., 127

MICROSCOPE SLIDES**Erie Scientific Co.**

1960: 22 Apr., 1250

National Instrument Laboratories, Inc.

1960: 18 Mar., 760

MICROTOMES AND ACCESSORIES**American Optical Co.**

1959: 9 Oct., 936; 4 Dec., 1612; 18 Dec., 1724


1960: 20 May, 1572; 29 July, 312; 9 Sept., 692

Brunswick-Balke-Collender Co., Aloe Scientific Div.

1959: 16 Oct., 987

Hacker, William J., & Co., Inc.

1960: 18 Mar., 858

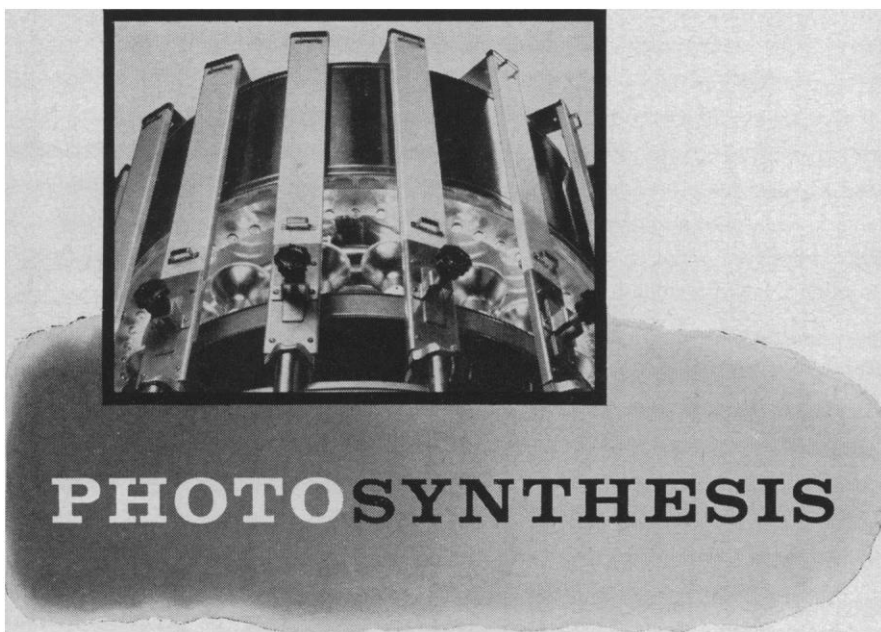**WARBURG APPARATUS**

by **GME**

This version of the GME-Lardy Circular Warburg apparatus has a specially constructed water bath with a transparent plastic bottom. 30-watt reflector spotlights are suitably placed beneath the bath, providing 1000 to 1400 foot-candles on each flask.

- Excursion continuously variable from 0 to 5 cm.
- Shaking rate continuously variable from 75 to 150 per minute
- Temperature range ambient to 50° C.
- Accommodates 18 manometers, 16 of them with lights
- Accurate temperature control, better than $\pm .02^\circ \text{C}$.
- Diameter: 26 inches

Unlimited rotation when lights are not used. Refrigerated models also available, as well as a somewhat smaller model with accommodations for 14 manometers, 12 of them with lights.

Gilson Medical Electronics

Middleton, Wisconsin
 (On Madison's West Beltline Highway)

NOW! TWO MODELS

Provides a wide range of sensitivity, stability, and linear response particularly at extreme low-light levels. Choice of interchangeable photomultiplier tubes for optimum response in selected spectral regions. This compact, easy-to-operate instrument is now available in two models: battery power supply or transformer for line operation. Either model can be supplied with a galvanometer or with a highly sensitive microammeter.

Farrand
Electron Multiplier

PHOTOMETER



Technical data available on request
specify Bulletin No. 804S

FARRAND OPTICAL CO., INC.

BRONX BLVD. AND EAST 238th STREET • NEW YORK 70, N. Y.
Engineering, Research, Development, Design and Manufacture of Precision Optics, Electronic and Scientific Instruments

SAVE OVER 300% . . .

with the revolutionary new instrument
that takes the place of six individual
burettes — plus magnetic stirrer!

The New Buchler POLYBURETTE

**FOR RAPID TITRATION—ELIMINATES
TIME-CONSUMING MANIPULATIONS
DISPENSES A VARIETY OF SIX SUB-
STANCES WITH AN INDEPENDENT
BURETTE FOR EACH**


- Eliminates need for intermediate rinsing of the burette when different reagents are used simultaneously for multiple titrations.
- Illuminated background facilitates reading.
- Interchangeable burettes for deliveries from 0.001 ml to 1.0 ml.
- Built-in magnetic stirrer.
- All glassware easily sterilized.

For details, request Bulletin S2-2600

Laboratory Apparatus



Precision Instruments

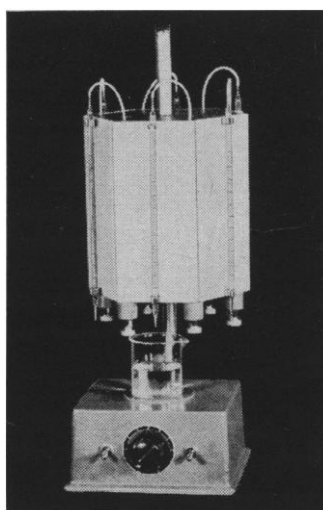

\$194⁰⁰

Other Versatile
Laboratory
Aids

BY BUCHLER

That Save Time
and Labor!

**ROTARY EVAPO-MIX
FLASH EVAPORATOR
FRACTION COLLECTORS
CHLORIDOMETER
OMNI-SHAKER**

Send for Bulletins!

BUCHLER INSTRUMENTS, INC.

formerly Laboratory Glass & Instruments Corp.

514 WEST 147th STREET, N.Y. 31, N.Y. ADirondack 4-2626

It's So!



when an
EA
recording
DC MICROAMMETER

says it's so!

You can count on whatever a DC Microammeter records because, first and foremost, it's designed and built for RELIABILITY.

In today's space-age technology, reliability of the highest possible order is an absolute necessity. And in a recording instrument, reliability of this high order is achieved only through simplicity of design and rugged construction.

Esterline-Angus does it by building its recorders with a minimum of components, all of long-life design . . . by building recorders that require few— and simple—adjustments.

It's the outcome of more than 50 years of development and testing . . . of production experience and conscientious quality control . . . of specializing in fine recording instruments.

It's the reason why the Esterline-Angus DC Microammeter, like all E-A recording instruments, is guaranteed for two years.

Send for Catalog Section 41

The
ESTERLINE-ANGUS
Company

*No. 1 in fine Recording Instruments
for more than 50 years.*

DEPT. L, BOX 596, INDIANAPOLIS 6, INDIANA

Lafayette Radio

1959: 23 Oct., 1013

Leitz, E., Inc.

1959: 9 Oct., 889

1960: 19 Feb., 434; 3 June, 1634; 16 Sept., 694

LKB Instruments, Inc.

1960: 22 Jan., 190; 29 Jan., 311; 26 Feb., 615; 18 Mar., 873

National Instrument Laboratories, Inc.

1959: 23 Oct., 1032

1960: 18 Mar., 760

Schueler & Co., Schuco Scientific Div.

1960: 9 Sept., 689; 23 Sept., 839

Sorvall, Ivan, Inc.

1959: 23 Oct., 1025

1960: 15 Jan., 170; 22 Apr., 1128; 20 May, 1561; 22 July, 231; 26 Aug., 567

MICRO-WAVE APPARATUS

Central Scientific Co.

1959: 16 Oct., 988

Raytheon Co.

1959: 9 Oct., 892; 16 Oct., 991; 23 Oct., 1044; 30 Oct., 1162; 13 Nov., 1302; 27 Nov., 1482; 18 Dec., 1719

1960: 22 Jan., 192; 19 Feb., 452; 18 Mar., 770; 22 Apr., 1148; 20 May, 1480, 1553; 17 June, 1772, 1829; 22 July, 184, 241; 26 Aug., 512, 561; 23 Sept., 772

MIXERS

Brunswick-Balke-Collender Co., Aloe Scientific Div.

1960: 22 Apr., 1265; 20 May, 1555

Buchler Instruments, Inc., formerly Laboratory Glass & Instrument Corp.

1960: 22 Jan., 180; 19 Feb., 460; 22 Apr., 1226

Heller, Gerald K., Co.

1960: 18 Mar., 843; 22 Apr., 1258; 20 May, 1542; 22 July, 239; 23 Sept., 830

Scientific Industries, Inc.

1960: 16 Sept., 748

MOLECULAR MODEL SETS

LaPine, Arthur S., and Co.

1960: 23 Sept., 822

Will Corp., Bronwill Scientific Div.

1960: 18 Mar., 864; 8 Apr., 1055; 9 Sept., 680

MONOCHROMATORS

Bausch & Lomb Optical Co.

1960: 11 Mar., 698

Farrand Optical Co., Inc.

1959: 13 Nov., 1351; 4 Dec., 1583

1960: 19 Feb., 563; 17 June, 1815; 7 Oct., 965

Perkin-Elmer Corp., Instrument Div.

1959: 4 Dec., 1496

1960: 15 Jan., 124

Photovolt Corp.

1959: 2 Oct., 867

1960: 1 Jan., 51; 4 Mar., 673; 29 Apr., 1324; 3 June, 1687; 5 Aug., 367

NEPHELOMETERS

Klett Manufacturing Co.

1960: 26 Feb., 618; 18 Mar., 843; 25 Mar., 945; 8 Apr., 1051; 29 Apr., 1325; 6 May, 1384; 20 May, 1552; 3 June, 1687; 1 July, 47; 8 July, 94; 29 July, 311; 12 Aug., 429; 19 Aug., 477; 16 Sept., 747; 23 Sept., 850; 7 Oct., 973

Series 1200

PARR Calorimeter



for determining the heat of combustion of solid and liquid fuels.

Excellent for either routine or research calorimetry.

Any of seven different PARR oxygen bombs can be used in the Series 1200 adiabatic calorimeter for testing samples liberating up to 10,000 calories. The bomb chamber is completely enclosed within a circulating water jacket which can be adjusted to maintain either adiabatic conditions or a static reference temperature during the calorific test.

Ask for Specification 1200



INSTRUMENT COMPANY
MOLINE, ILLINOIS

PHOTOGRAPHIC OPTIMUM

Linhof
**SUPER
TECHNIKA
cameras...**

Available in
2¼x3¼, 4x5, 5x7...



Linhof Super Technika cameras... photographic mainstays of top-level research teams throughout the world, meet exacting challenges—in the field and in the laboratory—wherever photo-analysis is crucial to scientific understanding.

Send 50¢ for colorful, 120-page
Linhof Products Handbook.



KLING PHOTO CORPORATION

257-T Park Avenue South, New York 10, N. Y.

Thomas, Arthur H., Co.
1960: 22 July, 260; 16 Sept., 752
Will Corp.
1960: 19 Feb., 561

NEUTRON GENERATORS

Central Scientific Co.
1959: 20 Nov., 1431
1960: 19 Feb., 549
Kaman Aircraft Corp., Nuclear Div.
1959: 4 Dec., 1528
Texas Nuclear Corp.
1960: 18 Mar., 877

NUCLEAR LABORATORY INSTRUMENTS

Anton Electronic Laboratories, Inc.
1960: 23 Sept., 759
Baird-Atomic, Inc.
1959: 4 Dec., 1508
1960: 19 Feb., 468; 20 May, 1515
Budd Co., Nuclear Systems Div.
1959: 4 Dec., 1498
Johnston, William H., Laboratories, Inc.
1960: 17 June, 1834
Nuclear-Chicago Corp.
1959: 27 Nov., 1492
1960: 22 Jan., 260; 19 Feb., 570; 4 Mar., 682
Packard Instrument Co., Inc.
1959: 16 Oct., 946
Picker X-Ray Corp.
1959: 23 Oct., 1015
1960: 18 Mar., 775; 17 June, 1775
Radiation Counter Laboratories, Inc.
1960: 19 Feb., 545
Radiation Instrument Development Laboratory, Inc.
1960: 19 Feb., 473; 7 Oct., 964
Technical Associates
1960: 18 Mar., 865
Technical Measurement Corp.
1959: 23 Oct., 1048; 20 Nov., 1380; 4 Dec., 1532
Tracerlab, Inc.
1960: 23 Sept., 760
Vanguard Instrument Co.
1960: 26 Aug., 506
Victoreen Instrument Co.
1960: 22 Jan., 252

OPTICAL CRYSTALS

Harshaw Chemical Co.
1959: 2 Oct., 869; 4 Dec., 1595
1960: 19 Feb., 539; 8 Apr., 1055; 10 June, 1747; 19 Aug., 477; 7 Oct., 965
Isomet Corp.
1959: 23 Oct., 1139; 4 Dec., 1601
1960: 18 Mar., 883; 20 May, 1552

OSCILLATORS, SONIC

Raytheon Co.
1960: 22 Jan., 241; 19 Feb., 551; 18 Mar., 869; 22 Apr., 1237; 23 Sept., 837


OSMOMETERS

Rosemount Engineering Co.
1960: 22 Apr., 1244

OVENS

Boeckel, Wm., & Co., Inc.
1960: 20 May, 1537
Central Scientific Co.
1960: 29 July, 311

LOW
BACKGROUND
BETA
COUNTING
SYSTEM

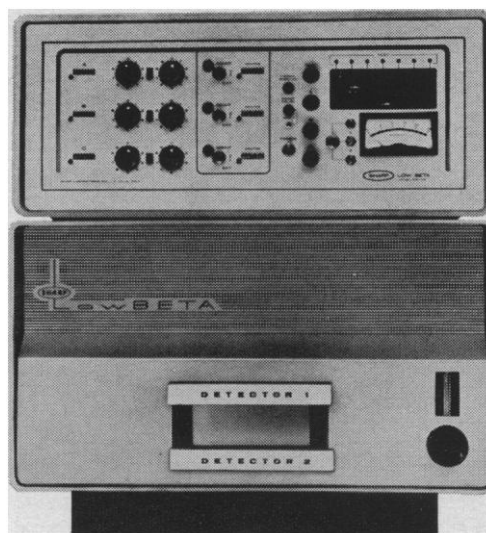

LOW-BACKGROUND DETECTION SYSTEMS

LOWBETA and LOWBETA/MATIC: Manual and Automatic Low Background Beta Counting Systems. Background less than $\frac{1}{4}$ count per minute for 1-inch diameter detector. Detectors available from $\frac{1}{2}$ " to 3" diameter. Shield size only 18 inches square. Shield weight only 1500 lbs. Transistorized electronics. Plug-in printed circuit cards. Illuminated programming panel for simplified control. Electronics ideal for carbon dating.

GAMMAMATIC: Sample Changing System for Well Counters. Holds 52 samples up to $1\frac{1}{8}$ " diameter. Achieves a constant background by using a stationary sample rack and a moving selector arm. Rack configuration may be chosen to suit individual requirements.

LOWGAMMA: Low Background Gamma Counting Systems. Counts large and small samples. Manual and automatic.

DATASHARP: Automatic Readout Systems. Counts, times, indicates time of day, sample or index number, etc. Reads out into DATASHARP parallel printers or any other conventional readout device, including punch cards and tape.

ENVIRONMENTAL MONITORING SERVICE

RADIOCHEMICAL CONSULTING SERVICE


Represented exclusively by BAIRD-ATOMIC, INC. See your BAIRD representative or write or call Sharp Laboratories, Inc., Dept. S-1, Box 1302, La Jolla, California.



LABORATORIES, INC.

Forced Convection Ovens

**MAXIMUM 500° F.
FOR LABORATORY
TESTING**

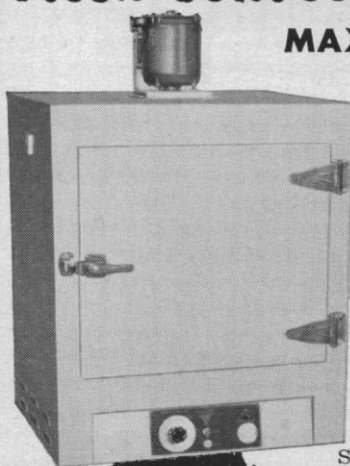


Sterilizing, tempering glass, preheating plastics—only a few of many uses for these versatile ovens. Forced air convection allows accurate automatic control of evenly-distributed heat. Rugged construction, ease of operation and economy—plus practical good looks—guarantee a wise investment.

Small size overall dimension: 28" wide, 16" deep, 43 1/2" high. Inside dimensions: 20" x 16" x 18"; gives option of several heats in a single laboratory. Models available for either 110 or 220 vac.

Write Today for free bulletin 203-108U


**Price
\$330⁰⁰**

**DESPATCH
OVEN
CO.**

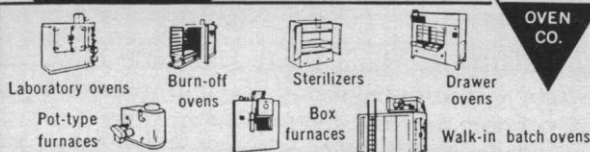

DESPATCH OVEN CO. 619 S.E. 8th St., Minneapolis 14, Minn.

ULTRA LOW-LEVEL BETA COUNTER

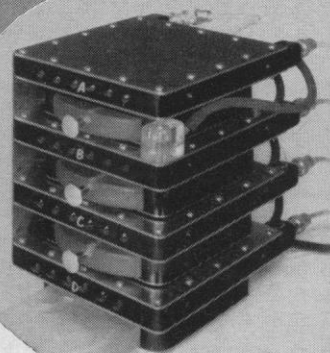

Sample Detector

Choice of up to 4 gas flow geiger detectors of plastic and copper with diameters of up to 3 inches

Counter Characteristics

Background 0.4 cpm for the 1 1/4" diameter, operating at 1050 v. with a 150 v. plateau

Shielding

One gas flow guard detector mounted above each sample detector. Unit surrounded by 4" lead lined with copper


Electronics

Printed card plug-in units using transistors and solid-state diodes for long trouble-free performance. Shielded detectors and electronics mounted in single cabinet 20" x 18" x 37".

For complete information write to:

ISOTOPE, INC.


123 Woodland Avenue, Westwood, New Jersey



HELLER ELECTRONIC CONTROLLED LAB MIXER

PROVIDES:

- **CONSTANT TORQUE**
- **VARIABLE DC SPEEDS
FROM AC LINES**

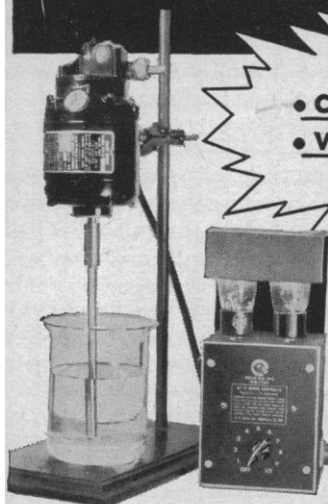

Complete with
attachments
F.O.B. Las Vegas

\$90

• Thyatron tubes on the Heller GT-21 controller supply demanded current by converting power in stepless variation to the direct current motor. Assures constant torque as mixes become either viscous or fluid. Variable, reversible motor has direct and gear drive. Armature shaft speed, 0-5000 rpm. Gear shaft 18:1 ratio. Chuck, shafts, 3-step pulley included.

Order from your Laboratory Supply Dealer or write—

GERALD K. HELLER CO.
1819 Industrial Road Las Vegas, Nevada

MEASURE MOLECULAR WEIGHT AND PARTICLE SIZE



**NEW BRICE-PHOENIX UNIVERSAL
LIGHT SCATTERING PHOTOMETER**

Measures:

1. Absolute Turbidity
2. Dissymmetry
3. Depolarization

This instrument is listed in U.S. Government specifications for the evaluation of certain clinical materials.

PHOENIX PRECISION INSTRUMENT COMPANY
3805 N. 5th St. Philadelphia 40, Pa.

Fisher Scientific Co.

1960: 22 Apr., 1160

National Appliance Co.

1959: 23 Oct., 1118; 13 Nov., 1353

1960: 8 Jan., 111

New Brunswick Scientific Co., Inc.

1959: 23 Oct., 1123; 11 Dec., 1666

1960: 5 Feb., 367; 13 May, 1452; 24 June, 1896; 23 Sept., 849

New York Laboratory Supply Co., Inc.,

1960: 18 Mar., 863; 17 June, 1819

Precision Scientific Co.

1959: 13 Nov., 1352; 4 Dec., 1588

1960: 26 Aug., 568

Research Specialties Co.

1959: 23 Oct., 1043

Sargent, E. H., & Co.

1959: 2 Oct., 820

1960: 22 July, 188

pH METERS**American Hospital Supply Corp.**

1960: 24 June, 1857

Beckman Instruments, Inc., Scientific and Process Instruments Div.

1959: 16 Oct., 943; 18 Dec., 1676

1960: 5 Feb., 321; 15 Apr., 1069; 17 June, 1763; 15 July, 163

Brinkman, C. A., & Co., Inc.

1959: 6 Nov., 1219; 13 Nov., 1363

1960: 22 Jan., 215, 217, 218; 29 Jan., 307; 4 Mar., 678; 8 Apr., 1004

Cambridge Instrument Co., Inc.

1959: 23 Oct., 1150

Coleman Instruments, Inc.

1959: 4 Dec., 1515

1960: 22 Jan., 181; 20 May, 1483

Harshaw Chemical Co., Harshaw Scientific Div.

1960: 18 Mar., 848; 20 May, 1538

Photovolt Corp.

1959: 11 Dec., 1663

1960: 22 Jan., 251; 11 Mar., 747; 8 Apr., 1055; 13 May, 1457; 27 May, 1628; 15 July, 160; 16 Sept., 749

Riseman Development Laboratory

1960: 23 Sept., 850

Scientific Glass Apparatus Co., Inc.

1960: 25 Mar., 942; 22 Apr., 1242; 20 May, 1477

Thomas, Arthur H., Co.

1960: 19 Aug., 492

Welwyn International Inc.

1959: 23 Oct., 1036; 13 Nov., 1286

1960: 22 Jan., 259; 22 Apr., 1144; 20 May, 1478; 23 Sept., 778

PHOTOMETERS**Farrand Optical Co., Inc.**

1960: 20 May, 1539

Phoenix Precision Instrument Co.

1960: 19 Feb., 599; 20 May, 1552; 23 Sept., 849

Photovolt Corp.

1960: 29 Jan., 307; 5 Feb., 367; 25 Mar., 943; 6 May, 1386; 10 June, 1749; 29 July, 311; 12 Aug., 425; 9 Sept., 681; 30 Sept., 904; 7 Oct., 967

Welch, W. M., Manufacturing Co.

1960: 7 Oct., 967

PHOTOMETERS, FLAME**Baird-Atomic, Inc.**

1959: 23 Oct., 1145

1960: 22 Jan., 248; 19 Feb., 554; 18 Mar., 856; 22 Apr., 1256; 20 May, 1548;

17 June, 1839; 22 July, 238; 26 Aug., 574; 23 Sept., 850

Coleman Instruments, Inc.

1959: 23 Oct., 1047

1960: 17 June 1774; 26 Aug., 502

Perkin-Elmer Corp.

1959: 23 Oct., 1000

Will Corp.

1960: 23 Sept., 815

PHOTOMICROGRAPHIC EQUIPMENT**Aloe, A. S., Co., Aloe Scientific Div.**

1960: 1 Jan., 48

American Optical Co.

1959: 6 Nov., 1276

1960: 15 Jan., 172; 22 Apr., 1272; 6 May, 1392; 15 July, 164

Bausch & Lomb Optical Co.

1960: 26 Feb., 578

Hacker, William J., & Co., Inc.

1960: 22 Jan., 185; 19 Feb., 449; 23 Sept., 763

Leitz, E., Inc.

1959: 2 Oct., 818; 16 Oct., 938; 20 Nov., 1374; 27 Nov., 1444

1960: 1 Jan., 2; 15 Jan., 122; 5 Feb., 314

Photovolt Corp.

1959: 16 Oct., 987

1960: 5 Feb., 367; 25 Mar., 943; 10 June, 1749; 12 Aug., 425; 30 Sept., 904

United Scientific Co.

1959: 23 Oct., 1076; 13 Nov., 1280

1960: 22 Jan., 176; 29 Jan., 304; 25 Mar., 940; 17 June, 1840; 24 June, 1852; 29 July, 264; 9 Sept., 683; 23 Sept., 756

Zeiss, Carl, Inc.

1959: 23 Oct., 1023

1960: 15 Jan., 127

PLASMA GENERATORS**Avco Corp., Research and Advanced Development Div.**

1959: 2 Oct., 827

POLARIMETERS**Kern Co.**

1960: 7 Oct., 964

Leitz, E., Inc.

1959: 4 Dec., 1529

1960: 4 Mar., 624

Photovolt Corp.

1959: 23 Oct., 1137; 11 Dec., 1663

1960: 8 Jan., 116; 1 July, 47

Rudolph Instruments Engineering Co.

1959: 23 Oct., 1034

Zeiss, Carl, Inc.

1959: 9 Oct., 893

1960: 19 Feb., 455; 3 June, 1638; 8 July, 56; 9 Sept., 679

POLARISCOPES**Bethlehem Apparatus Co., Inc.**

1960: 23 Sept., 848

POLAROGRAPHS**Brinkmann, C. A., & Co.**

1960: 22 Jan., 216; 29 Apr., 1327; 3 June, 1685; 15 July, 155

Fisher Scientific Co.

1960: 19 Feb., 475



Sargent, E. H., & Co.

1960: 22 Jan., 193; 20 May, 1485; 15 July, 111; 26 Aug., 505

Welwyn International, Inc.

1960: 18 Mar., 790

BETHLEHEM POLARISCOPE

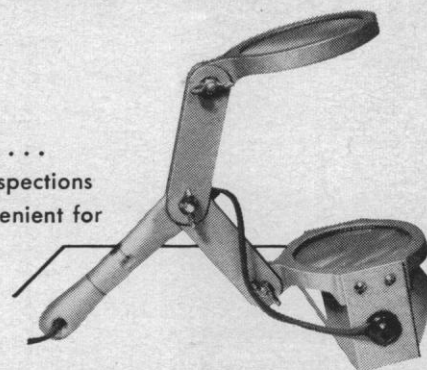*for showing strains in glass or plastic** **FULL COLOR . . .** for high sensitivity and clarity.* **A DUAL PURPOSE UNIT . . .**
excellent for BENCH inspections
. . . and light and convenient for
PORTABLE USE.**Model P5 BETHLEHEM POLARISCOPE**

- * Adjustable Arms
- * 110 v. Light Source
- * Switch in Cord
- * Constructed of Aluminum and Steel
- * Finished in Baked Hammertone Grey
- * Net Weight . . . 1-³/₄ lb.
- * Price . . . \$65.00

**BETHLEHEM APPARATUS COMPANY, INC.**

HELLERTOWN, PA.

now, at low cost, the new ASCO "50" enables you to compare your present processing costs with those of

MOLECULAR DISTILLATION



hundreds
now in
use...

Fields of investigation heretofore made prohibitive through use of highly expensive investigative techniques can now be explored with this simple-to-operate molecular still. Since the "50" still is the laboratory counterpart of the large commercial Rota-Film Still, results obtained may be duplicated on a commercial scale of any magnitude.


With this simple-to-operate still you may...

- explore falling agitated film evaporation and distillation
- distill materials with molecular weights ranging from 200 to 1250 weight (hydrocarbons) and some materials to 4000 molecular weight (silicones and halocarbons)
- deglycerinate and distill mixtures of mono-, di- and tri-glycerides
- distill tall oil
- distill paraffin from slack wax or petroleum residue
- deodorize oils
- remove color bodies from materials of high molecular weights.

FEATURES

- Batches from 10 ml to 20 liters
- Vacuum range from atmospheric to 1 micron Hg.
- Temperature range to 450°C.
- Teflon or carbon rotor-wiper blades
- Stainless-steel (18-8 type 304) wiper-holders (Available with Hastelloy B)
- Continuous or batch feed
- All parts made of glass except wiper-holders and top plate
- UNITS MAY BE COUPLED FOR FRACTIONATION.

ARTHUR F. SMITH, INC. • 311 ALEXANDER ST., ROCHESTER 4, N. Y.

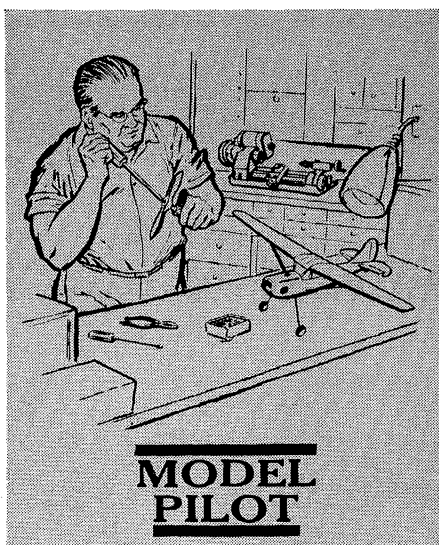


Ray Haines, Director of Research & Development at Aurora Plastics Corp., finds that he's also a test pilot for the firm's ready-to-fly model planes. These models have to perform as well as their prototypes, and Ray perfects the motors using his UNIMAT to machine the small parts. No matter what the problem is, it can be solved with this multifunctional machine-shop-in-miniature. UNIMAT is ten interchangeable machines on one base no larger than a jeweler's lathe. WRITE FOR FULLY ILLUSTRATED CATALOG AND PRICE LIST.

UNIMAT
AMERICAN EDELSTAAL INC.
350 BROADWAY, DEPT. AJ, N. Y. 13, N. Y.



designed to produce and utilize sound energy for the mechanical disintegration of cells and bacteria.

- Cabinet construction as a single unit with acoustically insulated working chamber.
- Titanium probes provide greater resistance to corrosion and erosion.
- Built-in thermo-ammeter to give accurate indication of tuning.
- At 20,000 cycles.

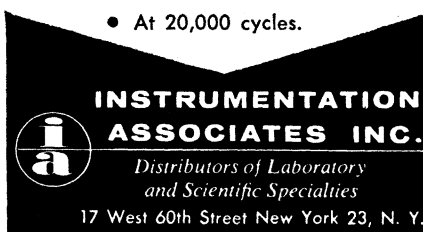

POTENTIOMETERS, SLIDEWIRE

B & H Instrument Co., Inc.
1959: 23 Oct., 1031

POWER GENERATORS

Raytheon Co.

1959: 9 Oct., 892; 16 Oct., 991; 23 Oct., 1044; 30 Oct., 1162; 13 Nov., 1302; 27 Nov., 1482; 18 Dec., 1719
1960: 22 Jan., 192; 19 Feb., 452; 18 Mar., 770; 22 Apr., 1148; 20 May, 1480, 1553; 17 June, 1772, 1829; 22 July, 184, 241; 26 Aug., 512, 561; 23 Sept., 772

POWER SUPPLIES

American Electronic Laboratories, Inc.

1959: 23 Oct., 1139

1960: 18 Mar., 778

Fluke, John, Manufacturing Co., Inc.

1960: 26 Aug., 503

Harvey-Wells Electronics, Inc.

1960: 17 June, 1825

Sorensen & Co.

1960: 19 Feb., 541; 18 Mar., 866; 20 May, 1468; 26 Aug., 555; 23 Sept., 841

Zeiss, Carl, Inc.

1959: 4 Dec., 1525

1960: 7 Oct., 975

PRESSURE APPARATUS

Parr Instrument Co.

1959: 23 Oct., 1135

1960: 22 Jan., 242; 22 July, 242

PRIMATE RESTRAINT SYSTEMS

Foringer & Co., Inc.

1960: 7 Oct., 971

PROGRAMMERS, AUTOMATIC

Foringer & Co., Inc.

1959: 4 Dec., 1603

PROJECTORS

Bausch & Lomb Optical Co.

1959: 23 Oct., 1050; 6 Nov., 1224; 4 Dec., 1534

1960: 29 Jan., 268; 26 Feb., 578; 20 May, 1492; 3 June, 1640; 1 July, 8

Edmund Scientific Co.

1959: 9 Oct., 886; 6 Nov., 1221; 27 Nov., 1446; 4 Dec., 1506

1960: 19 Feb., 459; 18 Mar., 791; 22 Apr., 1138; 27 May, 1631; 22 July, 259

Leitz, E., Inc.

1959: 13 Nov., 1293

1960: 20 May, 1462; 7 Oct., 910

PUMPS

Eastern Industries, Inc.

1959: 13 Nov., 1296

1960: 18 Mar., 840; 17 June, 1830; 23 Sept., 838

Harvard Apparatus Co., Inc.

1959: 23 Oct., 1139

1960: 22 Apr., 1261; 22 July, 239

Phipps & Bird, Inc.

1960: 18 Mar., 853; 22 July, 254; 29 July, 309; 2 Sept., 629; 9 Sept., 686

Sigmamotor, Inc.

1959: 23 Oct., 1132; 4 Dec., 1604

1960: 8 Apr., 1053

PUMPS, VACUUM

Central Scientific Co.

1960: 25 Mar., 941

Hevi-Duty Electric Company

1960: 8 Jan., 111; 4 Mar., 677

LaPine, Arthur S., and Co.

1960: 18 Mar., 842; 20 May, 1550

New York Air Brake Co., Kinney Vacuum Div.

1960: 19 Feb., 533; 18 Mar., 849; 22 Apr., 1225; 17 June, 1819; 19 Aug., 483

Precision Scientific Co.

1960: 17 June, 1828; 22 July, 230; 23 Sept., 840

Welch, W. M., Manufacturing Co.

1959: 6 Nov., 1267

RADIATION COUNTERS

Amperex Electronic Corp.

1959: 23 Oct., 1029

Atomic Accessories, Inc.

1959: 4 Dec., 1591

Johnston, William H., Laboratories, Inc.

1960: 17 June, 1834

Nuclear-Chicago Corp.

1959: 16 Oct., 996; 11 Dec., 1672

1960: 1 Apr., 1000; 13 May, 1460; 10 June, 1752; 8 July, 104; 5 Aug., 372; 2 Sept., 632

Packard Instrument Co., Inc.

1959: 16 Oct., 946

Picker X-Ray Corp.

1959: 23 Oct., 1015; 13 Nov., 1304; 11 Dec., 1619

1960: 22 Jan., 187; 19 Feb., 461; 18 Mar., 775; 20 May, 1489; 12 Aug., 379; 23 Sept., 775

Radiation Counter Laboratories, Inc.

1960: 19 Feb., 545; 22 Apr., 1235

Radiation Instrument Development Laboratory, Inc.

1960: 7 Oct., 964

Technical Associates

1960: 18 Mar., 865; 20 May, 1563; 22 July, 247

Technical Measurement Corp.

1959: 9 Oct., 894

1960: 22 Apr., 1162; 15 July, 112; 26 Aug., 516

Tracerlab, Inc.

1960: 19 Feb., 448; 23 Sept., 760

Victoreen Instrument Co.

1960: 17 June, 1755

RADIOACTIVE WASTE CONTAINER

Blickman, S., Inc.

1960: 23 Sept., 830

RATEMETERS

Packard Instrument Co., Inc.

1960: 29 Apr., 1286; 10 June, 1704; 5 Aug., 322; 16 Sept., 706

Picker X-Ray Corp.

1960: 19 Feb., 461; 22 Apr., 1151; 20 May, 1489; 15 July, 107; 12 Aug., 379; 23 Sept., 775

Radiation Instrument Development Laboratory, Inc.


1960: 7 Oct., 964

READERS, STRIP CHART

Benson-Lehner Corp.

1960: 19 Feb., 440; 18 Mar., 777

21 OCTOBER 1960




DURA-VAC[®]
PLASTIC DESICCATOR

COMBINES THE LIGHT WEIGHT,
THE IMPACT AND
SHATTER RESISTANCE
OF PLASTIC WITH THE
TRANSPARENCY OF GLASS.


1) "DURA-VAC is transparent."

92% light transmission.

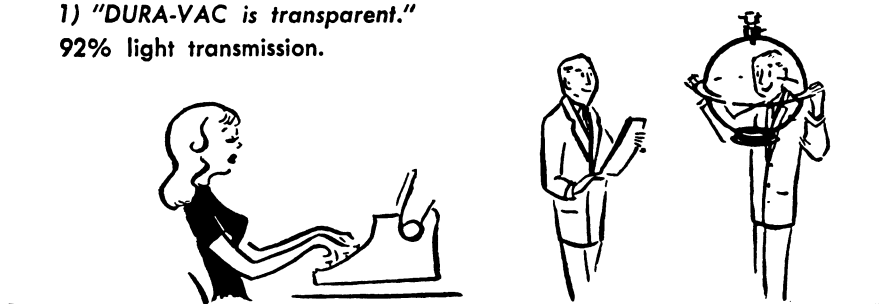

2) "DURA-VAC is featherweight."

50% lighter than glass.

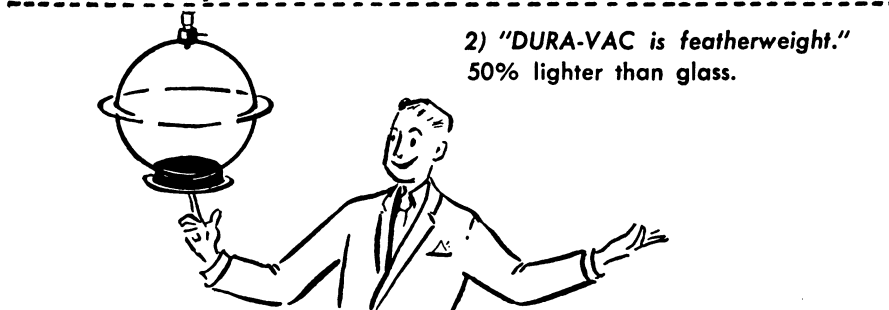


3) "DURA-VAC is strong and safe."

Yes, DURA-VAC is strong and safe. It is extremely implosion resistant. You can even drop it and 99 times out of a 100, DURA-VAC will remain intact.

4, 5, 6) "DURA-VAC has other advantages": The patented self-releasing lid does not stick, does not freeze to bottom during evacuation. DURA-VAC has a large working area: holds 2 lbs. of Drierite or similar material. DURA-VAC has a unique stopcock with upward vents that prevent returning air from disturbing contents.

Find out all about DURA-VAC. Write Dept. S for Bulletins #5810 and #5815.

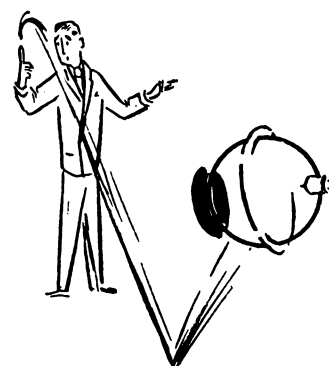

® T. M. Ace Glass

ACE GLASS
INCORPORATED

Louisville, Ky., Vineland N. J. Springfield, Mass.

Circle No. 1189 on Readers' Service Card

1189

1960: 22 Jan., 240; 23 Sept., 755
Baker, J. T., Co.
1959: 23 Oct., 1030; 13 Nov., 1352;
4 Dec., 1503
1960: 8 Jan., 65; 18 Mar., 767; 22
Apr., 1124; 20 May, 1535; 10 June, 1740
Borden Chemical Co.
1959: 4 Dec., 1584; 25 Dec., 1728
Colorado Serum Co.
1959: 4 Dec., 1597
1960: 15 Jan., 165; 9 Sept., 681
Difco Laboratories
1959: 13 Nov., 1351; 18 Dec., 1713
1960: 18 Mar., 853; 22 Apr., 1221; 22
July, 239; 26 Aug., 563
Eastern Chemical Corp.
1960: 7 Oct., 971

1857: 4 Dec., 1587
Klett Manufacturing Co.
 1859: 9 Oct., 931; 30 Oct., 1202; 6
 Nov., 1269; 4 Dec., 1597; 11 Dec., 1665;
 25 Dec., 1767
 1860: 1 Jan., 47; 8 Jan., 115; 15 Jan.,
 165; 29 Jan., 305; 12 Feb., 425; 19 Feb.,
 545; 26 Feb., 618; 11 Mar., 747; 25
 Mar., 945; 8 Apr., 1051; 15 Apr., 1106;
 22 Apr., 1236; 6 May, 1384; 13 May, 1452;
 3 June, 1687; 17 June, 1833; 24 June,
 1896; 8 July, 94; 22 July, 254; 5 Aug.,
 369; 12 Aug., 429; 26 Aug., 575; 2 Sept.,
 628; 23 Sept., 850; 30 Sept., 905; 7 Oct.,
 973
Mallinckrodt Chemical Works
 1859: 23 Oct., 1002, 1003
Matheson Co., Inc.
 1859: 23 Oct., 1124

1959: 16 Oct., 996
Schueler and Co., Schuco Scientific Div.
 1960: 19 Feb., 565; 23 Sept., 814
Scientific Glass Apparatus Co., Inc.
 1959: 23 Oct., 1026
Sigma Chemical Co.
 1959: 9 Oct., 931
Worthington Biochemical Corp.
 1960: 1 Jan., 48

1960: 8 Jan., 62: 5 Feb., 371

SCIENCE, VOL. 132

CLEANEST CLEANEST CLEANEST CLEANEST CLEANEST CLEANEST CLEANEST
CLEANEST CLEANEST CLEANEST CLEANEST CLEANEST CLEANEST CLEANEST
THE
CLEANEST CLEANEST CLEANEST CLEANEST CLEANEST CLEANEST CLEANEST
WORLD'S
CLEANEST CLEANEST CLEANEST CLEANEST CLEANEST CLEANEST CLEANEST
FINEST
CLEANEST CLEANEST CLEANEST CLEANEST CLEANEST CLEANEST CLEANEST
DETERGENT
CLEANEST CLEANEST CLEANEST CLEANEST CLEANEST CLEANEST CLEANEST
ALCONOX

Made especially for the exacting requirements of
LABORATORY, HOSPITAL AND MEDICAL USE!

MORE EFFECTIVE than any known detergent in
powder form or any liquid detergent that costs four
times as much!

Also makers of ALCOJET for all equipment washed by
machine and ALCOTABS in tablet form for all pipette
washers.


Order from your supplier or ask him for samples
and **FREE Cleaning Guide.**

Sold by All Leading Laboratory, Hospital and Sur-
gical Supply Dealers in the United States as well
as in
**CANADA • ENGLAND • SWITZERLAND • BELGIUM • NETHERLANDS • MEXICO
VENEZUELA • PERU • BRAZIL • PANAMA • PUERTO RICO • HAWAII**

The Master Cleaner
ALCONOX
WETTING AGENT
For Cleaning
BOROSILICATE
and GLASSWARE
LEAVING IT
Sparkling Brilliance
MADE BY
ALCONOX, INC.
NEW YORK, N.Y.

Meets Highest
Government Specifications

ALCONOX, INC., 853 BROADWAY, NEW YORK 3, N.Y.

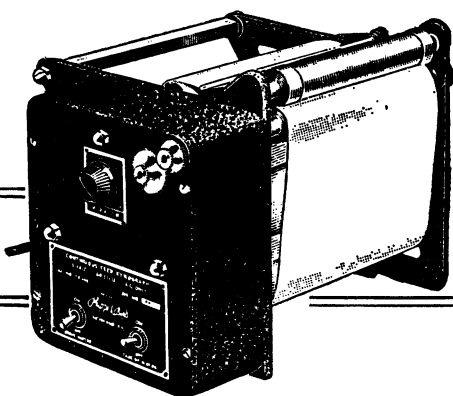

Bird, Continuous Feed

KYMOGRAPH

The outstanding features of modern industrial recorders are retained in this instrument without losing the versatility necessary for kymograph work. Ink writing levers are used exclusively.

The machine feeds an 80 foot roll of paper, 6 inches wide, at any of its eight speeds. Four of these are had with external gears of 40 and 56 teeth in one position, by simply operating a gear-shift knob. By reversing the external gears, four additional speeds become available.

Cat. No. 70-140

PHIPPS & BIRD, INC.

Manufacturers & Distributors of Scientific Equipment



6th & Byrd Streets - Richmond, Va.

ETHODIN

for preparation of

GAMMA GLOBULIN


Available from

Special Chemicals Dept.

WINTHROP LABORATORIES

1450 Broadway, New York 18, N.Y.

PERCIVAL PLANT GROWTH LAB

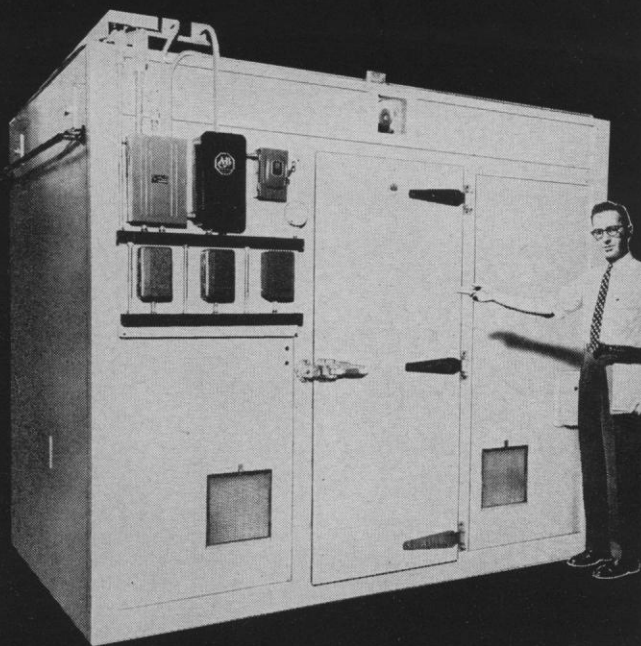

meets the exacting climatic needs
for botanical research

- **HIGH LIGHT INTENSITY:** 3,000 foot candles at 36 inches guaranteed. May be varied downward to 700 foot candles.
- **FLEXIBILITY:** Reproduces climatic requirements from 45° F to 95° F, and any photo period desired.
- **PRACTICAL SIZE:** Convenient walk-in unit. Inside dimensions: 98¾" long, 62¾" wide, 85⅝" high.
- **ECONOMY:** Low initial cost. Low operating cost.

for further information
MAIL COUPON TODAY



PERCIVAL REFRIGERATION & MFG. CO.

Box 589-S • Boone, Iowa

Please send bulletin on Percival Plant Growth Lab.

Name _____

Address _____

City _____ Zone _____ State _____



Laboratory Conductivity Bridges and Cells

- DESIGNED FOR
INSTRUCTIONAL WORK
- TITRATION MEASUREMENTS

Industrial Instruments manufactures a versatile line of laboratory conductivity bridges and cells designed specifically for instructional applications in colleges and universities.

RC-12B2 Conductivity Bridges are particularly designed for titration measurements and feature high sensitivity for an extremely wide range of measurements. Variable sensitivity control permits easy and rapid balancing. Effective scale length of 84 inches provides fast and easy dial readings. Separate resistance and conductance scales are provided. The RC-16B2 is a true AC bridge with bridge frequencies of 60 or 1000 CPS selected by means of panel mounted switch. Bridge balance indicated by electron-ray eye tube. Bridges are available in battery and line operated models.

For complete details on our complete line of laboratory conductivity instruments and cells, fill in your name and address on coupon and mail today.


Send detailed literature on
Laboratory Bridges & Cells to...

Name.....

Address.....

City.....Zone.....State.....

Industrial



**Industrial
Instruments Inc.**

89 Commerce Road, Cedar Grove, Essex County, N. J.

REFRACTOMETERS

Lafayette Radio

1959: 23 Oct., 1012, 1013

Leitz, E., Inc.

1959: 4 Dec., 1529

1960: 4 Mar., 624

Phoenix Precision Instrument Co.

1960: 19 Feb., 563; 20 May, 1542; 23 Sept., 839

Zeiss, Carl, Inc.

1960: 8 July, 56; 9 Sept., 679

REFRIGERATORS

Union Carbide Corp., Linde Co. Div.

1959: 23 Oct., 1130

1960: 19 Feb., 564; 18 Mar., 860; 17 June, 1836

SCALES

Brinkmann, C. A., & Co.

1960: 1 Apr., 954

Mettler Instrument Corp.

1960: 18 Mar., 779; 22 July, 235

Welch, W. M., Manufacturing Co.

1960: 6 May, 1385; 5 Aug., 367

SCALERS, NUCLEAR

Baird-Atomic, Inc.

1959: 4 Dec., 1505

1960: 17 June, 1765; 22 July, 173

Nuclear-Chicago Corp.

1960: 18 Mar., 865

Packard Instrument Co., Inc.

1959: 23 Oct., 1041; 11 Dec., 1628

1960: 22 Jan., 196; 29 Apr., 1286; 10 June, 1704; 5 Aug., 322; 16 Sept., 706

Pickering X-Ray Corp.

1959: 13 Nov., 1304

1960: 22 Jan., 187; 19 Feb., 461; 15 July, 107; 12 Aug., 379; 23 Sept., 775

Radiation Counter Laboratories, Inc.

1960: 19 Feb., 545; 22 Apr., 1235

Radiation Instrument Development Laboratory, Inc.

1960: 23 Sept., 847

Technical Associates

1960: 5 Aug., 372

Technical Measurement Corp.

1959: 9 Oct., 894; 23 Oct., 1048

1960: 19 Feb., 476; 22 Apr., 1162; 13 May, 1404; 26 Aug., 516; 16 Sept., 704

Tracerlab, Inc.

1959: 23 Oct., 1037

1960: 17 June, 1770

Victoreen Instrument Co.

1959: 23 Oct., 1131; 13 Nov., 1304

SCINTILLATION CRYSTALS

Harshaw Chemical Co.

1959: 2 Oct., 869; 4 Dec., 1595

1960: 19 Feb., 539; 8 Apr., 1055; 10 June, 1747; 19 Aug., 477; 7 Oct., 965

Isomet Corp.

1959: 23 Oct., 1139

Pilot Chemicals, Inc.

1960: 19 Feb., 555; 22 Apr., 1258; 17 June, 1842; 26 Aug., 572

SHAKERS

New Brunswick Scientific Co., Inc.

1959: 9 Oct., 929; 16 Oct., 993; 30 Oct., 1202; 13 Nov., 1351; 20 Nov., 1432; 27 Nov., 1489; 4 Dec., 1581

1960: 1 Jan., 47; 22 Jan., 255; 29 Jan.,

new **THERMOLYNE**

micro size

hot plate

< 3 9/16" dia. >



Precise, stepless
thermostatic control,
from 6°C above
ambient to 370°C (700°F)

Type 2300—invaluable for those laboratory situations where a single or multiple heat source is needed, yet space and money are scarce. Ruggedly built to withstand hard, continuous usage. Takes less than nine minutes to reach 370°C top temperature (reserve power at 370°C is 46%). Perforated stainless steel case . . . well ventilated . . . long-life heating element . . . cast aluminum top. Stepless control automatically compensates for fluctuations in line voltage and ambient temperatures. Easily read control dial 3 9/16" dia top plate . . . 3 3/4" height. 115 v a-c. Price complete with 5' cord and 3-prong plug,

\$15.00



THERMOLYNE CORPORATION

(Formerly Thermo Electric Mfg. Co.)

568 Huff St., Dubuque, Iowa

309; 12 Feb., 426; 19 Feb., 559; 18 Mar., 877; 22 Apr., 1235; 27 May, 1626; 10 June, 1747; 17 June, 1938

Palo Laboratory Supplies, Inc.

1960: 22 Apr., 1268

SHIELDS, LEAD

Instrument and Development Products Co., Inc.

1960: 18 Mar., 863

Instruments for Research and Industry

1960: 18 Mar., 878

Technical Associates

1960: 18 Mar., 865; 20 May, 1563; 22 July, 247

SIEVES

Custom Scientific Instruments, Inc.

1960: 22 Jan., 234; 22 July, 236; 23 Sept., 834

New York Laboratory Supply Co., Inc.

1960: 18 Mar., 863

SLIDE RULES

Edmund Scientific Co.

1960: 22 Apr., 1138; 17 June, 1764; 22 July, 259; 26 Aug., 508

SKELETON MODEL

Welch, W. M., Manufacturing Co.

1959: 4 Dec., 1589

1960: 1 July, 51

SPECTROMETERS

Baird-Atomic, Inc.

1959: 23 Oct., 1021

Bausch & Lomb Optical Co.

1960: 29 July, 268

Bendix Aviation Corp., Cincinnati Div.

1959: 13 Nov., 1355

1960: 19 Feb., 553; 18 Mar., 880; 20 May, 1567; 17 June, 1821; 26 Aug., 557

Farrand Optical Co., Inc.

1960: 22 Jan., 237

High Voltage Engineering Corp.

1960: 26 Feb., 576; 18 Mar., 798

Leitz, E., Inc.

1959: 4 Dec., 1529

1960: 4 Mar., 624

Nuclear-Chicago Corp.

1960: 1 Apr., 1000

Packard Instrument Co., Inc.

1959: 2 Oct., 830; 16 Oct., 946; 23 Oct., 1041; 13 Nov., 1306; 27 Nov., 1448; 11 Dec., 1628; 25 Dec., 1734

1960: 8 Jan., 72; 22 Jan., 196; 5 Feb., 328; 19 Feb., 478; 4 Mar., 634; 18 Mar., 800; 22 Apr., 1152; 13 May, 1406; 27 May, 1582; 24 June, 1862; 8 July, 60; 22 July, 190; 19 Aug., 440; 2 Sept., 590; 30 Sept., 864

Perkin-Elmer Corp., Instrument Div.

1959: 4 Dec., 1496

1960: 15 Jan., 124

Phillips Electronics, Inc.

1959: 13 Nov., 1285

Picker X-Ray Corp.

1959: 23 Oct., 1015; 13 Nov., 1304

1960: 22 Jan., 187; 22 Apr., 1151


Radiation Instrument Development Laboratory, Inc.

1960: 23 Sept., 847

Technical Associates

1960: 20 May, 1563

FROM A SIMPLE ADDITION to a COMPLETE LABORATORY —

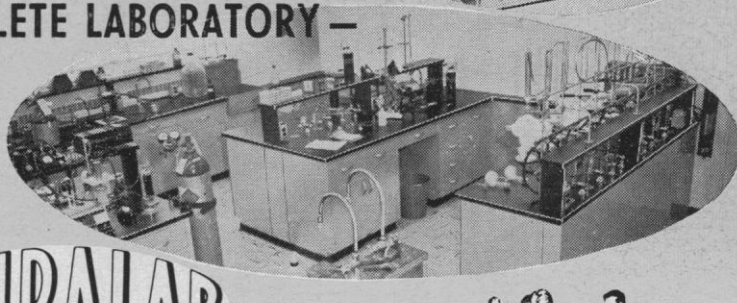

THE
DURALAB

TEAM works
for you!*



Send for our new complete Catalog D5

Sweets File No. 23L

DU

A.I.A. File No. 35-E

Working directly with architects, engineers and lab personnel, your particular requirements are integrated into plans for a finished job to serve you efficiently, economically and provide for the utmost in utility.

- * 8 Engineering Services available to you at no additional cost.
- Preliminary Layouts
- Specifications
- Budgetary Estimates
- Firm Estimates
- Detailed Plans
- Controlled Manufacturing Procedures
- On-Time Deliveries
- Precision Installations

FACTORY TRAINED FIELD REPRESENTATIVES
IN PRINCIPAL CITIES

DURALAB EQUIPMENT CORP.

Manufacturers and Designers of Laboratory Furniture & Equipment

980 LINWOOD STREET, BROOKLYN, N. Y.

PICK ONE (OR MORE)

DUAL TISSUE GRINDERS

... WE NOW HAVE SIX SIZES

The Duall Tissue Grinders have proved so popular that we're forced (quite willingly) to offer two new small sizes. One has an operating capacity of 1 ml.; the other 3 ml. These, with the four larger sizes already offered, provide capacities up to 50 ml.

Why is the Duall so popular? The homogenizer's unique design allows two-stage grinding on its conical and cylindrical surfaces. Particle size reduction starts in the conical section. Final homogenization occurs when material is forced past the cylindrical surfaces. Here uniform particle size is attained.

Bulletin 460A gives full information on the entire Duall line (both Teflon and glass pestles are offered). Write for your free copy.

Catalog No. K-88545 Duall Tissue Grinder—All Glass

Size	Capacity ml.	COMPLETE
AA	1	9.05
A	3	9.05




**KONTES
GLASS
COMPANY**

First Choice For Quality Technical Glassware

Vineland, New Jersey

Midwest Distributor: Research Apparatus, Inc., Wauconda, Ill.

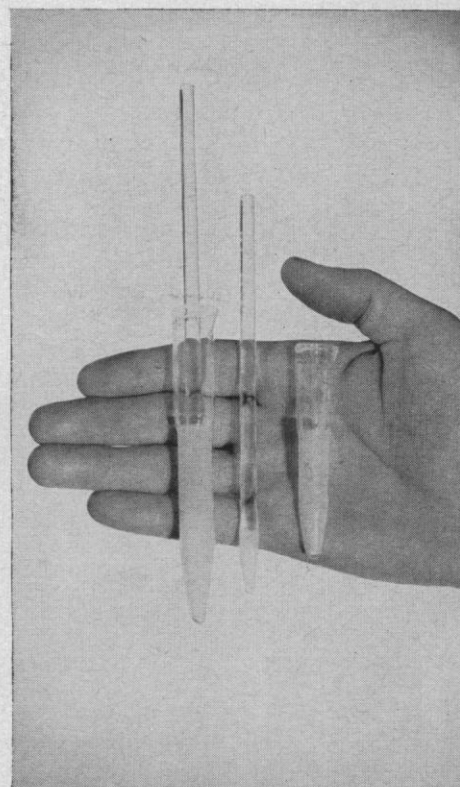

Tracerlab, Inc.

1959: 23 Oct., 1037

Varian Associates

1959: 13 Nov., 1290

1960: 8 Jan., 58; 11 Mar., 696; 6 May, 1336; 9 Sept., 639; 7 Oct., 920

Victoreen Instrument Co.

1959: 23 Oct., 1131; 13 Nov., 1304

1960: 18 Mar., 784; 17 June, 1755

SPECTROPHOTOMETERS AND ACCESSORIES**American Electronic Laboratories, Inc.**

1959: 23 Oct., 1139

American Hospital Supply Corp.

1960: 6 May, 1338

Applied Physics Corp.

1959: 23 Oct., 1119; 6 Nov., 1266

1960: 18 Mar., 867; 20 May, 1541; 23 Sept., 823

Bausch & Lomb Optical Co.

1960: 18 Mar., 772, 773; 25 Mar., 896; 8 Apr., 1014; 13 May, 1453; 17 June, 1780; 19 Aug., 479; 7 Oct., 924

Beckman Instruments, Inc., Scientific and Process Instruments Div.

1959: 20 Nov., 1379; 4 Dec., 1500, 1501

1960: 15 Jan., 128; 12 Feb., 379; 15 Apr., 1068; 22 Apr., 1125; 29 July, 305; 12 Aug., 383; 26 Aug., 499; 16 Sept., 699; 7 Oct., 915

Brinkmann, C. A., & Co.

1960: 22 Jan., 215

Brunswick-Balke-Collender Co., Aloe Scientific Div.

1959: 2 Oct., 868

Coleman Instruments, Inc.

1959: 23 Oct., 1047

1960: 8 Apr., 1008; 22 July, 182

Gilson Medical Electronics

1960: 8 Jan., 117

National Instrument Laboratories, Inc.

1959: 23 Oct., 1032

New York Laboratory Supply Co., Inc.

1959: 23 Oct., 1135

1960: 23 Sept., 843

Perkin-Elmer Corp., Instrument Div.

1959: 20 Nov., 1376; 4 Dec., 1496

1960: 29 Jan., 264; 11 Mar., 686; 20 May, 1464; 17 June, 1756; 16 Sept., 696

Scientific Glass Apparatus Co., Inc.

1960: 23 Sept., 832

Thomas, Arthur H., Co.

1960: 8 Jan., 120; 19 Feb., 472

Will Corp.

1960: 19 Feb., 561; 18 Mar., 847

Zeiss, Carl, Inc.

1960: 22 Apr., 1142

ISOLATE CHROMATOGRAPH FRACTIONS QUICKLY, ACCURATELY

HAMILTON FRACTION COLLECTOR



You can isolate exceedingly pure gas chromatograph fractions for supplemental analysis with this *single* instrument—the Hamilton Fraction Collector! It uses the “Freeze-Out” method of fraction collection, capturing the sample in a U tube on ultra pure silica sand chilled to liquid nitrogen temperatures... *providing up to 98% plus recovery!*

- Rapid, easy, one stroke operation
- Available with heated line for high boiling fractions
- 10 second preparation; samples at 5 second intervals
- Unlimited fractions from single run
- Economical fraction containers, no stopcocks, need no grease



Order direct, or write today for literature and prices.
Also available through your supply house.

HAMILTON COMPANY, INC.
P. O. Box 307-K Whittier, California

PRECISION MEASURING EQUIPMENT FOR CLINICAL AND MEDICAL RESEARCH

SPECTROSCOPES AND ACCESSORIES**Bausch & Lomb Optical Co.**

1960: 26 Feb., 578; 3 June, 1640; 23 Sept., 784

Edmund Scientific Co.

1960: 8 Jan., 69; 18 Mar., 791

Fisher Scientific Co.

1960: 17 June, 1759

Isomet Corp.

1959: 4 Dec., 1601

1960: 18 Mar., 883

Lafayette Radio

1959: 23 Oct., 1013

Radio Corporation of America

1959: 23 Oct., 1018

Zeiss, Carl, Inc.

1959: 9 Oct., 893

1960: 8 July, 56; 9 Sept., 679

STERILIZERS**American Sterilizer Co.**

1959: 23 Oct., 1009

1960: 19 Feb., 443; 22 July, 177

Hospital Supply Co., Inc.

1959: 23 Oct., 1142; 13 Nov., 1354; 4 Dec., 1592

Wilmot Castle Co.

1959: 23 Oct., 1039; 13 Nov., 1291

1960: 18 Mar., 764; 20 May, 1472; 26 Aug., 504; 2 Sept., 588

STILLS**American Sterilizer Co.**

1960: 22 July, 177; 23 Sept., 761

Barnstead Still and Sterilizer Co.

1959: 23 Oct., 1042

1960: 18 Mar., 854; 22 Apr., 1248; 20 May, 1566; 26 Aug., 576

Smith, Arthur F., Co.

1959: 23 Oct., 1005

1960: 18 Mar., 758; 20 May, 1470; 23 Sept., 827

STIMULATORS**American Electronic Laboratories, Inc.**

1959: 23 Oct., 1139; 4 Dec., 1581

1960: 22 Jan., 233; 18 Mar., 778; 23 Sept., 825

Harvard Apparatus Co., Inc.

1960: 19 Feb., 533

THE HUGHES ION PUMP

**NEW IONIZATION PUMP
OFFERS FAST PUMPING AND
LONG LIFE**

When your ultra-high-vacuum requirements demand fast pumping and long life at *low cost*, a full range of Hughes Ion Pumps is available to fill your needs.

One example is the fast, 6-liter-per-second pump. This advanced, ultra-high vacuum ionization pump offers you:

Long operating life: Up to 50,000 hours! Made clean. Designed to stay clean.

Trouble-free operation: No refrigerants, traps, oils or heating elements to repair or replace.

High efficiency: Maintains pressures from 10^{-4} to 10^{-9} mm Hg in closed vacuum systems.


Small size: Only 5" x 3" x 5"

Versatility: Useable on either metal or glass vacuum systems.

Dual usage: Gauges as it pumps.

For complete information and detailed specifications on the new Hughes Ion Pump, write or wire today:
**HUGHES, Vacuum Tube Products Division,
2020 Short Street, Oceanside, Calif.**

For export information, write: Hughes International, Culver City, California.

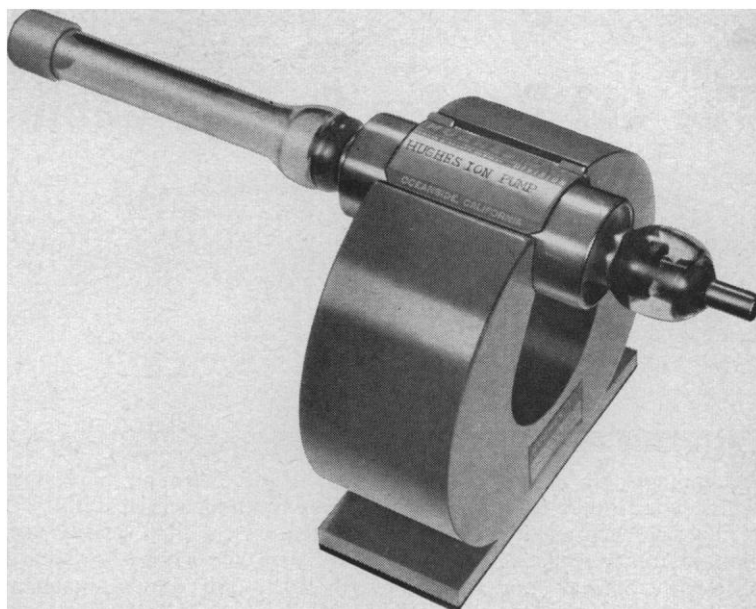

*See the Hughes Ion Pump and the complete line of Hughes vacuum gauges and controls on display at
WESCON — Booths: 2826-2827.*

Creating a new world with ELECTRONICS

HUGHES

**VACUUM TUBE PRODUCTS DIVISION
HUGHES AIRCRAFT COMPANY**

THE PRICE OF PPO HAS (2,5-DIPHENYLOXAZOLE) JUST BEEN CUT IN HALF!

*You save exactly 50%
on highest purity
scintillation grade
PPO* when you specify*




PILOT


**The quality of Pilot PPO remains exactly as before — unsurpassed!*

FOR FREE SAMPLES WRITE: PILOT CHEMICALS, INC., 36 PLEASANT STREET, WATERTOWN 72, MASSACHUSETTS

For Sub-Zero Storage The CSI Dry Ice Storage Cabinet

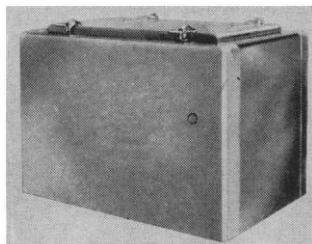

MODEL GS-34

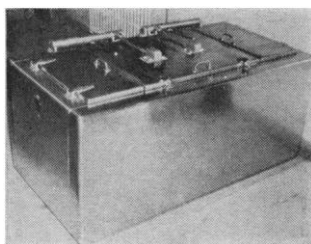

SPECIAL


All cabinets are manufactured of welded and polished stainless steel which contributes to cleanliness, appearance and serviceability. Efficiency has been accounted for in such features as high quality insulation, interchangeable storage inserts and size. The width allows passage through a normal door and the length is the only dimension changed in the three sizes. The cabinets are built with or without the CO₂ entering the storage compartment. The cabinet on the left is our standard model and the unit on the right is specially constructed to the customer's design.

Folder and Prices Upon Request

CUSTOM SCIENTIFIC INSTRUMENTS, INC.

541 Devon St.

Kearny, N.J.

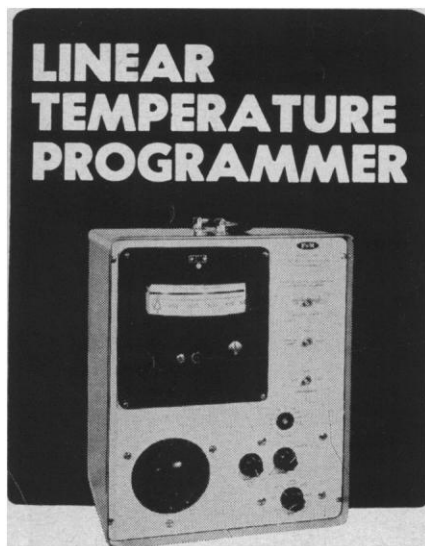

THE F&M MODEL 40 LINEAR TEMPERATURE PROGRAMMER linearly increases temperature of heating equipment or maintains it at constant temperature. 18 linear heating rates from 0.3 to 42°C/min. are provided from 0 to 500°C; adaptable to 1600°C.


WRITE FOR BROCHURE 40

F&M

F&M SCIENTIFIC CORP.

1202 ARNOLD AVE., N. C. C. AIR BASE
NEW CASTLE, DEL. PHONE EA 8-6606

STEREO- MICROSCOPE

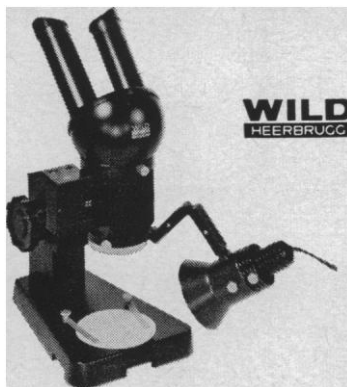

PROMPT DELIVERY

Long Working Distance
Reasonably Priced
Magnifications 5X-160X
Large Variety of Accessories
Old World Craftsmanship

ERIC SOBOTKA CO.

108 West 40th St.

New York 18, N. Y.

Specialists in Imported Equipment

STIRRERS

Ace Glass, Inc.

1960: 18 Mar., 855

Central Scientific Co.

1960: 26 Feb., 619; 22 Apr., 1236; 17 June, 1838

Eastern Industries, Inc.

1959: 13 Nov., 1296

1960: 18 Mar., 840; 17 June, 1830; 23 Sept., 838

Kontes Glass Co.

1959: 13 Nov., 1366

LaPine, Arthur S., and Co.

1960: 19 Feb., 560; 20 May, 1550

Smith, Arthur F., Inc.

1960: 22 Apr., 1253; 22 July, 251

Standard Scientific Supply Corp.

1960: 20 May, 1544; 26 Aug., 564

Thomas, Arthur H., Co.

1959: 4 Dec., 1494

Tri-R Instruments

1959: 23 Oct., 1137

1960: 22 Apr., 1258

STOPCOCKS AND ACCESSORIES

Ace Glass, Inc.

1960: 23 Sept., 829

Corning Glass Works

1960: 5 Feb., 322, 323; 3 June, 1636

Fischer & Porter Co.

1959: 13 Nov., 1287

1960: 22 Apr., 1137

Kimble Glass Co.

1959: 30 Oct., 1164; 6 Nov., 1222; 20 Nov., 1375; 4 Dec., 1519; 18 Dec., 1675

1960: 22 Jan., 183; 12 Feb., 381; 13 May, 1399; 10 June, 1701; 8 July, 58; 12 Aug., 381

Kontes Glass Co.

1959: 16 Oct., 985

Scientific Glass Apparatus Co., Inc.

1959: 11 Dec., 1662

1960: 19 Feb., 466

Thomas, Arthur H., Co.

1959: 13 Nov., 1372

Will Corp.

1960: 22 Apr., 1267; 27 May, 1625

STOPPERS

Thomas, Arthur H., Co.

1960: 27 May, 1632; 24 June, 1900

STOPWATCHES

Heuer Timer Corp.

1960: 22 Jan., 250

STORAGE CABINETS, DRY ICE

Custom Scientific Instruments, Inc.

1960: 18 Mar., 840; 20 May, 1546

STUDENT SCIENCE MATERIALS

American Electronic Laboratories, Inc.

1960: 23 Sept., 825

Atomic Associates, Inc.

1959: 4 Dec., 1505

Bausch & Lomb Optical Co.

1960: 26 Feb., 578; 22 Apr., 1164; 3 June, 1640; 23 Sept., 784


Central Scientific Co.

1959: 16 Oct., 988; 30 Oct., 1203; 13 Nov., 1368; 4 Dec., 1581; 11 Dec., 1666

1960: 15 Jan., 164; 22 Jan., 255; 12 Feb., 426; 11 Mar., 744; 18 Mar., 857; 15

KJELDAHL APPARATUS

for protein determination

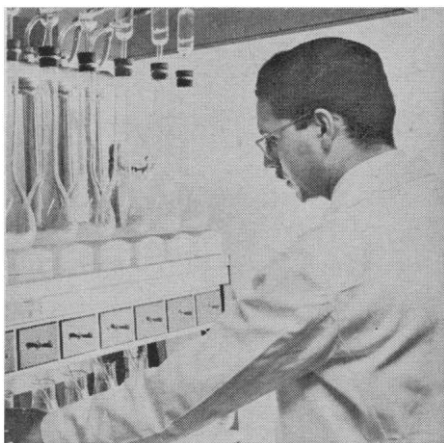

LABCONCO



Wrote
the
book

... Here it is. Get your copy now. No cost, no obligation.

Labconco is the world's largest manufacturer of Kjeldahl apparatus for protein determination. We also manufacture a complete line of fat extractors, crude fiber condensers and other apparatus and equipment for agricultural and allied laboratories. See what's new in the world's most complete line in this field. Get your copy of our new catalog today. Just write . . .

**Laboratory
Construction
Company**

8811 Prospect, Kansas City 32, Mo.

Apr., 1108; 13 May, 1452; 20 May, 1549; 17 June, 1833; 19 Aug., 482

Edmund Scientific Co.

1959: 9 Oct., 886; 6 Nov., 1221; 27 Nov., 1446; 4 Dec., 1506

1960: 8 Jan., 69; 19 Feb., 459; 18 Mar., 791; 22 Apr., 1138; 27 May, 1631; 17 June, 1764; 22 July, 259; 26 Aug., 508; 23 Sept., 855

Elgeet Optical Co., Inc.

1959: 13 Nov., 1301

1960: 22 Jan., 186; 18 Mar., 793; 20 May, 1487; 10 June, 1699; 22 July, 185; 5 Aug., 318; 19 Aug., 491; 2 Sept., 631; 16 Sept., 698; 7 Oct., 914

Graf-Apsco Co.

1959: 23 Oct., 1121; 4 Dec., 1595

1960: 22 Jan., 237; 19 Feb., 563; 22 Apr., 1244; 20 May, 1549; 9 Sept., 686; 23 Sept., 816

Harvard Apparatus Co., Inc.

1959: 4 Dec., 1605

International Equipment Co.

1959: 25 Dec., 1730, 1731

Leitz, E., Inc.

1959: 23 Oct., 1033; 18 Dec., 1674

Mistaire Laboratories

1959: 27 Nov., 1489; 4 Dec., 1608; 11 Dec., 1660; 18 Dec., 1714

Nuclear-Chicago Corp.

1959: 27 Nov., 1492; 11 Dec., 1672

1960: 19 Feb., 570; 29 Apr., 1332; 8 July, 104

Packard Instrument Co., Inc.

1960: 29 Apr., 1286; 10 June, 1704; 5 Aug., 322; 16 Sept., 706

Pickering X-Ray Corp.

1960: 12 Aug., 379; 23 Sept., 775

Pioneer Scientific Corp.

1960: 16 Sept., 703

Science Materials Center

1959: 6 Nov., 1217

Technical Measurement Corp.

1960: 19 Feb., 476; 16 Sept., 704

United Scientific Co.

1959: 30 Oct., 1201

1960: 22 Jan., 176; 4 Mar., 677; 1 Apr., 996; 15 Apr., 1064; 22 Apr., 1246; 13 May, 1454; 20 May, 1562; 15 July, 156; 16 Sept., 748; 30 Sept., 902

Welch, W. M., Manufacturing Co.

1959: 4 Dec., 1589

1960: 1 Jan., 51; 3 June, 1685

Will Corp., Bronwill Scientific Div.

1960: 18 Mar., 864; 8 Apr., 1055; 9 Sept., 680

SURVEYING INSTRUMENTS

Wild Heerbrugg Instruments, Inc.

1959: 9 Oct., 890; 23 Oct., 1046; 6 Nov., 1218; 20 Nov., 1435; 4 Dec., 1530; 18 Dec., 1678

1960: 8 Jan., 68; 22 Jan., 230; 29 Jan., 263; 12 Feb., 380; 26 Feb., 614; 11 Mar., 694; 18 Mar., 796; 8 Apr., 1010; 22 Apr., 1260; 13 May, 1400; 27 May, 1627; 10 June, 1700; 24 June, 1858; 8 July, 95; 22 July, 250; 12 Aug., 378; 19 Aug., 486; 26 Aug., 552; 9 Sept., 685; 23 Sept., 828

Zeiss, Carl, Inc.

1960: 26 Feb., 621

SYRINGES AND ACCESSORIES

Hamilton Co., Inc.

1959: 9 Oct., 930; 23 Oct., 1136; 25 Dec., 1764

1960: 18 Mar., 852; 25 Mar., 944; 22

COLORIMETRIC DETERMATUBE C-LDH

A modification of the regular DERMATUBE LDH (reading at 340 m μ), which makes it possible to determine LDH activity in the visible light region (600 m μ) using any standard laboratory colorimeter.

All that is necessary in either case, is to dissolve the contents of the vial, add serum, and read.



Recent work by Wroblewski and Riley (Science 132, 151, 1960) would seem to indicate that serum lactic dehydrogenase activity is elevated in animals with various experimental tumors and in some patients with malignant neoplasia.

As research along these and similar lines progresses, it becomes increasingly important to have available simplified means for making accurate determinations.

May we suggest that you write for the Worthington booklet on Enzyme Reagents to:

worthington
BIOCHEMICAL CORPORATION
FREEHOLD 1, NEW JERSEY

Apr., 1234; 22 July, 253; 26 Aug., 513; 23 Sept., 831

Phipps & Bird, Inc.

1960: 25 Mar., 943; 1 Apr., 997; 8 Apr., 1051

Scientific Industries, Inc.

1960: 23 Sept., 834

TACHOMETERS

Sticht, Herman H., Co., Inc.

1959: 23 Oct., 1137

TAPE RECORDERS

Precision Instrument Co.

1960: 23 Sept., 852; 7 Oct., 963

TEACHING MACHINES

Foringer & Co., Inc.

1959: 4 Dec., 1603

TELESCOPES

Edmund Scientific Co.

1959: 9 Oct., 886; 27 Nov., 1446; 4 Dec., 1506

1960: 8 Jan., 69; 19 Feb., 459; 18 Mar., 791; 27 May, 1631; 17 June, 1764; 22 July, 259; 26 Aug., 508; 23 Sept., 855

United Scientific Co.

1959: 30 Oct., 1201; 6 Nov., 1266; 4 Dec., 1584

1960: 8 Jan., 114; 6 May, 1388; 5 Aug., 364

Zeiss, Carl, Inc.

1960: 26 Feb., 621

TEMPERATURE CONTROL EQUIPMENT

Brinkmann, C. A., & Co., Inc.

1959: 6 Nov., 1219, 1270; 4 Dec., 1609

1960: 5 Feb., 361; 22 Apr., 1241; 20 May, 1549

F & M Scientific Corp.

1960: 18 Mar., 766; 22 July, 252

Instruments for Research and Industry

1959: 23 Oct., 1148

1960: 19 Feb., 546; 18 Mar., 878

National Appliance Co.

1960: 8 Apr., 1056

Will Corp., Brownwill Scientific Div.

1959: 23 Oct., 1110

1960: 19 Feb., 450; 22 Apr., 1146; 17 June, 1769; 26 Aug., 507

THERMOMETERS

Greiner, Emil, Co.

1960: 18 Mar., 858

Instruments for Research and Industry

1960: 22 Apr., 1266; 20 May, 1566

New York Laboratory Supply Co., Inc.

1959: 20 Nov., 1431

Tri-R Instruments

1959: 23 Oct., 1137

1960: 18 Mar., 864; 23 Sept., 816

Yellow Springs Instrument Co., Inc.

1960: 23 Sept., 818

TIMERS

Foringer & Co., Inc.

1959: 4 Dec., 1603

Standard Scientific Supply Corp.

1959: 4 Dec., 1596

1960: 22 Apr., 1254

TISSUE CULTURE APPARATUS

Belco Glass Inc.

1959: 23 Oct., 1129; 13 Nov., 1368; 4 Dec., 1507; 18 Dec., 1713

1960: 8 Jan., 113; 22 Jan., 255; 5 Feb., 368; 19 Feb., 539; 4 Mar., 678; 18 Mar., 879; 8 Apr., 1051; 22 Apr., 1243; 6 May, 1385; 20 May, 1542; 3 June, 1689; 17 June, 1842; 8 July, 94; 22 July, 257; 5 Aug., 367; 19 Aug., 482; 9 Sept., 684; 23 Sept., 850; 7 Oct., 970

Falcon Plastics Co.

1960: 24 June, 1860; 1 July, 5

Fisher Scientific Co.

1959: 4 Dec., 1606

Harvard Apparatus Co., Inc.

1959: 13 Nov., 1368

Kontes Glass Co.

1959: 4 Dec., 1588

1960: 22 Jan., 253; 19 Feb., 558; 18 Mar., 859; 22 Apr., 1228; 20 May, 1536; 22 July, 252

Nalge Co., Inc.

1960: 26 Aug., 570; 23 Sept., 824

TITRATION EQUIPMENT

Boekel, Wm., & Co., Inc.

1960: 20 May, 1537

Brinkmann, C. A., & Co., Inc.

1959: 6 Nov., 1219; 13 Nov., 1363

1960: 22 Jan., 215, 216, 218; 29 Jan., 309; 26 Feb., 613; 4 Mar., 673; 25 Mar., 939; 6 May, 1386

Buchler Instruments, Inc., formerly Laboratory Glass & Instruments Corp.

1960: 26 Aug., 572


California Laboratory Equipment Co.

1959: 9 Oct., 929; 6 Nov., 1267; 11 Dec., 1666

Coleman Instruments, Inc.

1959: 18 Dec., 1716

1960: 15 Jan., 166; 20 May, 1560; 23 Sept., 836

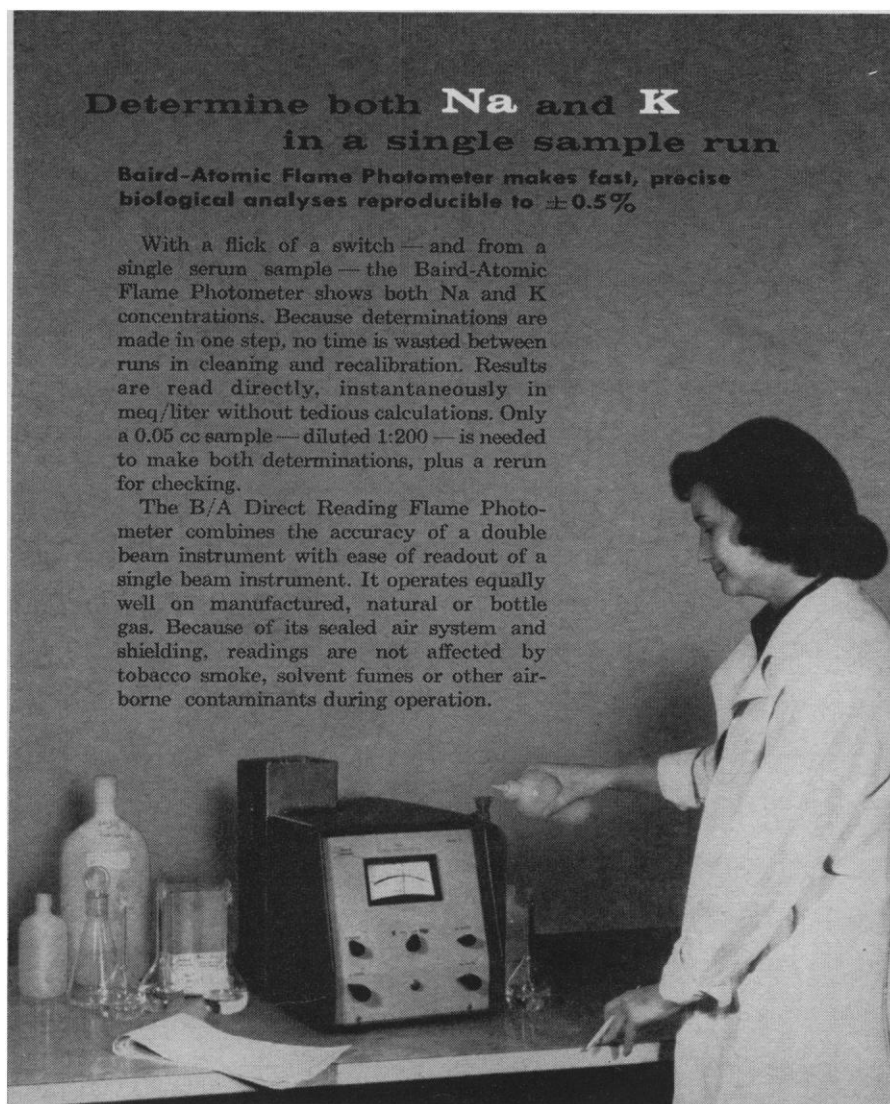

**Determine both Na and K
in a single sample run**

**Baird-Atomic Flame Photometer makes fast, precise
biological analyses reproducible to $\pm 0.5\%$**

With a flick of a switch — and from a single serum sample — the Baird-Atomic Flame Photometer shows both Na and K concentrations. Because determinations are made in one step, no time is wasted between runs in cleaning and recalibration. Results are read directly, instantaneously in meq/liter without tedious calculations. Only a 0.05 cc sample — diluted 1:200 — is needed to make both determinations, plus a rerun for checking.

The B/A Direct Reading Flame Photometer combines the accuracy of a double beam instrument with ease of readout of a single beam instrument. It operates equally well on manufactured, natural or bottle gas. Because of its sealed air system and shielding, readings are not affected by tobacco smoke, solvent fumes or other air-borne contaminants during operation.

Write today for more
complete information.

B/A Flame Photometer Condensed Specifications. Metals Analyzed and Guaranteed Sensitivity (1% of full scale):

Metal	meq/l	mg%	ppm
Na	0.001	0.002	0.02
K	0.0025	0.001	0.01
Li	0.028	0.02	0.02


Reproducibility: $\pm 0.5\%$ av. Size: 15" x 17" x 16" Wgt.: 35 lbs.



BAIRD-ATOMIC, INC.

33 university road • cambridge 38, mass.

Direct Measurement of Difference in Refractive Index

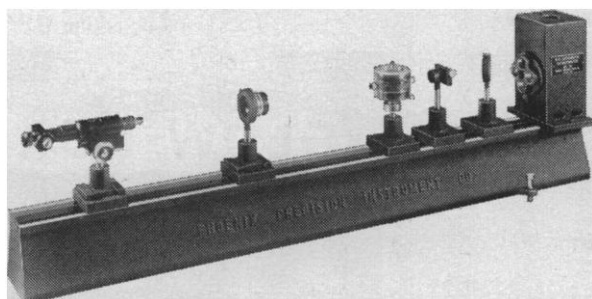


The New Brice-Phoenix Differential Refractometer uses a split cell to measure the difference in refractive index between a dilute solution and its solvent.

Limited sensitivity 3×10^{-6} .

PHOENIX PRECISION INSTRUMENT COMPANY
3805 N. 5th St. Phila. 40, Pa.

THE FINEST IN CAGES FOR LABORATORY DOGS & PRIMATES

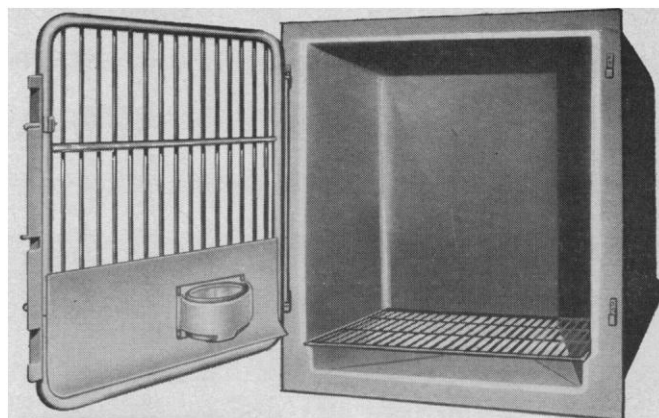

**THE ORIGINAL
TIME-TESTED
GLASS PLASTIC
CAGE**

molded seamless construction of rugged fiber glass reinforced plastics...minimum effort required to clean and disinfect... maximum animal comfort...extremely strong doors with fool proof catches...economical to purchase and maintain....For further information write:
Department KS *Kirschner*
Vashon, Washington

for trouble-free filtration use

**COORS
U.S.A.**

Porous Bottom Crucibles

These can be ignited to extremely high temperatures without cracking of the filtering discs or alteration of the pore size. Easily cleaned and made ready for re-use. Carefully controlled pore sizes in 3 ranges for bacteriological separations and filtering of fine and coarse precipitates.

Special forming techniques have resulted in a porous disc formed into the crucible wall in such a way as to prevent cracking or dropping out during ignition or use. Made of the same high quality materials as Coors Chemical Porcelain, the disc will not disintegrate when acids (except HF) or moderate alkaline solutions are in contact with the porous medium.

Write for Bulletin



COORS PORCELAIN COMPANY GOLDEN, COLORADO



CLASSIFY LABORATORY QUANTITIES

for product or new
material research


DETERMINE PARTICLE SIZE DISTRIBUTION

below 60 microns . . . in materials such as:

Beryllium Powder	Grinding Sand
Catalyst	Metal Oxides
Ceramic Powders	Penicillin
Chemicals	Polymers
Diatomaceous Earth	Powdered Metals
Drugs	Milk Solids
Dry Powders	Standard Dust
Fly Ash	Samples

with the
DIETERT-DETROIT
(BAHCO)
**MICRO-PARTICLE
CLASSIFIER**

Model
No. 6000,
totally
enclosed
220 volt,
3 phase
motor,
operates at
3500 rpm.

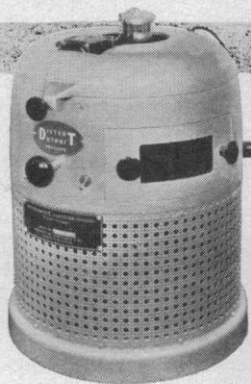

Widely used for particle size control in many industrial processes . . . for scientific study of fine materials . . . for pre-testing dust collector needs . . . for determining the separating efficiency of air cleaners. An 8-fraction analysis can be completed at the rate of 15 minutes per fraction by unskilled operators. Fractions are precisely defined and may be retained for accurate study.

HARRY W. DIETERT CO.
CONTROL EQUIPMENT

9330 ROSELAWN DETROIT 4, MICHIGAN

Send me 8-page Micro-Particle Classifier bulletin.

Name _____
Company _____
Address _____
City _____ State _____

1200

Corning Glass Works

1960: 8 Apr., 1011; 13 May, 1450

Doerr Glass Co.

1959: 13 Nov., 1283; 4 Dec., 1499

Greiner, Emil, Co.

1960: 22 July, 246

Hamilton Co., Inc.

1960: 22 Jan., 254; 20 May, 1558

Instrumentation Associates

1960: 19 Feb., 556; 23 Sept., 840

Kimble Glass Co.

1959: 2 Oct., 823

Kontes Glass Co.

1959: 16 Oct., 985; 30 Oct., 1204; 6 Nov., 1220

LaPine, Arthur S., and Co.

1960: 22 Jan., 250; 23 Sept., 822

Nalge Co., Inc.

1960: 20 May, 1564; 17 June, 1824; 22 July, 248

Polarad Electronics Corp.

1960: 19 Feb., 469; 18 Mar., 787; 20 May, 1475; 22 July, 187

Precision Scientific Co.

1960: 22 Jan., 245

Sargent, E. H., & Co.

1960: 18 Mar., 794; 23 Sept., 780

Scientific Industries, Inc.

1960: 23 Sept., 834

Standard Scientific Supply Corp.

1960: 17 June, 1843

Thomas, Arthur H., Co.

1959: 13 Nov., 1372

1960: 5 Feb., 372

Will Corp.

1960: 22 Apr., 1267; 27 May, 1625

TRANSDUCERS, PRESSURE

Sanborn Co.

1959: 11 Dec., 1623

TUBE FITTINGS

Beckman Instruments, Inc., Scientific and Process Instruments Div.

1960: 23 Sept., 826

VACUUM EQUIPMENT

Ace Glass, Inc.

1960: 22 July, 237

Blickman, S., Inc.

1960: 20 May, 1557

Central Scientific Co.

1959: 27 Nov., 1485

1960: 25 Mar., 941; 29 July, 309

Granville-Phillips Co.

1960: 7 Oct., 970

Greiner, Emil, Co.

1960: 18 Mar., 881

Hevi-Duty Electric Co.

1960: 8 Jan., 111; 4 Mar., 677

Kimble Glass Co.

1960: 22 Jan., 183; 11 Mar., 689

LaPine, Arthur S., and Co.

1960: 18 Mar., 842; 20 May, 1550

National Appliance Co.

1959: 13 Nov., 1353

New York Air Brake Co., Kinney Vacuum Div.

1960: 19 Feb., 533; 18 Mar., 849; 22 Apr., 1225; 17 June, 1819; 19 Aug., 483

New York Laboratory Supply Co., Inc.


1960: 17 June, 1819

Phillips Electronic, Inc.

1960: 17 June, 1766, 1767

Precision Scientific Co.

1960: 17 June, 1828; 22 July, 230

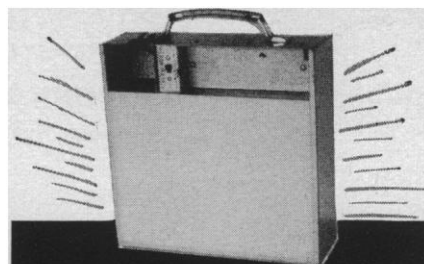

GLOW-BOX

THE SCIENTISTS' LIGHT BOX



STANDS UPRIGHT FOR
DEMONSTRATIONS



TILTS FOR TABLE TOP USE



FITS STANDARD DESK DRAWER
FOR STORAGE OR FOR USE



**INSTRUMENTS for
RESEARCH and
INDUSTRY**
CHELTENHAM, PA.

SCIENCE, VOL. 132

Smith, Arthur F., Inc.
1960: 17 June, 1844
VirTis Co., Inc.
1959: 23 Oct., 1038
Welch, W. M., Manufacturing Co.
1959: 6 Nov., 1267

VALVES

Granville-Phillips Co.
1960: 7 Oct., 970
New York Air Brake Co., Kinney Vacuum Div.
1960: 19 Feb., 533; 18 Mar., 849; 22 Apr., 1225; 17 June, 1819; 19 Aug., 483
Phipps & Bird, Inc.
1960: 16 Sept., 749; 23 Sept., 814

VISCOMETERS

Ferranti Electric, Inc., Electronics Div.
1960: 18 Mar., 861
Fish-Schurman Corp.
1959: 4 Dec., 1608
Polarad Electronics Corp.
1960: 19 Feb., 470; 18 Mar., 788; 20 May, 1475; 22 July, 187

VOLTAGE CONVERTERS

Central Scientific Co.
1960: 15 July, 160

VOLTAGE TESTERS

Sorensen & Co.
1960: 22 Apr., 1223

WARBURG APPARATUS

Gilson Medical Electronics
1959: 11 Dec., 1665
1960: 10 June, 1746; 8 July, 97
Will Corp., Bronwill Scientific Div.
1959: 16 Oct., 989
1960: 19 Feb., 450; 22 Apr., 1146; 17 June, 1769; 26 Aug., 507

WARING BLENDERS

Waring Products Corp.
1959: 30 Oct., 1202, 1203
1960: 8 Apr., 1007; 13 May, 1455; 10 June, 1743; 23 Sept., 825

WASHERS, GLASSWARE

Fisher Scientific Co.
1959: 16 Oct., 992

WATER BATHS


LaPine, Arthur S., and Co.
1960: 19 Feb., 560; 26 Aug., 556
National Appliance Co.
1960: 18 Mar., 850; 9 Sept., 688

WATER PROCESSING SYSTEMS


American Sterilizer Co.
1960: 22 Apr., 1159

X-RAY EQUIPMENT

Philips Electronics, Inc.
1959: 13 Nov., 1284, 1285
1960: 17 June, 1766, 1767
Radio Corporation of America
1959: 23 Oct., 1018; 4 Dec., 1518

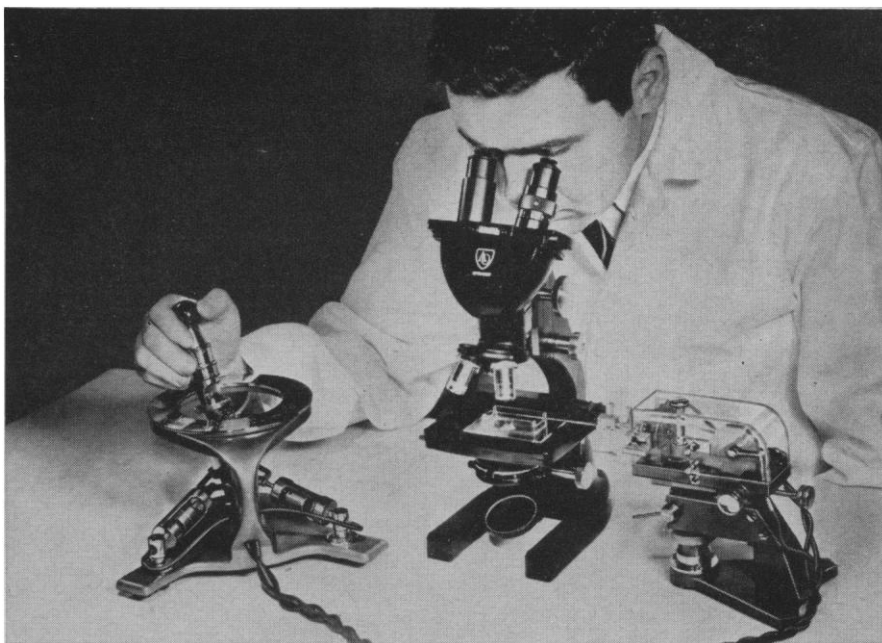

de Fonbrune Micromanipulator — Has Smooth, Uniform Pneumatic Movement



Improved de Fonbrune Micro-Forge With Binocular Body

Specifically developed for use in the fabrication of simple and intricate micro-tools of glass or metal under controlled conditions. Use of the de Fonbrune micro-forge is recommended with any type micromanipulator. The forge is now built with binocular stereoscopic microscope. With this modification, the image is observed erect — not inverted — in three dimensions, an important factor in rapid, accurate work.

Affords new simplicity and flexibility for micro-studies in biological or chemical technics

The de Fonbrune micromanipulator has proved to be of great value in micro-studies in many fields. In biology the instrument is used in cell dissection and isolation . . . micro-injection and operation on protozoa . . . pH studies on living cells . . . isolation and transfer of single bacteria, etc. It has proved equally serviceable in study of fibers and yeast cells, in investigating oils, rust deposits, colloidal, and other materials.


Manufactured under exclusive license of the French patents, the instrument consists of a manipulator and receiver. Use with any microscope . . . arranged for right or left hand operation. The micro-tool is mounted on the receiver; impulses from the manipulator are transmitted to the tool through sensitive pneumatic membranes. Within a range of 3 mm, the micro-instrument may be moved in any plane or angle by a single control. Ratio of displacement of control lever and micro-tool may be adjusted from 1:50 to 1:2500.

Write for prices and descriptive bulletin T114.

aloe scientific

DIVISION OF BRUNSWICK CORPORATION

General Offices: 1831 Olive, St. Louis 3, Missouri
FULLY STOCKED DIVISIONS COAST-TO-COAST



ADVERTISERS APPEARING IN "THE MARKET PLACE"


2 October 1959 through 7 October 1960

MINIATURE WELL-TYPE GAMMA SCINTILLATION PROBE

Model MWC-149

As reliable and convenient as GM counters, but about 100 times more efficient for gammas. 1" x 1" NaI well-type crystal holds up to 1.5 cc. Cable included.

ONLY \$250.00

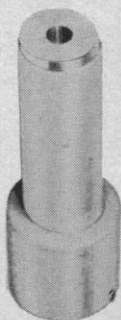

ALL NEW Low Cost TRAINING AIDS for teaching Nuclear Science


WELL SCINTILLATION SYSTEM.. COMPLETE!

Model WSS-93A
consists of:

- MWC-149 Counter
- Tube Mount
- Lead Shield
- Sample Holders

Quantitatively measures small-size samples of gamma emitters in solid or liquid form.

COMPLETE \$350.00



Also Available:

Alpha and Beta Scintillation Probes, plus a full range of educational kits and accessories.

For more details, ask for Bulletin ED-85

ATOMIC
accessories inc.

Subsidiary of Baird-Atomic, Inc.
811 W. Merrick Rd., Valley Stream, N. Y.
CUrtiss 5-9300

Represented Nationally by
Baird-Atomic Sales Offices in:

Boston • New York • Philadelphia
Cleveland • Washington, D.C.
Atlanta • Chicago • Detroit
Dallas • Los Angeles
San Francisco
In Canada:
Ottawa, Ontario

Abrahams Magazine Service
56 E. 13 St., New York 3

Albino Farms
P. O. Box 331, Red Bank, N.J.

American-Lincoln Incubator Co.
New Brunswick, N.J.

Analytica Corp.
118 E. 28 St., New York 16

Animal Research Center
Bainbridge, N.Y.

Applied Science Laboratories, Inc.
108 N. Gill St., State College, Pa.

Badger Research Corp.
P.O. Box 527, Madison 1, Wis.

Bio-Rad Laboratories
32nd and Griffin Ave., Richmond, Calif.

Black Light Eastern Corp.
4 Manhasset Ave., Port Washington, N.Y.

Brookline Surgical Specialties
50 Harris St., Brookline 46, Mass.

Canner's, Inc.
618 Parker St., Boston 20, Mass.

Charles River Breeding Laboratories, Inc.
1093 Beacon St., Brookline 46, Mass.

Colorado Serum Co.
4950 York St., Denver 16, Colo.

Curta Co.
14435 Cohasset St., Van Nuys, Calif.

Dimco-Gray Co.
214 E. 6 St., Dayton 2, Ohio

Dyna Slide Co.
600 S. Michigan Ave., Chicago 29, Ill.

Electro-Medical Laboratory, Inc.
South Woodstock 2, Vt.

Esbe Laboratory Supplies
459 Bloor St. West, Toronto, Canada

Food and Drug Research Laboratories,
Inc.

Maurice Ave. at 58 St., Maspeth 78, N.Y.

Green Hills Farm
Box 381, Jeffersonville, N.Y.

Greenwich Book Publishers
489 Fifth Ave., New York, N.Y.

Hemens, Rollin D.
1225 E. 60 St., Chicago 37, Ill.

Hoeltge Bros., Inc.
1919 Gest St., Cincinnati 4, Ohio

Holling Press
501 Washington St., Buffalo, N.Y.

Hormone Assay Laboratories, Inc.
8159 S. Spaulding Ave., Chicago 29, Ill.

Huntingdon Farms, Inc.
2548 N. 27 St., Philadelphia 32, Pa.

Instruments for Research and Industry
Cheltenham, Pa.

Isotopes Specialties Co.
Box 688, Burbank, Calif.

KBR Associates
120 Liberty St., New York 6

Kern Co.
121 Nassau St., New York 38

Landis, John C.
1908 Virginia Ave., Hagerstown, Md.

LaMotte Chemical Co.
Chestertown, Md.

LaWall & Harrison
1921 Walnut St., Philadelphia 3, Pa.

Library of Congress
Washington 20, D.C.

Mackesey Farms
Box 166, Route 4, Madison, Wis.

Maxwell, Meier & Holmes, Inc.
103 Fifth Ave., New York 3

Microbiological Research & Consulting
Laboratory
618 E. South St., Orlando, Fla.

Microchemical Specialties Co.
1825 Eastshore Highway,
Berkeley 10, Calif.

Monitron Co.
1815 Willaroy Terrace, Cincinnati 30, Ohio

Nelles Translations
119 W. Ontario St., Chicago 10, Ill.

Orlando Research, Inc.
P.O. Box 6491, Orlando, Fla.

Oxford Laboratories
961 Woodside Rd., Redwood City 3, Calif.

Pathway Research Laboratories, Inc.
11102 S. Artesian Ave., Chicago 43, Ill.

Pel-Freez Rabbit Meat Co.
Rogers, Ark.

Regis Chemical Co.
1219 N. Wells St., Chicago 10, Ill.

Research Animals, Inc.
3401 Fifth Ave., Pittsburgh 13, Pa.

Rider, John F., Publisher, Inc.
116 W. 14 St., New York 11

Rozsa, George L.
142 Linwood Ave., Buffalo 9, N.Y.

Science Materials Center
59 Fourth Ave., New York 3

Scientific Equipment Co.
Box 19086, Indianapolis 19, Ind.

Scientific & Laboratory Appliances
61-C Reade St., New York 7

Scientific Publishing Co.
2328 Eutaw Place, Baltimore 17, Md.

S & K Animal Co.
Box 479A, Jamesburg, N.J.

Slavic Library
3330 13th St., Boulder, Colo.

Taconic Farms
Germantown, N.Y.

Texas Inbred Mice Co.
305 Alameda-Genoa Rd., Houston 21, Tex.

United States Testing Co., Inc.
1415 Park Ave., Hoboken, N.J.

University of Colorado
Boulder, Colo.

Van Nostrand, D., Co., Inc.
120 Alexander St., Princeton, N.J.

Vantage Press
120 W. 31 St., New York 1

Wabash Metal Products Co.
1614 Morris St., Wabash, Ind.

Wilkens Instrument & Research Inc.
Box 313, Walnut Creek, Calif.

Wisconsin Alumni Research Foundation
P.O. Box 2217, Madison 1, Wis.

Zenith Optical Laboratory
Copiague, L.I., N.Y.

Just Published: Vol. 14 (391 pages)

ANNUAL REVIEW OF

MICROBIOLOGY

Editors: C. E. Clifton, S. Raffel, M. P. Starr
Editorial Committee: C. E. Clifton, C. A. Evans,
R. E. Hungate, T. L. Jahn, P. R. Miller, W. W.
Umbreit

Contents:

Variation in Phytopathogenic Fungi
Microbial Nutrition
Intramural Spread of Bacteria and Viruses in
Human Populations
Protein Synthesis in Microorganisms
Energy Metabolism in Chemolithotropic Bacteria
Industrial Fermentations
Intracellular Symbiosis in Insects
Nutrition, Metabolism, and Pathogenicity of Mi-
croorganisms
Interpretations of Immunodiffusion Tests
In Vitro Cell-Virus Relationships Resulting in Cell
Death
The Genetics and Cytology of *Chlamydomonas*
Fine Structure of Virus-Infected Cells
Enzyme Localization in Bacteria
Arthropod-Borne Viruses of Man and Other Ani-
mals
Synchronous Division of Microorganisms
Gene Action
Immunological Speculations


\$7.00 postpaid (U.S.A.); \$7.50 postpaid (elsewhere)

ANNUAL REVIEWS, INC.

231 GRANT AVENUE, PALO ALTO, CALIFORNIA

TESTMATIC BALANCE

Excitingly New!

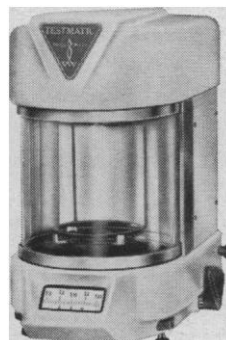

*Write for further
information.
Dealer inquiries
invited.*

For fast repetitive weighing the Test-
matic Balance is a leader in its field.
The superb performance of this remark-
able balance was created by the world's
finest Swiss craftsmen. Check it over
feature by feature and you will see why.

- **Direct optical readout with 1000 divi-
sions on the scale.**
- **Easy to read scale divisions 2.5 mm
apart.**
- **Scale is in direct line of sight with
the pan.**
- **The Testmatic is priced surprisingly
low.**


MODEL TYPE	T-1	T-10	T-100
Optical Scale in Grams	0-1 g.	0-10 g.	0-100 g.
Scale Divisions	1-mg	10-mg	100-mg
Legibility with Vernier	0.1-mg	1-mg	10-mg
Weighing Time	8-Sec.	3-5 Sec.	2-3 Sec.

C. H. STOELTING CO.

Analytical Balances, Micro-Manipulators, Stereotaxic
Instruments, Strip Chart Recorders, Polygraphs,
Research Microscopes, Kymographs


424 NORTH HOMAN AVENUE, CHICAGO 24, ILL.

TRI-R VERSATILE LABORATORY INSTRUMENTS

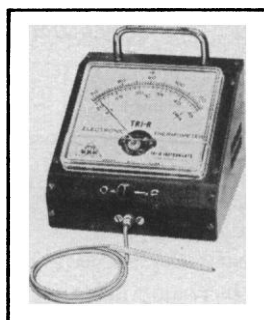


ELECTRONIC THERMOMETER

- Rapid, Accurate, Direct
Reading
- Low Cost, Portable,
Thermistor Type
- Many Ranges from -35
to +100° C.
- Interchangeable & Spe-
cial Probes
- Controllers & Recorders
Available

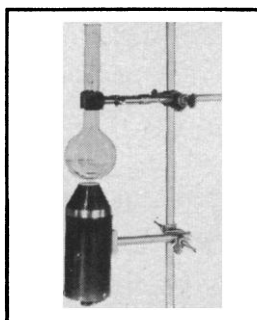

COMPACT MAGNETIC STIRRER

- Stir at Any Angle
- In Open or Closed Ves-
sels
- Under Vacuum or Pres-
sure
- With or without Hot-
plate

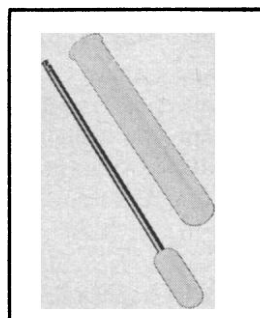

TEFLON TISSUE HOMOGENIZERS

- Interchangeable Teflon
Pestles
- Precision Bore Pyrex
Glass Tubes
- Notched for Quick
Change Chuck
- Complete Apparatus
Available



AUTOMATIC EGG-PUNCH

- For Opening Embryo-
nated Eggs
- Open 60 Eggs Per Min-
ute
- Clean 1" Circular Frac-
ture
- One Hand Efficient Op-
eration

*Write for individual bulletins
or complete catalog to Dept. S-10.*

TRI-R INSTRUMENTS

Developers of Electronic and Mechanical Instruments for Scientific Research


144-13 JAMAICA AVENUE, JAMAICA 35, N. Y.

INDEX OF ADVERTISERS—21 October 1960

Abrahams Magazine Service	1207	Falcon Plastics	1037	Pergamon Press	1154
Ace Glass, Inc.	1189	Farrand Optical Co., Inc.	1183	Perkin-Elmer Corp.	1034
Ajusto Equipment Co.	1152	Ferranti Electric, Inc.	1159	Philosophical Library	1158
Albino Farms	1207	Fisher Scientific Co.	1086	Phipps & Bird, Inc.	1191
Alconox, Inc.	1190	Fish-Schurman Corp.	1152	Phoenix Precision Instrument Co.	1180, 1186, 1199
Aloe Scientific Div., Brunswick Corp.	1201	F & M Scientific Corp.	1058, 1196	Photovolt Corp.	1179
American Edelstaal, Inc.	1188	Gilson Medical Electronics	1182	Picker X-Ray Corp.	1073
American Hospital Supply Corp.	1076	Graf-Apsco Co.	1156	Pilot Chemicals, Inc.	1195
American Optical Co.	1212	Greiner, Emil, Co.	1180	Polarad Electronics Corp.	1045
American Sterilizer Co.	1071	Hacker, William J., & Co., Inc.	1057	Precision Instrument Co.	1055
Annual Reviews, Inc.	1203	Hamilton Co., Inc.	1194	Precision Scientific Co.	1164
Anton Electronic Laboratories, Inc.	1149	Harvard Apparatus Co.	1179	Professional Tape Co., Inc.	1151
Atomic Accessories, Inc.	1202	Heller, Gerald K., Co.	1186	Radiation Dynamics, Inc.	1047
Baird-Atomic, Inc.	1083, 1151, 1198	Hoeltge Bros., Inc.	1207	Radiation Instrument Development Laboratory, Inc.	1042
Baker, J. T., Chemical Co.	1085	Hotpack	1172	Raytheon Co.	1032, 1209, 1210
Barber-Colman of Canada, Ltd.	1060	Houston Instrument Corp.	1175	Research Specialties Co.	1176
Barnstead Still and Sterilizer Co.	1168	Hughes Aircraft Co., Vacuum Tube Products Div.	1195	Riseman Development Laboratory	1166
Bausch & Lomb Optical Co.	1090	Huntingdon Farms, Inc.	1207	Ronald Press Co.	1168
Beckman Instruments, Inc., Scientific and Process Instruments Div.	1039	Hyland Laboratories	1153	Rudolph Instruments Engineering Co.	1064
Bello Glass, Inc.	1163	Industrial Instruments, Inc.	1192	Sargent, E. H., & Co.	1046
Bendix Corp., Bendix Computer Div.	1068	Instrumentation Associates, Inc.	1188	Sauter, August, of New York, Inc.	1181
Bethlehem Apparatus Co., Inc.	1157, 1187	Instruments for Research and Industry	1200	Schleicher, Carl, & Schuell Co.	1154
Blickman, S., Inc.	1177	International Equipment Co.	1048, 1049	Schwarz BioResearch, Inc.	1169
Brinkmann Instruments, Inc.	1119	Isotopes, Inc.	1186	Scientific Glass Apparatus Co., Inc.	1059
Bronwill Div., Will Corp.	1070	Isotopes Specialties Co. Div., Nuclear Corporation of America	1163	Scientific Industries, Inc.	1158
Buchler Instruments, Inc.	1183	Jet Propulsion Laboratory	1074	Servonuclear Corp.	1156
Burgess Publishing Co.	1152	Kewaunee Scientific Equipment	1170	Sharp Laboratories, Inc.	1185
Canal Industrial Corp.	1171	Kinney Vacuum Div., New York Air Brake Co.	1177	Sigma Chemical Co.	1205
Canner's, Inc.	1207	Kirschner Manufacturing Co.	1199	Sigmamotor, Inc.	1167
Central Scientific Co.	1051	Klett Manufacturing Co.	1152	Smith, Arthur F., Inc.	1188
Charles River Breeding Laboratories, Inc.	1207	Kling Photo Corp.	1184	Sobotka, Eric, Co.	1196
Coleman Instruments, Inc.	1082	Kontes Glass Co.	1193	Sorvall, Ivan, Inc.	1066, 1067
Colorado Serum Co.	1207	Laboratory Construction Co.	1197	Sprague Dawley, Inc.	1158
Columbia Broadcasting System, Inc., CBS Laboratories Div.	1160	Lafayette Radio	1062	Standard Scientific Supply Corp.	1150
Cooke, Troughton & Simms, Inc.	1061	LaPine, Arthur S., and Co.	1160	Stoelting, C. H., Co.	1203
Coors Porcelain Co.	1199	Leeds & Northrup Co.	1040	Taconic Farms	1207
Custom Scientific Instruments, Inc.	1196	Leitz, E., Inc.	1030	Technical Associates	1036
Danube International Trade Corp.	1148	Lourdes Instrument Corp.	1155	Technical Instrument Co.	1206
Day, Joseph P., Inc.	1146	Mallinckrodt Chemical Works	1069	Technical Measurement Corp.	1088
Despatch Oven Co.	1186	Maryland Plastics, Inc.	1087	Technicon Chromatography Corp.	1181
Dietert, Harry W., Co.	1200	Matheson Co., Matheson Coleman & Bell Div.	1174	Texas Instrument Co.	1053
Difco Laboratories	1167	Mechrolab, Inc.	1148	Thermolyne Corp.	1192
Dimco-Gray Co.	1207	Meinecke & Co., Inc.	1174	Thomas, Arthur H., Co.	1075
Doerr Glass Co.	1033	Mettler Instrument Corp.	1081	Torsion Balance Co.	1065
Donner Scientific Co.	1077	Nalge Co., Inc.	1072	Tracerlab, Inc.	1080
Duralab Equipment Corp.	1193	National Appliance Co.	1170	Tri-R Instruments	1203
Eastman Kodak Co.	1147	National Instrument Laboratories, Inc.	1120, 1121, 1122	United Scientific Co.	1208, 1212
Eaton-Dikeman Co.	1178	New Brunswick Scientific Co., Inc.	1163	Vanguard Instrument Co.	1044
E-C Apparatus Co.	1167	New England Nuclear Corp.	1151	Victoreen Instrument Co.	1079
Edmund Scientific Co.	1078	New York Laboratory Supply Co.	1205	VirTis Co.	1056
Elgeet Optical Co., Inc.	1052	Oak Ridge National Laboratory	1164	Welwyn International, Inc.	1050
Engis Equipment Co.	1173	Packard Instrument Co., Inc.	1054	Wild Heerbrugg Instruments, Inc.	1165
Erb & Gray Scientific, Inc.	1173	Parr Instrument Co.	1184	Will Corp.	1041
Ercon Corp.	1162	Percival Refrigeration & Manufacturing Co.	1191	Wilmot Castle Co.	1038
Esterline-Angus Co.	1184			Winthrop Laboratories	1191
Exact Weight Scale Co.	1161			Wisconsin Alumni Research Foundation	1207
				Worthington Biochemical Corp.	1197
				Zeiss, Carl, Inc.	1043


NYLAB has the

Big Jack

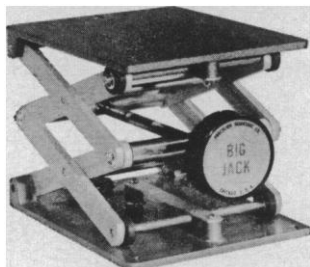

- Lifts up to 100 lbs.
- Opens from 3 to 12 inches
- Ideal for complex set-ups

Little Jack



- Lifts up to 10 lbs.
- Opens from 1½ to 5 inches
- Perfect for micro-set-ups

Two new laboratory jacks offering precise and effortless vertical height adjustment of hotplates, heaters, baths and glassware . . . provide a real lift for your laboratory.

write today for Bulletin 611



New York Laboratory Supply Co., Inc.

76-78 VARICK STREET

NEW YORK 13, N. Y.



Now Available from Sigma PEPTIDES and INTERMEDIATES

N-2,4-DINITROPHENYL-L-ALANINE
N-(2,4-DINITROPHENYL)-L-VALINE
3,5-DINITRO-L-TYROSINE
N-EPSILON FORMYL-L-LYSINE
o-FLUOROPHENYL ALANINE HCl
m-FLUOROPHENYL ALANINE
p-FLUOROPHENYL ALANINE
GLYCYL-GLYCINE or HCl
GLYCYL GLYCINE AMIDE ACETATE
GLYCYL GLYCINE BENZYL ESTER-p-TOLUENE
SULFATE
GLYCYL-L-HISTIDINE
N-GLYCYL-L-ISOLEUCINE
GLYCYL-DL-NORLEUCINE
GLYCYL-DL-NORVALINE
N-GLYCYL-DL-PHENYLALANINE
GLYCYL-L-SERINE
N-GLYCYL-L-TRYPTOPHANE
N-GLYCYL-D-VALINE
DL-β-HYDROXY-β-METHYL-Δ-VALERIC LACTONE
DL-LEUCINE AMIDE HCl
L-LEUCINE BENZYL ESTER-p-TOLUENE
SUFONATE
L-LEUCINE, METHYL ESTER, HCl
L-LEUCYL-β-NAPHTHYLAMIDE, HCl
L-LYSINE ETHYL ESTER diHCl
L-LYSINE METHYL ESTER diHCl
DL-METHIONINE METHYL SULFONIUM
CHLORIDE
β-METHYL ASPARTIC ACID
4-METHYL-DL-TRYPTOPHANE
6-METHYL-DL-TRYPTOPHANE
NITRO-L-ARGININE
p-NITROPHENYL ALANINE
DL-PHENYLALANINE AMIDE HCl
PHTHALOYL-β-ALANINE
PHTHALOYL AMINO BUTYRIC ACID
PHTHALOYL GLYCINE
PHTHALOYL-DL-LEUCINE
PHTHALOYL-DL-METHIONINE
PHTHALOYL-L-PHENYLALANINE
PHTHALOYL GLYCINE
L-SERINE AMIDE HCl
DL-TRYPTOPHANE AMIDE HCl
DL-TRYPTOPHANE METHYL ESTER
L-TYROSINE METHYL ESTER HCl
L-VALINE, METHYL ESTER, HCl
L-VALYL GLYCYL GLYCINE
L-VALYL-L-LEUCINE

Many others are in preparation.

CALL US COLLECT AT ANY TIME, JUST TO GET ACQUAINTED

Day, Station to Station,
PRospect 1-5750

Night, Person to Person,
Dan Broida, WYdown 3-6418



The Research Laboratories of

SIGMA
CHEMICAL COMPANY

3500 DEKALB ST., ST. LOUIS 18, MO., U. S. A.



When it Comes to . . .

MICROSCOPES

CONSULT

Technical Instrument Company

98 GOLDEN GATE AVE.

SAN FRANCISCO 2, CALIF.

You will be pleasantly surprised at their prices and by their service.

Of course, you might ask for a catalog first.

WATER AND AGRICULTURE

A symposium presented at the AAAS
Washington Meeting,
December 1958. Published June 1960.

Roy D. Hockensmith, Editor
6 x 9, 206 pp., 21 illus., cloth
\$5.00 AAAS members' cash orders, \$4.50

CONTENTS

Water for the future: E. A. Ackerman, C. A. Davis, C. B. Brown, and R. L. Nace

Water sources: W. C. Ackermann, H. T. Orville, C. H. M. Van Bavel, and G. L. Barger

Water planning and use: C. H. Wadleigh, H. C. Storey, W. D. Criddle, and W. I. Palmer

Water control: T. W. Edminster, F. L. Timmons, D. L. Klingman, G. E. Harbeck, Jr., and C. B. Tanner

British agents: Bailey Bros. & Swinfen, Ltd.
Hyde House, West Central Street
London, W.C.1

**American Association for the
Advancement of Science**

1515 Massachusetts Avenue, NW
Washington 5, D.C.

PERSONNEL PLACEMENT

CLASSIFIED: Positions Wanted, 25¢ per word, minimum charge \$4. Use of Box Number counts as 10 additional words. Payment in advance is required.

COPY for ads must reach **SCIENCE** 2 weeks before date of issue (Friday of every week).

DISPLAY: Positions Open. Rates listed below—no charge for Box Number. Rates net. No agency commission. No cash discount. Minimum ad: 1 inch. Ads over 1 inch will be billed to the nearest quarter inch. Frequency rate will apply to only repeat of same ad. No copy changes. Weekly invoices will be sent on a charge basis—provided that satisfactory credit is established.

Single insertion \$40.00 per inch
4 times in 1 year 38.00 per inch

For **PROOFS** on display ads, copy must reach **SCIENCE** 4 weeks before date of issue (Friday of every week).

Replies to blind ads should be addressed as follows:

Box (give number)
Science
1515 Massachusetts Ave., NW
Washington 5, D.C.

POSITIONS WANTED

Married Couple from Argentina, both M.D.'s, ages 31 and 28, want a medical position with research possibilities on neuropsychiatric diseases. Experience on medical therapy of oligophrenic and in clinical use of psychotogenic drugs (LSD and Psilocibine). Write Dr. J. David, Juez Tedin 3043, Buenos Aires, Argentina. X

Microbiologist, Ph.D., experience teaching, hospital laboratory, research, drug evaluation, tissue culture, medical mycology. Desires teaching, research, and/or product development. Box 197, SCIENCE. X

POSITIONS WANTED

Medical Editor-Writer, extensive pharmaceutical and publishing experience and medical education, seeks similar creative work in East. Box 191, SCIENCE. 10/21

Physician-Physiologist, strong background laboratory, clinical research, teaching, administration. Publications in coronary disease, hypertension, cardiovascular dynamics. Desires challenging opportunity. Box 196, SCIENCE. X

POSITIONS OPEN

Biochemist, Ph.D. Position available for Ph.D. biochemist as Division Chief of Toxicology in commercial clinical and industrial analytical laboratory in southern California. Must have had some experience in analytical methods for routine toxicological laboratory (Pb, As, barbiturates, and so forth). Position involves supervision of technicians for routine tests, some contact work with industry, research in methodology (research technician available), and liaison with other analytical sections of the laboratory. Salary open. Please submit résumé with photo, stating salary requirements. Box 193, SCIENCE. 10/21

PSYCHIATRIC INSTITUTE AND HOSPITAL—Offers challenging and unusually rewarding opportunities to qualified research scientists. Laboratories in various phases of activation include experimental psychology, neuroanatomy and neurohistochemistry, neurophysiology and socio-environmental studies. Positions available involve varying degrees of responsibility in the planning, development, coordination, and direction of research laboratories and programs. Inquiries are invited from individuals with an M.D. or Ph.D. degree and research competence in the following fields: **Human Genetics, Neuropathology, Virology**. Write Dr. Edward N. Hinko, Director, Cleveland Psychiatric Institute and Hospital, 1708 Aiken Avenue, Cleveland 9, Ohio. 10/28; 11/4

POSITIONS OPEN

BIOCHEMIST OR BIOPHYSICIST

Ph.D. Research on the composition, conformation, heterogeneity, and metabolism of nucleic acids. Salary: Commensurate with experience. Send résumé to Dr. Saul Kit, Head, Section of Nucleoprotein Metabolism, The University of Texas, M.D. Anderson Hospital and Tumor Institute, Houston, Texas. 10/21

PHARMACOLOGIST or PHYSIOLOGIST, Ph.D. with several years' experience in the investigation of autonomic drugs. Must have demonstrated ability to do independent research.

BIOCHEMIST, Ph.D. with proven research experience in protein chemistry and enzymology.

Excellent working conditions in a new pharmaceutical plant, fine benefit program with profit sharing. Live near your work in the San Fernando Valley. Write John Permantier, Personnel Manager.

Riker Laboratories, Inc.
Northridge, Calif.

POSITIONS OPEN

CHEMIST

Experienced in drug analyses. Able to apply modern physical methods. Willing to work at bench and assume supervision of others. Long-established independent laboratory, central Philadelphia. State training and experience. Immediate opening, starting date may be as late as 1 November. Replies confidential until after personal interview.

Box 179, SCIENCE

SOIL SCIENTIST with experience and training in plant ecology or plant nutrition. Training and/or experience in soil morphology as relating to edaphic factors.

FIELD BIOLOGIST with experience of training in radiobiology or radiation biology.

Ph.D. required for both positions; minimum of 5 years' experience; full-time environmental and laboratory research in the general area of environmental radioactive contamination as related to above field; interest in and ability to conduct pre- and postgraduate training; ability to organize and direct field observations and studies with up to ten staff members; travel and extended periods in the field may be necessary. Salary: \$7500 to \$10,000, depending on experience. Citizenship required.

Application should be sent to Mr. K. H. Larson, Chief, Environmental Radiation Division, Laboratory of Nuclear Medicine and Radiation Biology, University of California, Los Angeles 24, Calif.

VIRUS RESEARCH

M.D. or Ph.D. interested in infectious diseases, basic studies on mechanisms of infection and on etiology, pathogenesis and epidemiology of virus diseases of infancy and childhood. Excellent facilities. Salary \$6000 per annum. Address

Box 195, SCIENCE

FELLOWSHIPS

The Department of Pharmacology, University of Buffalo School of Medicine, Buffalo 14, N.Y., offers a 4-year program of course work and research training leading to the Ph.D. degree. Research opportunities include the action of drugs on the kidney, the heart and circulation, the autonomic ganglia, and skeletal muscle. Annual stipends of \$1800 to \$2200 plus full tuition, plus \$500 for each dependent. Applications now being considered for entrance February or September 1961. Detailed information supplied on request.

NEW ZEALAND SENIOR RESEARCH FELLOWSHIPS. Applications are invited for Senior Research Fellowships to be taken up in New Zealand in 1961. Applicants should possess a Ph.D. degree, or an equivalent qualification, or while not having such qualification have a distinguished record of scientific research. There is no age limit and no restriction regarding nationality, but successful applicants must meet New Zealand immigration requirements. A good working knowledge of English is required.

The fellowships will be awarded for research at any of the branches of the New Zealand Department of Scientific and Industrial Research. They will be tenable for periods of between 6 months and 1 year initially, but may be extended to a total period of 2 years. The value of each fellowship will range between £400 and £1900 a year, with an additional £250 a year for a married man. These amounts are taxable. (£NZ1 equals approximately \$2.80.) A grant for return fares by surface transport to New Zealand at tourist rates is payable to each fellow, and an allowance of two-thirds of this grant may be paid where a fellow is accompanied by his wife. While in New Zealand reasonable traveling expenses incurred in connection with the fellow's research work will be paid.

Application forms and further particulars are obtainable from:

1) New Zealand Scientific Liaison Office, B.C.S.O., Africa House, Kingsway, London W.C.2, England

2) New Zealand Scientific Liaison Office, P.O. Box 680, Benjamin Franklin Station, Washington, D.C.

3) Department of Scientific and Industrial Research, P.O. Box 8018, Wellington, New Zealand

Applications should reach New Zealand by 1 February 1961.

The Market Place

BOOKS • SERVICES • SUPPLIES • EQUIPMENT

DISPLAY: Insertions must be at least 1 inch in depth. Weekly invoices will be sent on a charge account basis—provided that satisfactory credit is established.

Single insertion	\$40.00 per inch
4 times in 1 year	38.00 per inch
7 times in 1 year	36.00 per inch
13 times in 1 year	34.00 per inch
26 times in 1 year	34.00 per inch
52 times in 1 year	32.00 per inch

For PROOFS on display ads, copy must reach SCIENCE 4 weeks before date of issue (Friday of every week).

PROFESSIONAL SERVICES



LABORATORY SERVICES
for the FOOD, FEED, DRUG and CHEMICAL INDUSTRIES
Analyses, Biological Evaluation, Toxicity Studies, Insecticide Testing and Screening, Flavor Evaluation.
Project Research and Consultation

Write for Price Schedule
P. O. Box 2217 • Madison 1, Wis.

SUPPLIES AND EQUIPMENT


SWISS MICE



Send for booklet

TACONIC FARMS

GERMANTOWN NEW YORK

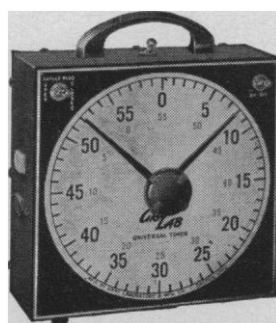

ELECTRIC LAB TIMER
Giant 8" Dial

GRA LAB INTERVAL TIMER Automatic signalling and switching over unusually wide range of 3600 possible settings.
GRA LAB MICRO TIMER 1/10 sec. or 1/1000 min. stop clock. Remote start stop control. Write for catalog.

DIMCO-GRAY COMPANY
214 E. SIXTH ST., DAYTON 2, OHIO

SWISS MICE

BACTERIOLOGICAL AND GROSS TISSUE STUDY TECHNIQUES USED IN OUR QUALITY CONTROL

HUNTINGDON FARMS, INC.
2548 NORTH 27th ST. PHILA. 32, PA.

SUPPLIES AND EQUIPMENT



Mice

CAESAREAN-DERIVED
CHARLES RIVER CD-1
Hypophysectomies
THE CHARLES RIVER MOUSE FARMS
Affiliate, The Charles River Breeding Labs
1018 Beacon St., Brookline 46, Mass. RE 4-2000

YOU NEED THIS FREE CATALOG FOR YOUR FILES

Serums, antisera and bloods of all kinds for technicians and tissue culture laboratories. No salesman will call.

COLORADO SERUM CO.
4950 York St. • MAin 3-5373 • Denver 16, Colo.

ANIMAL CAGES

BUY DIRECT FROM MANUFACTURER
SHIPMENT OF STANDARD ITEMS FROM STOCK
HOELTGE BROS., Inc.
1919 Gast St. Cincinnati 4, Ohio
Write for Illustrated Catalog
SERVICE SINCE 1856


Rats from the Wistar Strain

Laboratory Animals

since 1929
ALBINO FARMS, P.O. BOX 331
RED BANK, NEW JERSEY

Swiss Mice — Albino Rabbits

"From the hand of the veterinarian to research"



Albino rats

CHARLES RIVER CD
(Caesarean derived)
CHARLES RIVER SD
(Sprague-Dawley descendants)
CHARLES RIVER W
(Wistar descendants)

HYPOPHYSECTOMIZED RATS

- Only Charles River CD animals used
- Rigidly controlled environment (same bldg.) birth to surgery.
- High speed surgery by graduate biologists.
- 10 years experience animal surgery.
- Overnight air service from Boston

THE CHARLES RIVER BREEDING LABS
1018 Beacon St., Brookline 46, Mass. RE. 4-2000
Henry L. Foster, D.V.M., President

BOOKS AND MAGAZINES

Your sets and files of scientific journals

are needed by our library and institutional customers. Please send us lists and description of periodical files you are willing to sell at high market prices. Write Dept. A38, CANNER'S, Inc. Boston 20, Massachusetts

SCIENTIFIC JOURNALS WANTED

Sets, Runs and Volumes bought at top prices. Your wants supplied from our Back Files of over 3,000,000 periodicals. Abrahams Magazine Service, N. Y. 3, N. Y.

Your best move is to UNITRON...

for a COMPLETE LINE of METALLURGICAL MICROSCOPES!

INVERTED METALLURGICAL MEC \$399

BINOCULAR METALLOGRAPH BU-11 \$1379

VACUUM HEATING STAGE HHS \$535

TOOLMAKERS MEASURING and METALLURGICAL TM \$1050

STANDARD METALLURGICAL MMU \$287

MONOCULAR METALLOGRAPH U-11 \$1195

INVERTED METALLURGICAL BMEC \$615
with camera attachment

Stage Micrometer \$11

Filar Micrometer \$69.50

ACCESSORIES

Turret Grain Size \$76

Grain Size \$25

Polaroid Land Camera attachment \$115

STUDENT METALLURGICAL MMA \$149

UNITRON'S Complete Line of Metallurgical Microscopes and Accessories covers the needs of Research, Industry and Education.

Quality optics . . . advanced optical and mechanical design . . . unique and convenient operational features . . . budget prices . . . free trial period — these, together with proven performance are the reasons why . . .

THE TREND IS TO UNITRON!

UNITRON

INSTRUMENT COMPANY • MICROSCOPE SALES DIV.
66 NEEDHAM ST., NEWTON HIGHLANDS 61, MASS.

Please rush UNITRON's Microscope Catalog 4-H-3

Name _____

Company _____

Address _____

City _____

State _____

*In the Laboratory . . . where optical quality counts
 . . . the trend is to **UNITRON** Microscopes*

POLARIZING MICROSCOPE
MPS \$269

BINOCULAR PHASE CONTRAST
BMPE \$490

BINOCULAR PHASE-CAMERA-MICROSCOPE
BU-13 \$1580

Polaroid Land Camera Attachment
\$115

BINOCULAR INVERTED
BMIC \$609

BINOCULAR AUTO-ILLUMINATION
BMLU \$425

STUDENT AUTO-ILLUMINATION MICROSCOPE
MSA \$107

Photomicrography Set
ACA \$39.95

Attachable Graduated Stage
GR \$31.50

STEREOSCOPIC MICROSCOPE
MSHL \$267

LABORATORY MICROSCOPE
MLK \$198

MICROSCOPE LAMP
LS \$14.75

FREE 16 DAY TRIAL ON ANY UNITRON

UNITRON offers an extensive line of Laboratory Microscopes & Accessories for Research, Industry and Education. Illustrated is a partial selection for biology, medicine, chemistry and related fields. UNITRON also has companion instruments for the metalworking industries.

Noted for optical quality . . . advanced optical and mechanical design . . . unique and convenient operational features . . . long wearing construction . . . attractive budget prices which include basic optics . . . these, together with years of proven instrument performance, are the reasons why . . .

THE TREND IS TO UNITRON!

UNITRON



INSTRUMENT COMPANY • MICROSCOPE SALES DIV.
 66 NEEDHAM ST., NEWTON HIGHLANDS 61, MASS.

Please rush UNITRON's Microscope Catalog 4-H-3

Name _____
 Company _____
 Address _____
 City _____ State _____

NOW! Snap it... See it...

IN BIG POLAROID LAND 4" x 5" PRINTS

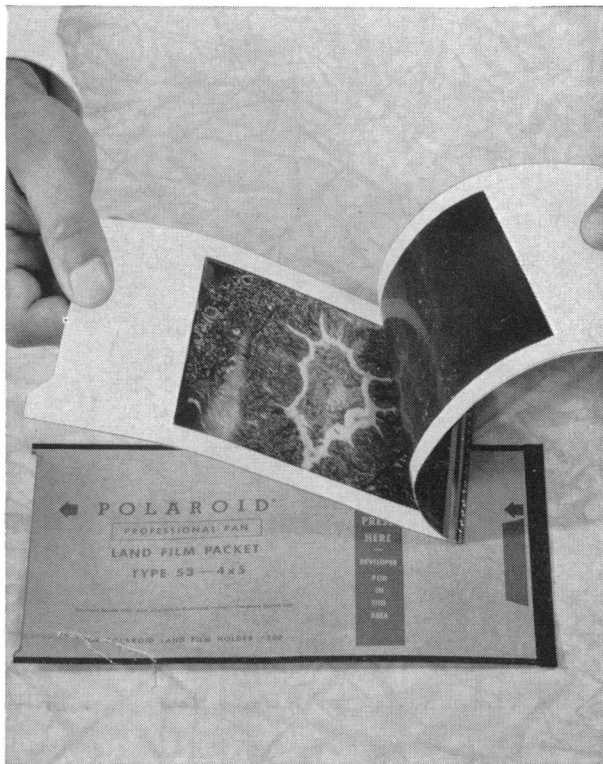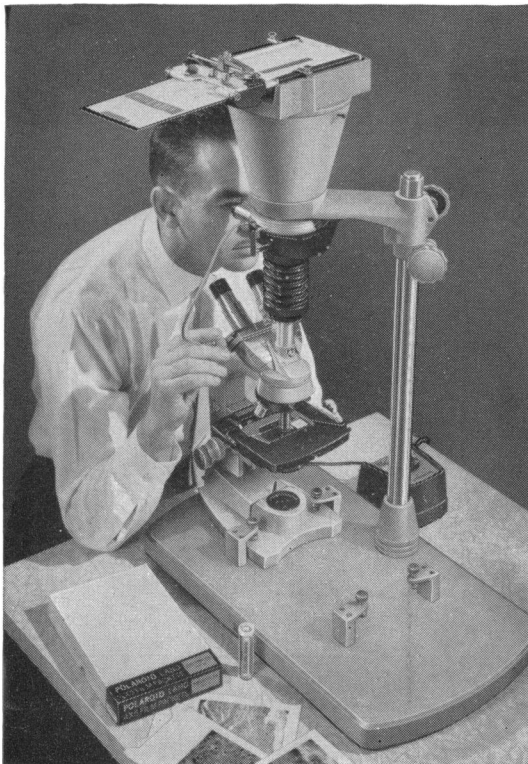

AO Spencer Photomicrographs ... just 60 seconds from snap to finish

Now your AO Photomicrographic Camera can be equipped with the new Polaroid Land Film Holder to give you big 4" x 5" finished, glossy prints... ready for your files... in just 60 seconds. A coupled visual and photographic system allows you to shoot exactly what you see... instantly and effortlessly. Processing of the picture takes place right in Polaroid's 4" x 5" Holder, thus possible errors in exposure, illumination or focus can be rectified immediately.

If you prefer, you have a wide choice of 5 other readily interchangeable camera backs; the Polaroid Land Camera Back for roll film, paper prints and transparencies, 4" x 5" fixed back, 4" x 5" Grafflok back, 35mm back and Bantam (roll film) back. You choose the camera back and film best suited to your specific requirements.

This new "Big-Size" 4" x 5" Polaroid Film Holder is available from your industrial photographic supplier.

Here, the No. 682G Camera being used with the AO Spencer Series 4 Microstar proves an ideal combination. The built-in base illuminator provides convenient Koehler-type illumination. You select specimen area and do all preliminary focusing through binocular portion of trinocular body... focus critically with the telescopic eyepiece.

The sturdy vertical pillar, the easily adjustable camera support, the camera back and the Microstar all combine to provide a compact unit in precise, rigid alignment. Successful photomicrography becomes a "snap".

Try it and see for yourself. Your AO Representative will be happy to arrange a convincing demonstration for you.



American Optical Company

INSTRUMENT DIVISION, BUFFALO 15, NEW YORK

Dept. K-3

- ☐ Please send me Brochure SB682 describing the entire line of AO Spencer Photomicrographic Cameras.
- ☐ Please send me Brochure SB124 describing the new Microstar line.

Name

Address

City Zone State