

go Kubo, Hiroshi Ichimura, Tsunemaru Usui, and Natsuki Hashizume. North-Holland, Amsterdam; Interscience (Wiley), New York, 1965. 437 pp. Illus. \$19.

Statistical Theories of Spectra: Fluctuations. With an introductory review by Charles E. Porter. Academic Press, New York, 1965. 592 pp. Illus. Paper, \$5.95; cloth, \$9.50. A collection of 51 reprints and original papers by S. Blumberg, A. Bohr, L. Dresner, F. J. Dyson, T. Ericson, L. Favro, D. Fox, M. Gaudin, J. Gunson, I. I. Gurevich, P. B. Kahn, T. J. Krieger, L. Landau, A. M. Lane, M. L. Mehta, M. I. Pevsner, C. E. Porter, N. Rosenzweig, Ya. Smorodinsky, R. G. Thomas, R. E. Trees, N. Ullah, E. P. Wigner, L. Wilets, and K. G. Wilson. Perspectives in Physics Series of Reprint Collections.

Textbook of Organic Chemistry. Lloyd N. Ferguson. Van Nostrand, Princeton, N.J., ed. 2, 1965. 767 pp. Illus. \$11.50.

Theory of Energy and Mass Transfer. A. V. Luikov and Yu. A. Mikhailov. Translated from the Russian edition by L. A. Fenn. J. S. Dunn and J. A. Weightman, Translation Eds. Pergamon, London; Macmillan, New York, revised English edition, 1965. 402 pp. Illus. \$12.75.

Theory of Fluid Flow in Undeformable Porous Media. V. I. Aravin and S. N. Numerov. Translated from the Russian edition (Moscow, 1953) by A. Moscona. Israel Program for Scientific Translations, Jerusalem; Davey, New York, 1965. 523 pp. Illus. \$22.25.

Theory of Indirect Speed Control. Miroslav Nechleba. Translated from the Czechoslovak by A. H. Hermann. SNTL Publishers of Technical Literature, Prague; Wiley, New York, 1964. 273 pp. Illus. \$10.

The Theory of Numbers. Neal H. McCoy. Macmillan, New York, 1965. 160 pp. Illus. \$4.95. Allendoerfer Advanced Series.

Topics in Phosphorus Chemistry. vol. 2. William E. McEwen, Ludwig Maier, and Bernard Miller. Interscience (Wiley), New York, 1965. 233 pp. Illus.

Transitional Elements. Edwin M. Larsen. Benjamin, New York, 1965. 195 pp. Illus. Paper, \$2.45; cloth, \$4.95. General Chemistry Monograph Series, edited by Russell Johnsen.

Ultrasonic Engineering. Julian R. Frederick. Wiley, New York, 1965. 393 pp. Illus. \$15.

The Undecidable. Basic papers on undecidable propositions, unsolvable problems, and computable functions. Martin Davis, Ed. Raven Press, Hewlett, N.Y., 1965. 446 pp. Illus. \$7.95. Collection of 17 papers of Kurt Gödel, Alonzo Church, Alan M. Turing, J. B. Rosser, Stephen C. Kleene, and Emil Post.

Universal Algebra. P. M. Cohn. Harper and Row, New York, 1965. 351 pp. Illus. \$9.75. Harper's Series in Modern Mathematics, edited by I. N. Herstein and Gian-Carlo Rota.

University Mathematics. vol. 2. Jack R. Britton, R. Ben Krieger, and Leon W. Rutland. Freeman, San Francisco, 1965. 662 pp. Illus. \$9.50.

Why Do Chemical Reactions Occur? J. Arthur Campbell. Prentice-Hall, Englewood Cliffs, N.J., 1965. 127 pp. Illus. Paper, \$1.50; cloth, \$4.50. Foundations of Modern Chemistry Series, edited by Robert W. Parry and Henry Taube.



- Only 10 inches high
- Temperature control to $\pm 0.1^\circ\text{K}$
- Only 4 pounds
- Operates in any orientation

CRYO-TIP refrigerators are being used for low-temperature experiments in UV, IR, visible and nuclear spectroscopy . . . with all makes of spectrophotometers.

CRYO-TIP operates on economical nitrogen and hydrogen cylinder gas . . . eliminates the need for liquid helium. Simply varying the gas pressure gives precise temperatures from 15°K to 200°K .

Standard CRYO-TIP units produce up to four watts net refrigeration by the open-cycle Joule-Thomson process.

Other CRYO-TIP applications include X-ray diffraction, Hall effect studies, field-ion and electron microscopy, semiconductor measurements, EPR, ESR, NMR, cooling of lasers and low-noise receivers.

Write for full technical information.



Air Products and Chemicals
ADVANCED PRODUCTS DEPARTMENT INC.

Allentown, Pennsylvania

INDEX TO ADVERTISERS—25 June 1965

Air Products and Chemicals Inc.	1787	Houston Omnigraphic Corp.	1778	Perkin-Elmer Corp.	1789
American Edelstaal Inc.	1779	Industrial Instruments Inc.	1772	Pharmacia Fine Chemicals Inc.	1660
Applied Physics Corp.	1639	Instrumentation Associates Inc.	1785	Philips-Duphar	1656
Bausch & Lomb	1760, 1775, 1780, 1783	International Equipment Co.	1650	Philips Electronic Instruments	1777
Beckman Instruments, Inc., Scientific and Process Instruments Div. 1663, 1670		Jarrell-Ash Co.	1638	Phoenix Precision Instrument Co.	1786
Beckman Instruments, Inc., Spinco Div.	1630	JEOLCO (U.S.A.), Inc.	1767	Photovolt Corp.	1776
Blackstone Ultrasonics	1782	Klett Manufacturing Co., Inc.	1780	Picker Nuclear	1637
Blickman, S., Inc.	1781	Lab Cages, Inc.	1765	Professional Tape Co., Inc.	1764
Cambridge Thermionic Corp.	1766	Laboratory Construction Co.	1782	Radiochemical Centre	1785
Clay-Adams, Inc.	1651	Linde Div., Union Carbide Corp.	1666	Reeve Angel	1769
Coleman Instruments Corp.	1654, 1655	LKB Instruments, Inc.	1642	Revco Inc.	1765
Corning Scientific Instruments 1634, 1635, 1644		London Co.	1667	Sargent, E. H., & Co.	1645
Difco Laboratories	1765	Lourdes Instrument Corp.	1662	Schwarz BioResearch, Inc.	1770
Eaton-Dikeman Co.	1761	Maryland Plastics, Inc., Econo-Lab Div.	1786	Scientific Glass Apparatus Co., Inc.	1668
E-C Apparatus Corp.	1641	Mercer Glassworks Inc.	1769	Scientific Industries Inc.	1768
Electronic Associates, Inc.	1653	Midwest Research Institute	1790	Sigma Chemical Co.	1777
E & M Instrument Co., Inc.	1780	Miles Chemical Co.	1782	Sorensen, unit of Raytheon Co.	1657
Esterline Angus Instrument Co., Inc. 1631		Missimers Inc.	1762	Squibb Institute for Medical Research 1790	
Falcon Plastics	1778	Nalge Co., Inc.	1784	Standard Scientific Supply Corp.	1776
Farrand Optical Co., Inc.	1764	National Appliance Co.	1649	Stanford Research Institute	1789
Fisher Scientific Co.	1665	New Brunswick Scientific Co., Inc.	1661	Thomas, Arthur H., Co.	1792
Gilson Medical Electronics	1672	New England Nuclear Corp.	1788	Tracerlab, Div. of Laboratory For Electronics, Inc.	1664
Graphic Controls Corp.	1791	Nikon Inc.	1646	Unitron Instrument Co.	1659
Hacker, William J., & Co., Inc.	1763	Nuclear-Chicago, Div. of Nuclear-Chicago Corp.	1671	Vanguard Instrument Corp., a subsidiary of Technical Measure- ment Corp.	1658
Hamilton Co., Inc.	1772	Nuclear Data, Inc.	1643	Vickers Instruments Inc.	1652
Harford Metal Products, Inc.	1784	Ohio Chemical, Div. of Air Reduction Co., Inc.	1762	Welch Scientific Co.	1762
Harvard Apparatus Co., Inc.	1762	Packard Instrument Co., Inc.	1674	Whittaker Corp., Gencom Div.	1766
Heat Systems Co.	1786	Paillard Inc.	1640	Wilmot Castle Co.	1636
				Worthington Biochemical Corps	1779

NEW LABELED COMPOUNDS

Specific Activity
mc/mM

Antipyrine-N-methyl- C^{14}	1-5
Chloramphenicol- C^{14}	1-5
Chloroquine- C^{14}	1-5
Procaine-carboxyl- C^{14}	1-5
Hydrochloride	1-5
Folic- H^3 Acid (g.l.)	2c/mM


Write for prices and CATALOG 'L'

NEN

LABELED
CHEMICALS

HAncock 6-7311

NEW ENGLAND NUCLEAR CORP.
575 ALBANY STREET, BOSTON 18, MASSACHUSETTS

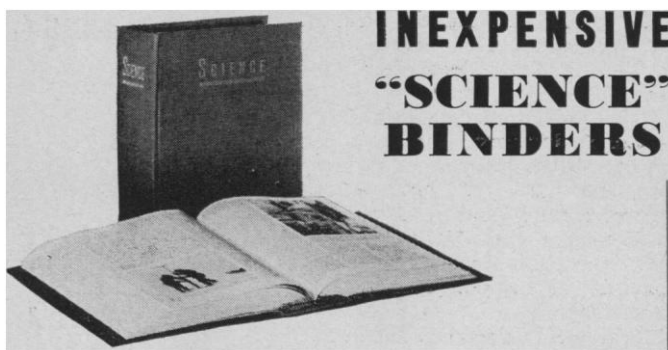

INEXPENSIVE "SCIENCE" BINDERS

Keep your copies of **SCIENCE** always available for quick, easy reference in this attractive, practical binder. Simply snap the magazine in or out in a few seconds—no punching or mutilating. It opens **FLAT**—for easy reference and readability. Sturdily constructed, this maroon buckram binder stamped in gold leaf will make a fine addition to your library.

Starting with January 1962, **SCIENCE** Binders hold one three-month volume of **SCIENCE**. They now have a 3-inch back and 13 flat fasteners. \$3.25 each. Four binders, \$12.00.

For six-month volumes, through December 1961, **SCIENCE** binders with 4-inch back and 26 flat fasteners are available. \$3.25 each.

Add 50¢ for orders outside the U.S. Name of owner, 75¢ extra; year of issues, 50¢ extra.

SCIENCE • 1515 Massachusetts Ave., NW,
Washington, D.C. 20005

Personnel Placement

POSITIONS WANTED

Basic Research, aerospace, research/teaching. Ph.D., physiology, minors: nutrition and biomedical engineering. M.S., nutrition. Box 193, SCIENCE. X

Biochemist Ph.D. Nucleic acid, protein, and cancer research experience. Publications. Wish permanent, independent-research and teaching position. Box 206, SCIENCE. X

Botanist (physiology-pathology) Ph.D., experienced post-harvest, pesticides, nutrition, isotopes. Teaching, research, postdoctoral considered. Box 201, SCIENCE. X

Microbiologist, Ph.D., biochemistry minor. Many years of experience in clinical bacteriology and in medical school. Desire academic position with research opportunity and/or supervision of clinical microbiology. Box 202, SCIENCE. X

(a) **Microbiology Ph.D.,** strong biochemistry background; research on polyglucose complexes; prefers industrial research or academic appointment. (b) **Bacteriology Ph.D.,** biochemistry post-doctorate; dairy manufacturing; M.S.; metabolism research; seeks pharmaceutical or medical research opportunity. Write Woodward Medical Personnel Bureau, 185 North Wabash Avenue, Chicago, Illinois 60601. X

Ph.D. Biochemist/Chemist. Seeks university teaching and research appointment in chemistry, biochemistry, or physiological sciences. Box 205, SCIENCE. X

Ph.D. Biochemistry, physical chemistry, 2 years toward M.D.; research, teaching experience; publications; prefers multidisciplinary situation. (b) **M.S. Anthropology-Botany;** extensive travel, publications, lectures; doctorate preliminary examination passed; interdisciplinary/research project organization, teaching experience; desires teaching, research. (c) **M.A. Zoology** (biochemist minor). 12 hours towards Ph.D. in anatomy; wishes teaching, hospital, or industrial situation. Please write Science Service, The Medical Bureau Inc., 900 North Michigan Avenue, Chicago, Illinois 60611. X

Physician, Scientist, Executive planning early retirement from government; broad and high level experience; prefer part-time, consulting, or short-term work; novel and challenging projects welcomed. Box 184, SCIENCE. X

Physiologist, Ph.D. Fifteen years' teaching in dental school. Publications. Prefers teaching/research in any college located in suburb or small city. Box 203, SCIENCE. X

Zoologist, desires position teaching general zoology. Honors B.A. Cambridge; Marshall Scholar, NSF Fellow, graduate study. Box 204, SCIENCE. X

POSITIONS OPEN

Ph.D.—ELECTRON MICROSCOPIST preferably familiar with viral work, for staff position open September-October in new, completely equipped, hospital research institute, southern Vermont. Salary to \$10,000. New JEM 7. Beautiful surroundings, excellent staff. Near six colleges. Write for details to *Dr. Helene W. Toolan, Director, Putnam Memorial Hospital Institute for Medical Research, Bennington, Vermont.*

Postdoctoral Traineeship, Ph.D. or M.D., in established research program in immunology and biochemistry of skin allergies. For further information write to *Dr. Theodore M. Inderbitzen, Department of Dermatology, Tufts University School of Medicine, 136 Harrison Avenue, Boston, Massachusetts 02111.*

RESEARCH ASSISTANTS

M.S. in biochemistry or chemistry, 2 yrs. experience. Positions in: (1) chemical physics—biochemistry of nucleic acids. (2) Clinical metabolism—development of biochemical procedures, strong interest in instrumentation.

SLOAN-KETTERING INSTITUTE
410 East 68 St. New York 10021, NY
TELEPHONE: TR 9-3000, EXT 2615

POSITIONS OPEN

BIOLOGICAL RESEARCH DIRECTOR

Veterinary Drugs

National Company. Will be responsible for biological R&D activities. Not mandatory but helpful to have Ph.D. in related area with 4 to 6 years' experience as director or assistant director, preferably veterinary drugs. Heavy virology experience and/or knowledge of tissue culture vaccine production an asset. This is a rare opportunity for the properly qualified individual. All replies will be held in utmost confidence.

Box 186, SCIENCE

PHYSIOLOGIST—Ph.D./M.D.

To perform as principal investigator on independent and government research programs associated with our expanding Life Sciences Laboratory. Position requires a minimum of five years experience in physiology of stress primarily in impact and vibration. Experience in aerospace programs desirable.

Please direct resumes to the Space Personnel Office,

NORTHROP SPACE LABORATORIES
3401 W. Broadway, Hawthorne, Calif. 90250
An equal opportunity employer

TECHNICAL WRITER

To research, write, edit, and coordinate production of technical and scientific materials for a graphic arts foundation. Job experience in technical writing or scientific journalism with knowledge of graphic arts preferred. Will consider less experienced candidate displaying good communication facilities and ability to learn a technical field fast. Salary: \$8000 to \$11,000, depending on background and experience. Write

Box 200, SCIENCE



SENSORY PSYCHOLOGIST

IMMEDIATE OPENINGS!

Excellent opportunity for a Ph.D. or M.S. in psychology to work with a small group of engineers, physiologists and other psychologists on basic research problems aimed at developing better models for human information processing. Requires a background in psychophysics, perception, and communication theory and interests in sensory information processing.

The present program is built around a computer-controlled system for presenting high-speed special-temporal patterns for literal data transmission or tracking experiments in taction and/or vision. Eye-movement studies are being initiated to study their effect on visual displays. Comparative auditory tracking experiments are also being initiated.

A primary goal is development of a sensory experimentation program to be conducted in connection with a real-time computer-controlled facility that can handle and present complex spatial-temporal signals in many sensory-motor modes simultaneously.

Interested applicants are invited to submit resumes to:

R. T. Cantu

STANFORD RESEARCH INSTITUTE

333 Ravenswood

Menlo Park, California

— an equal opportunity employer —

Electron Spin Resonance Spectroscopist

An outstanding opportunity with the world's leading manufacturer of analytical instruments. Responsibilities include guidance for product improvement and marketing programs.

The individual we are seeking should be capable of leading applications research and development programs on a new and unique ESR spectrometer.

Perkin-Elmer offers a broad and generous benefit program including cash bonus, paid sick leave, retirement, major medical, and income protection plans.

Submit resume to *Mr. Dale L. Wornstaff, The Perkin-Elmer Corporation, Main Ave., Norwalk, Conn.*
Phone (203) 847-0414. An equal opportunity employer.

PERKIN-ELMER

PHARMACOLOGISTS TOXICOLOGISTS

Senior or Associate Pharmacologist: Ph.D. in pharmacology with research training in pharmacological/toxicological areas for investigations in cardiovascular and renal pharmacology and/or toxicology.

Senior or Associate Pharmacologist: Ph.D. in pharmacology or biochemistry with research training in biochemical pharmacology for investigations in drug metabolism, interactions of chemical agents, and microsomal drug metabolizing enzymes.

Assistant Pharmacologists: M.S. or B.S. degree in pharmacology, physiology, or biochemistry, for investigations in cardiovascular and renal pharmacology and/or toxicology, or biochemical pharmacology.

Senior or Associate Toxicologist: Ph.D. degree or a minimum of five years' experience in toxicology or pharmacology, or DVM with research training in toxicological area for investigations in inhalation, irritation, acute, subacute and chronic toxicology, with emphasis on biochemical techniques in the study of mechanisms of actions and toxicological research.

CONTACT: MARTIN N. SCHULER



**MIDWEST
RESEARCH
INSTITUTE**

425 VOLKER BOULEVARD
KANSAS CITY, MISSOURI 64110

An Equal Opportunity Employer

RESEARCH BIOLOGISTS

Leading pharmaceutical research organization needs pharmacologist or physiologist with doctorate and research experience for responsible position in SCIENCE INFORMATION SECTION.

Also openings for applicants with bachelor's or master's degree and laboratory experience in biomedical sciences.

Same salary scale and staff ratings as laboratory research positions. Excellent company-paid benefits programs.

Ideal location 35 miles from New York City, near Rutgers and Princeton Universities.

For prompt consideration, send complete resume and general salary requirements to

BUSINESS MANAGER

**SQUIBB INSTITUTE
FOR MEDICAL RESEARCH
Division of OLIN**

New Brunswick

New Jersey

An equal opportunity employer

UNIVERSITY OF ALBERTA EDMONTON, CANADA

Applications are invited for the position of Assistant Professor of Microbiology. Duties to include formal lecturing and instruction with emphasis on immunology at both graduate and undergraduate levels. Qualifications: Ph.D. in microbiology with major in immunology or immunochimistry. Appointment as of 1 September 1965.

Minimum starting salary \$8500 per annum. Excellent pension plan, medical services and hospitalization plan, disability and group life insurance.

Well-equipped modern microbiological laboratory. Ample opportunity will be available for research.

Applications including personal data and details of training and experience should be addressed to **Dr. G. E. Myers, Acting Head, Department of Microbiology, Faculty of Science, University of Alberta, Edmonton, Canada.**

BIOLOGIST

with advanced degree (M.S., Ph.D., or D.V.M.) for position in research. Institute offers opportunity for broad investigations into basic toxicology or experimental pathology problems. Background in pharmacology, pathology, biochemistry, or histology desirable. Inquiries together with a curriculum vitae should be addressed to the **Director, Institute of Experimental Pathology and Toxicology, Albany Medical College, Albany, New York 12208.**



CARDIOVASCULAR AND C.N.S. PHARMACOLOGISTS

An expanding program within our St. Paul Central Research Laboratories requires Ph.D. pharmacologists with training and/or experience in the cardiovascular and C.N.S. areas. This is an opportunity to participate in the formation and growth of a new research group. Salary will be commensurate with experience.

For confidential consideration, send personal and work history to:

**Jerry A. Buegler
Employment Department
MINNESOTA MINING AND
MANUFACTURING COMPANY
2501 Hudson Road
St. Paul 19, Minnesota
An Equal Opportunity Employer**

GRADUATE FELLOWSHIPS IN BIOCHEMISTRY

A limited number of positions leading to Ph.D. still available for academic year 1965-66. Varied department research programs include mammalian and microbial metabolism, enzymology and nucleic acid biochemistry. Annual stipend starts at \$2400 plus dependency allowance and tuition. Address further inquiries to **Head, Department of Biochemistry, University of Maryland, School of Medicine, Baltimore, Maryland 21201.** 7/2

NEW ZEALAND SENIOR RESEARCH FELLOWSHIPS

Applications are invited for Senior Research Fellowships to be taken up in New Zealand in 1966. Applicants should possess a Ph.D. degree, or an equivalent qualification, or whilst not having such qualification have a distinguished record of scientific research. The fellowships are intended for research workers who have had several years of professional experience and have published original material. There is no age limit and no restriction regarding nationality, but successful applicants must meet New Zealand immigration requirements. A good working knowledge of English is required.

The fellowships will be awarded for research at any of the branches of the New Zealand Department of Scientific and Industrial Research. They will be tenable for periods of between 6 months and 1 year initially, but may be extended to a total period of 2 years. The value of each fellowship will range between £1605 and £2230 a year, with an additional £250 a year for a married man. These amounts are taxable. (NZ £1 approximately equals \$2.80 or £1 sterling.) A grant for return fares by surface transport to New Zealand at tourist class rates is payable to each Fellow, and an allowance of two-thirds of this grant may be paid where a Fellow is accompanied by his wife. While in New Zealand reasonable traveling expenses incurred in connection with the Fellow's research work will be paid. Application forms and further particulars are obtainable from:

The New Zealand Scientific Liaison Office, C.S.C., Africa House, Kingsway, London, W.C.2, England;

The New Zealand Embassy, 19 Observatory Circle, Washington, D.C., U.S.A., 20008;

The Office of the High Commissioner for New Zealand, Suite 804, Commonwealth Buildings, 77 Metcalfe Street, Ottawa, Ontario, Canada;

The Department of Scientific and Industrial Research, P.O. Box 8018, Wellington, New Zealand. Applications should reach New Zealand by 30 September 1965.

The Market Place

BOOKS • SERVICES • SUPPLIES • EQUIPMENT

SUPPLIES AND EQUIPMENT

GEL ELECTROPHORESIS SEPARATIONS

including densitometry, and/or reconstituted fraction recovery by elution convection.

CURRENT INC.

Research Laboratories
220 S. 40th St., Phila. 4, Pa.
Phone—215-EV-2-2205

STAINS • REAGENTS • PREPARED MICROSCOPIC SLIDES

Authorized American Agents for
GURR'S STAINS AND REAGENTS
(G. T. GURR, LTD.)
World Famous since 1915
Stains • Mountants • Immersion Oils • Buffers
—We shall be pleased to send full details—
JAYMAR SCIENTIFIC CO.
BOX 25, KENILWORTH, N.J. 07033

HAMSTERS

Dated Pregnancies
Weanlings

WHITNEY ANIMAL LABORATORIES
R.D. #3

Horseheads, New York 14845

IDENTIFY

dogs, cats, guinea pigs
with the animal care

Ident-A-Band®



Soft, slim, waterproof.
Color-coded inserts for
classification ease
in research.

HOLLISTER 835 N. Orleans, Chicago, Ill. 60610


SPRAGUE-DAWLEY, INC.

Pioneers in the development of the
STANDARD LABORATORY RAT.

P.O. Box 4220

Madison, Wisconsin

CE 3-5318

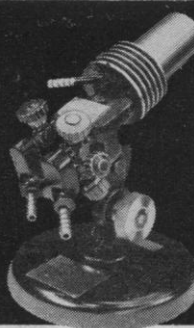

BETHLEHEM BENCH BURNER

- Surface-Mixed
- Water-Cooled
- Heavy-Duty


Offers unprecedented temperature ranges . . . two concentric fires, operating independently or as one . . . central fire can be varied from sharp needle point to long powerful jet . . . completely silent . . . no chance of flashback.

Write
for
Catalog
No. 61



BETHLEHEM

Apparatus Company, Inc.
Hellertown, Pa.

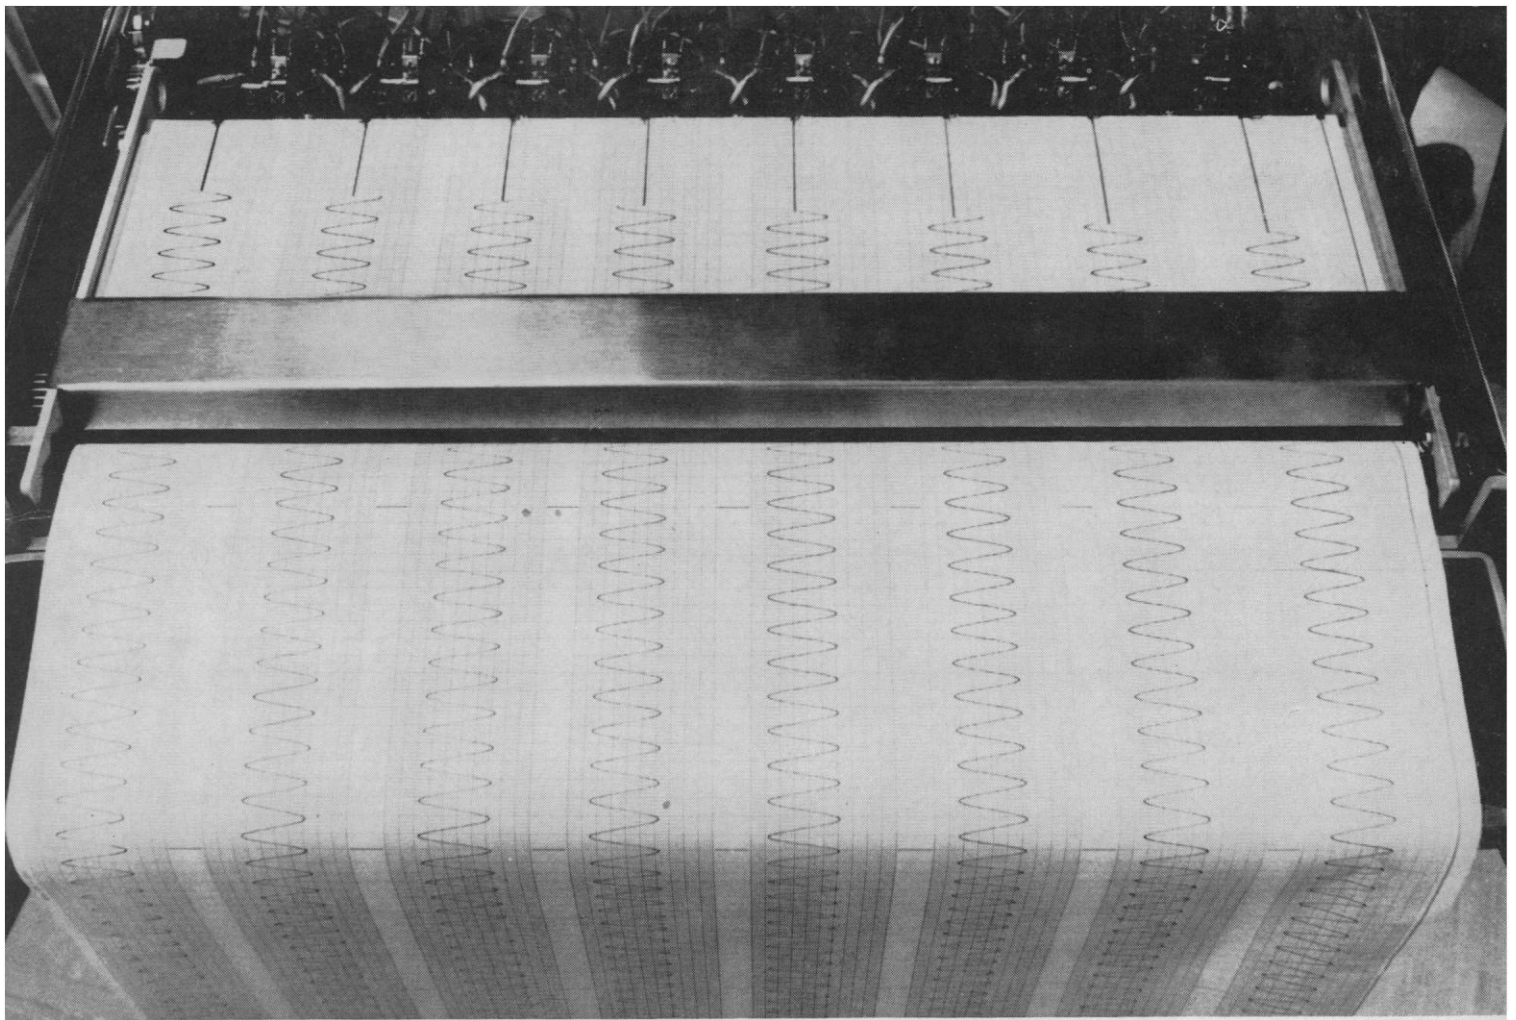


A few lines worth repeating...

Graphic Controls' thermal recording oscillograph charts produce distinct, black, clearly legible trace lines everytime.


The reason is the unique construction of our paper. We start with a specially processed, high-density undercoating that provides the blackest possible trace. To this we add an unusually sensitive, completely compatible surface coating that lets the stylus glide evenly and smoothly. Many critical areas that are blurred or indistinct on other papers become clear and precise with GC's oscillograph charts. Even the most complex functions and inputs are recorded easily.

Because the surface coating is applied by a new process, there's no variance in thickness from edge-to-edge. The caliper of the paper is constant. Creep is eliminated and uniform paper flow is assured. And at the same cost as the paper you are now using.

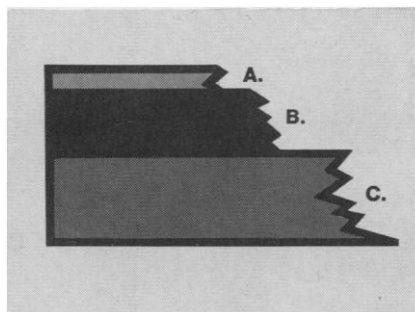

A. Thermal-reactant coating
B. Contrast undercoat
C. Substrate

In addition, GC's thermal recording charts are water resistant, durable, yet extremely lightweight. Their con-

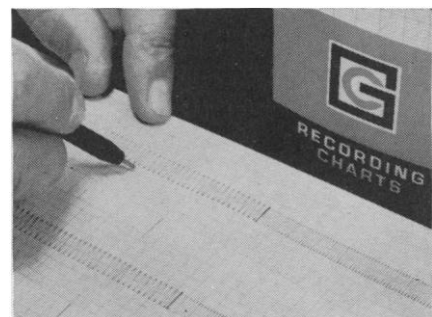

sistent performance has been proved in major aerospace, industrial, and scientific research applications.

Check the performance of GC's charts for yourself...and compare them with your present papers. For complete information, contact:



RECORDING CHART DIVISION
GRAPHIC CONTROLS CORPORATION
189 VAN RENSSELAER STREET, BUFFALO, NEW YORK 14210

New Corning Model 10

Expanded Scale pH METER



4875-C08.

- ◆ With 10-inch scale
—widest available—
for enhanced readability
- ◆ 3 pH expansion
readable to 0.01 pH
- ◆ Simple operation
combined with
high stability

A new, stabilized, line-operated, expanded scale pH Meter with a 10-inch scale—largest scale now available—for enhanced readability.

Can be switched instantly from normal range of pH 0 to 14 (or 0 to ± 1400 millivolts) to full-scale span of any 3-pH segment (or ± 300 mv unit) and easily read to 0.01 pH or 1 mv.

Suitable for critical measurements as well as for general purpose work in acidimetric or oxidation-reduction techniques and, by use of plug-in jumper, for Karl Fischer or other polarized electrode titrations.

Stability. Precision components throughout circuit; transistorized amplifier employs solid-state chopper for drift-free operation. Unaffected by line variations from 105 to 125 volts.

Large Scale Meter. Scale 10 inches long, with lower scale graduated 0 to 14 in 280 divisions, and two upper scales, 0 to 300 and 5.5 to 8.5, in 300 divisions. The range 5.5 to 8.5 is most frequently used but any 3-pH span can be read on this scale. Mirror band eliminates parallax error and provides excellent readability. Taut-band suspension of the meter movement is less susceptible to friction, and therefore more accurate, than conventional jewel-and-pivot movements.

Control Switches. Conveniently grouped on sloping front panel. Lower or function switch, pushed in, selects pH, +mv or -mv readout; pulled out, it switches to expanded scale. Standby position of same switch disconnects the electrodes from measuring circuit. Calibration control permits buffer standardization.

Temperature Compensation. Manual control for pH readings is calibrated in 2° divisions over range 0 to 100°C . Automatic Temperature Compensator, required for continuous recording, is applicable to both pH 0-14 and expanded ranges and covers 0 to 100°C .

Polarizing Current. Ten microamperes, for endpoint determinations in Karl Fischer and similar procedures.

Grounding. Operates with grounded or ungrounded solutions; an earth ground outlet is provided.

Recorder Output. Ten millivolts.

Housing. Heavy gauge aluminum, corrosion-resistant epoxy finish; 15 inches wide \times $6\frac{1}{2}$ deep \times 9 high. Terminal board in rear provides for connection of electrodes, polarizing jumper, recorder leads and automatic temperature compensator probe.

Adjustable Meter Angle. For convenient reading from a standing position, meter is provided with extension feet and a special wedge to support the meter at an angle with the electrode support rod remaining vertical to the bench.

Electrodes. Size 5 inches long \times $\frac{1}{2}$ -inch diameter, with 30-inch leads. Glass electrode range pH 0 to 14, for use from -5° to 100°C . Calomel reference electrode is of fiber junction type.

SPECIFICATIONS	pH		MV	
	Normal 0-14	Expanded any 3 pH	Normal 0 to ± 1400	Expanded 0 to ± 300
Readout				
Smallest scale division	0.05 pH	0.01 pH	5 mv	1 mv
Repeatability	± 0.02 pH	± 0.005 pH	± 2.0 mv	± 0.5 mv
Relative accuracy	± 0.05 pH	± 0.01 pH	—	—
Accuracy	—	—	± 14 mv	± 3 mv

4875-C08. Corning pH Meter, Expanded Scale Model 10, as described, with one each Glass and Calomel Electrodes, Polarizing Jumper, electrode holder and support rod, two extension feet, wedge adapter for use of Meter at an angle, 4 oz. KCl solution, 16 oz. pH 7.00 buffer solution, dust cover and 50 ml graduated beaker. With 3-wire cord, 3-prong plug and adapter; for 115 volts, 60 cycles, a.c., 6 watts. Without automatic temperature compensator..... **485.00**

4875-H55. Automatic Temperature Compensator, range 0 to 100°C ; size 5 inches long \times $\frac{1}{2}$ -inch diameter, with 30-inch lead **29.00**

Detailed descriptive bulletin sent upon request.



ARTHUR H. THOMAS COMPANY

Scientific Apparatus and Reagents

VINE STREET AT 3RD • P. O. BOX 779 • PHILADELPHIA 5, PA., U. S. A.