

Principles and Applications of Water Chemistry. Proceedings of the Fourth Rudolfs Research Conference (New Brunswick, N.J.). Samuel D. Faust and Joseph V. Hunter, Eds. Wiley, New York, 1967. 659 pp. Illus. \$12.50. Twenty-three papers.

Progress in High Temperature Physics and Chemistry. vol. 1. Carl A. Rouse, Ed. Pergamon, New York, 1967. 248 pp. Illus. \$11.50

Prothrombin in Enzymology, Thrombosis and Hemophilia. Walter H. Seegers. Thomas, Springfield, Ill., 1967. 199 pp. Illus. \$9.75.

Psychoanalytic Techniques. A handbook for the practicing psychoanalyst. Benjamin B. Wolman, Ed. Basic Books, New York, 1967. 606 pp. \$15. Twenty papers.

Psychology and Life. Floyd L. Ruch. Scott, Foresman, Glenview, Ill., brief ed. 7, 1967. 616 pp. Illus. Paper, \$5.50; cloth, \$6.50.

Race and Racism: A Comparative Perspective. Pierre L. van den Berghe. Wiley, New York, 1967. 181 pp. Illus. \$4.95.

Radiology as an Art and Other Essays. John L. McClenahan. Thomas, Springfield, Ill., 1967. 101 pp. Illus. \$5.75.

Reaction Index of Organic Syntheses. Shigehiko Sugawara and Seiji Nakai. Hirokawa, Tokyo; Wiley, New York, 1967. 257 pp. Illus. \$8.75.

Reagents for Organic Synthesis. Louis F. Fieser and Mary Fieser. Wiley, New York, 1967. 1469 pp. Illus. \$27.50.

The Rise and Development of Western Civilization. vol. 2. John L. Stipp, Allen W. Dirrim, and C. Warren Hollister. Wiley, New York, 1967. 738 pp. Illus. \$8.95.

Erwin Schrödinger: An Introduction to His Writings. William T. Scott. Univ. of Massachusetts Press, Amherst, 1967. 191 pp. \$6.50.

Science in Utopia: A Mighty Design. Nell Eurich. Harvard Univ. Press, Cambridge, Mass., 1967. 344 pp. \$7.95.

The Search for Understanding. Caryl P. Haskins, Ed. Carnegie Institution, Washington, D.C., 1967. 354 pp. Illus. \$6. Twenty-two selected writings of scientists of the Institution, published on the 65th anniversary of the Institution's founding.

Set Theory for the Mathematician. Jean E. Rubin. Holden-Day, San Francisco, 1967. 399 pp. Illus. \$10.75.

Sharks, Skates, and Rays. A symposium (Bimini, Bahamas), January-February 1966. Perry W. Gilbert, Robert F. Mathewson, and David P. Rall, Eds. Johns Hopkins Press, Baltimore, 1967. 640 pp. Illus. \$15. Thirty-nine papers.


A Short Course of Physical Chemistry. E. A. Moelwyn-Hughes. Elsevier, New York, 1967. 569 pp. Illus. \$8.50.

Soil Biochemistry. A. Douglas McLaren and George H. Peterson, Eds. Dekker, New York, 1967. 523 pp. Illus. \$22.75. Seventeen papers.

Thin-Layer Chromatography. Justus G. Kirchner. Interscience (Wiley), New York, 1967. 810 pp. Illus. \$21.95. Technique of Organic Chemistry Series, vol. 12.

Toward a Manpower Policy. Robert Aaron Gordon. Wiley, New York, 1967. 384 pp. Illus. \$8.95.

25 AUGUST 1967

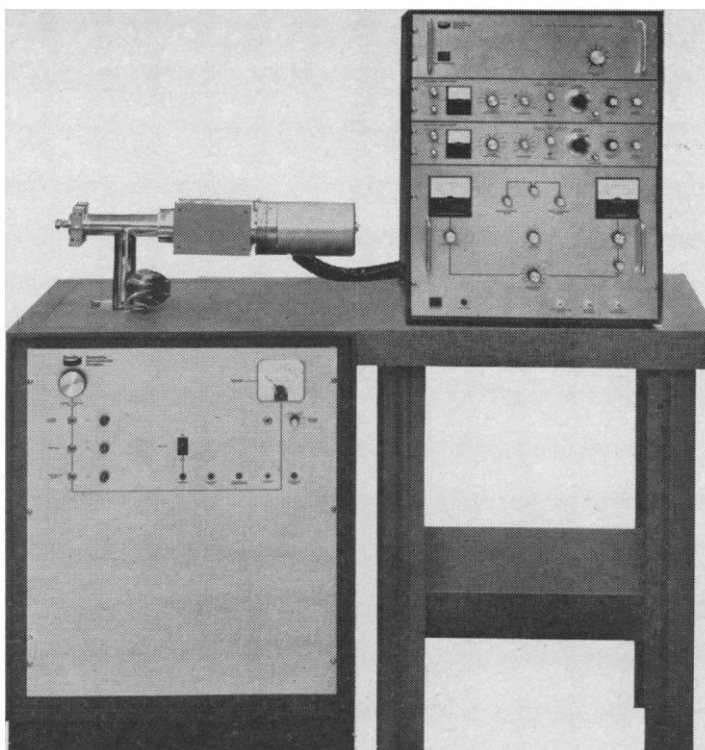

**Low-cost mass spectrometers
are nothing new.**

But this one is.



It's unique. It's the completely new Bendix® MA-1. It gives you both fast scan *and* high sensitivity. (How's that possible? It uses the new, exclusive, bakeable magnetic electron multiplier.) Yours, too: Simultaneous scope and recorder readout.

MA-1 is a complete system. Its 1-to-500 amu operating range permits application in both organic and inorganic research. This means that for \$10,500, you get a Time of Flight Mass Spectrometer that makes other low-cost models seem incomplete. With a 50,000 spectra-per-second oscilloscope scan rate. 1.5 seconds to 60 minutes recorder scan time for 2 to 200 amu. Resolution greater than 200. Mercury diffusion pump that gives operating pressure below 10^{-5} torr and, with addition of liquid nitrogen trap, to 10^{-8} torr. Stability of $\pm 1\%$ per hour on a permanent gas peak. Analyzer assembly bakeable to 300°C .

You'll find MA-1 particularly useful for examining short duration samples. Gas chromatograph effluents, for example. Its basic inlet system is suitable for direct sampling of volatile liquids and gases, and for direct coupling to gas chromatographs. Electronics? Table-top, integrated, solid state circuits for trouble-free performance and easy maintenance. For complete information write: The Bendix Corporation, Scientific Instruments Division, 3625 Hauck Road, Cincinnati, Ohio 45241. Or phone (513) 772-1600.



**What
you want
in a rotating
flash
evaporator**

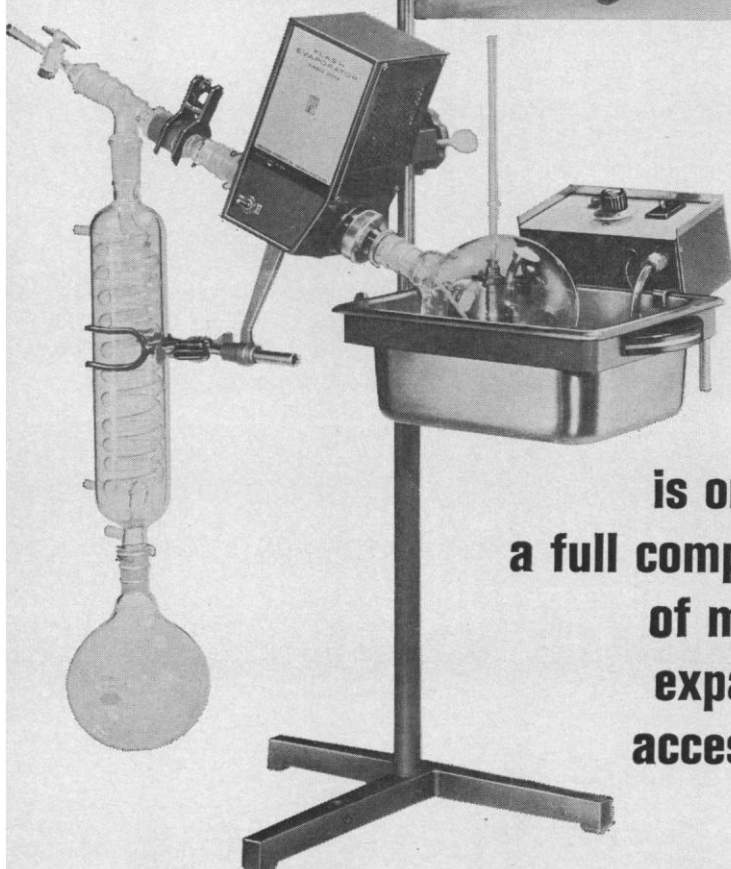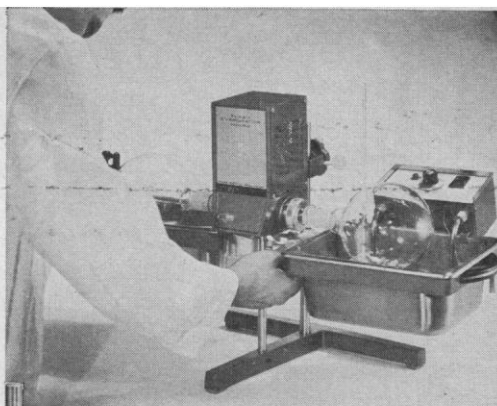

**is one with
a full complement
of modular,
expandable
accessories!**

Get it in a flash from Precision!

Yes, that's exactly what you get with Precision's all new and highly versatile line of rotating thin-film evaporators! And, perhaps more important, high speed evaporation of solutions, even those with high boiling points or those containing heat-sensitive solutes.

Starting with the basic unit, simply add a 1,000 or 2,000 ml evaporating flask (standard 24/40 joint)—then pick your preferred condensing means—a spiral condenser, a Dewar Condenser, or a flask. And there's a controlled heating bath for the evaporating flask.

There is a fixed speed model operating at 120 rpm and a variable speed model, with a

solid state SCR speed controller, which maintains high torque across its entire 30 to 250 rpm range. All-glass-and-Teflon® evaporating system assures you of contamination-free performance. No chance of contamination in the flask, either, as no O-Rings are used in the sealed system.

Select only the module needed for your current application, with full assurance that the conveniently added accessories will be immediately available as your requirements change. Complete information is in our Bulletin 653, ask your Precision Scientific Dealer or write us.

Since 1920 • The finest in Quality Laboratory Apparatus



3737 W. Cortland Street, Chicago, Illinois 60647
Local Offices in New York • Chicago • Los Angeles

Index of Advertisers

25 August 1967

Aldrich Chemical Co.	972
American Optical Co.	984
Bausch & Lomb	967
Beckman Instruments, Inc.	850, 855
Bendix Corp., Scientific Instruments Div.	979
Blickman, S., Inc.	863
Buchler Instruments, Inc.	969
Cary Instruments	857
Digital Equipment Corp.	865
Durst (USA) Inc., Photo Technical Div.	871
Electro Scientific Industries Inc. ...	870
Farrand Optical Co., Inc.	973
Fisher Scientific Co.	858
Gilford Instrument Laboratories, Inc.	983
Hacker, William J., & Co., Inc.	968
Hewlett-Packard, Loveland Div.	861
Hewlett-Packard Co., Sanborn Div. ...	880
IIT Research Institute	981
Instrumentation Associates, Inc.	969
International Equipment Co.	860
Klett Manufacturing Co., Inc.	976
Lab Cages Inc.	869
Labindustries	876
Lea & Febiger	968
London Co.	862
Mann Research Laboratories	978
Manor Research	964
Maryland Plastics, Inc.	877
Matheson Scientific	978
Mech-Tronics Nuclear Corp.	876
Mettler Instrument Corp.	969
MSE Inc.	866
Nalgene Labware Div.	873
N.J.E. Corp.	970
Ohaus Scale Corp.	981
Olin Mathieson Chemical Corp.	854
Olympus Corporation of America ...	859
Orion Research, Inc.	875
Percival Refrigeration & Mfg. Co. ...	970
Philbrick Researches, Inc.	878
Phipps & Bird, Inc.	975
Precision Scientific Co.	980
Princeton Applied Research Corp. ...	872
Professional Tape Co., Inc.	973
Saunders, W. B., Co.	851
Scientific Glass Apparatus Co., Inc.	977
Scientific Products, Div. of American Hospital Supply Corp.	856
Shandon Scientific Co., Inc.	974
Siemens America Inc.	971
Sigmamotor, Inc.	976
Sobotka, Eric, Co., Inc.	972
Tracerlab	975
TRW Instruments	864

Personnel Placement

POSITIONS WANTED

Anatomist Ph.D., seeking academic position to teach gross anatomy and neuroanatomy; member of American Association of Anatomists; postdoctoral research training. Write for curriculum vitae to Box 522, SCIENCE. 9/1.

Environmental Engineer, Ph.D. October 1967, radiological health, water pollution, analytical chemistry, mass spectrometry. Desires challenging position in research or administration. Kenneth Murphy, 2174 5th Ave., Troy, N.Y. 12180. X

(a) **IMMUNOCHEMISTRY Ph.D.**; microbiology minor; cancer, schizophrenic research; desires research opportunity. (b) **DVM: Public Health M.S.** completing postdoctoral anaplasma infection studies; seeks research position. **WOODWARD PERSONNEL BUREAU**, 185 North Wabash, Chicago 60601.

POSITIONS OPEN

—Ph.D.— BACTERIOLOGIST/ IMMUNOLOGIST

Seeking a Ph.D. with training or 3-5 years' research experience in areas such as immunology, immunochemistry, bacterial chemotherapy, and pathogenic bacteriology. Duties will involve conducting a research program and supervising a bacteriology unit investigating various infectious disease processes in animals. Of particular value is a broad understanding of biochemistry and intermediary metabolism. Please send resume to: **Cyrus M. Greenberg, Ph.D., Director of Scientific Employment.**

**SMITH KLINE &
FRENCH LABORATORIES**



1552 Spring Garden Street
Philadelphia, Pa. 19101

An Equal Opportunity Employer

(a) **CONSULTING BIOCHEMIST Ph.D.** or Ph.D.-M.D.; good clinical exp or retired univ prof; \$15-20,000; private lab serving many hosps; Calif. (b) **ASST PROF BIOPHYSICS** grad teach & research; large state univ; \$20,000; SE. (c) **ASST PROF BOTANY** teach and research; new science bldg, expd grad state univ; \$10,000 up; MidW. (d) **AGRICULTURAL BIOCHEMIST** food growth & production research; univ agric station; \$14,000; NW. (e) **LAB MGR Ph.D.** or unlicensed MD; clinical exo supv 25; \$15,000 up; 300-bed hosp; E. (f) **BACTERIOLOGIST** fermentation research; \$12,000 up; mfg firm; MidW. Write **WOODWARD PERS BUREAU**, 185 N. Wabash, Chicago 60601. X

Research Administrator:

With or without experience in administration. Research and advanced course work in Biomedical Sciences desirable. Located in pleasant academic environment. Please send resume including salary history to **The Ohio State University Research Foundation**, 1314 Kinnear Road, Columbus, Ohio 43212.

Technical Abstractor-Indexer—World-wide abstracting-indexing publication and affiliated information center. Degree in chemistry, biochemistry of chemical engineering, foreign language preferred. Ideal for ambitious recent graduate interested in documentation career. Research-academic environment in ideal college town.

Write **Dr. McLeod**
The Institute of Paper Chemistry
Box 1048
Appleton, Wisconsin 54911

25 AUGUST 1967

MICROBIOLOGISTS

Advanced research studies on host-parasite relationships involving viruses and mycoplasma have created excellent opportunities for microbiologists with BS or MS degrees and some experience in virology and/or tissue culture methodology.

As part of our unique, pan-technological team, you'll be working in an atmosphere of interdisciplinary research projects that span industry's and government's most pressing needs.

IITRI is located in Chicago on the campus of the Illinois Institute of Technology. This provides an ideal academic atmosphere and convenient access to graduate studies. Send resumes in confidence to **Mr. J. E. Katzenberger, Personnel Supervisor.**

IITRI IIT
Research
Institute

10 West 35th Street
Chicago, Illinois 60616

An Equal Opportunity Employer (M/F)

SEEING DOUBLE?



We just want you to know you can own two of these attractively redesigned OHAUS AUTOGRAM balances for the price you might pay for an equivalent optical projection balance now being offered for laboratory use.

MODEL 1000

\$ 325.00

(each ... of course)

Why over-buy when this AUTOGRAM 1000 gives you direct optically projected readings and convenient external top loading to 1000 grams.

Permanently adjusted magnetic damping adds speed to your weighing.

Built-in 200 gram tare capacity, complete portability, reversible weight rack for comparison weighings, insensitivity to out-of-level conditions, and a variety of weighing platforms put this precision weighing instrument in a class twice its price!

Want more information? ... thinking twice about rising R&D costs? ... then write:

OHAUS SCALE CORPORATION

1050 COMMERCE AVENUE • UNION, N. J. 07083

dept. HE



129

981

Senior Microbiologist

A position with good growth potential is open in the area of fermentation development for a microbiologist (Ph.D. or equivalent) with supervisory experience. Responsibilities include supervision of mutation induction studies, culture evaluation, fermentation improvement studies, radiochemical and chromatographic procedures.

Please send complete resume of training and experience including salary expectations to:

Professional Employment

Bristol Laboratories

Division of Bristol-Myers Company
Syracuse, New York 13201

An equal opportunity employer

Medical Physiologist. Teaching and research position available for Fall term in medically oriented college. Excellent opportunity and brilliant future for the right man. Ph.D. required. Salary commensurate with background and experience. Send resume to: **Director of Basic Sciences, Pennsylvania College of Podiatry, 8th and Pine Sts., Philadelphia, Pa.**

Basic Science Instructor to teach the laboratory courses in Biochemistry, Physiology, and Microbiology in a medically oriented college. Requires B.S. or M.S. in Biological Sciences. Further educational and research opportunities available. Salary open. Send resume to: **Director of Basic Sciences, Pennsylvania College of Podiatry, 8th and Pine Sts., Philadelphia, Pa.**

Research Assistant with B.S., M.S., or recent Ph.D. in Biochemistry for purification and characterization of microbial enzymes and isozymes. Salary commensurate with background and experience. Send resume to: **Dr. Carl Abramson, Pennsylvania State University, Ogontz Campus, Abington, Pa.**

NATIONAL CENTER FOR AIR POLLUTION CONTROL

With the recent reorganization of the National Center for Air Pollution Control, there is a new emphasis on the development of air quality criteria and vehicle emission standards. That's why we urgently need top professional staff members to work in the area of **RESOURCE INFORMATION DEVELOPMENT AS THE BASIS FOR FEDERAL EMISSION STANDARDS APPLICABLE TO MOTOR VEHICLES.**

Suitable educational backgrounds would include mechanical engineering, chemical engineering, engineering physics, and the mathematical and physical sciences. Assignments involve:

- (1) the preparation of analyses of the desirability, feasibility, economic costs, changes in activity patterns, technological changes and time factors involved in achieving various degrees of control of emission of pollutants from motor vehicles.
- (2) the evaluation of methods and procedures for measuring emission of pollutants from motor vehicles and the preparation of requirements for determining compliance with established emission standards.

These are career Federal Civil Service positions. The salaries, educational assistance, and other benefits are fully competitive with those of private industry. You'll have unprecedented opportunities for individual contribution and development. Publication of research results is encouraged, along with participation in the activities of technical societies and committees.

Interested? Forward resume in complete confidence to:

Mr. J. C. Romanovsky
Vehicle Emission Standards Activity
Criteria and Standards Development Branch
National Center for Air Pollution Control
550 Main Street, Rm. 5008
Cincinnati, Ohio 45202

An Equal Opportunity Employer

DEMONSTRATOR

Individual with interest in and experience with instruments such as scintillation counters, spectrophotometers, ultracentrifuges and amino acid analyzers to take responsibility for the instruments, instruct students in their use, operate them for others. Send resume to **Dr. A. E. Schaefer, Department of Chemistry, State University of New York at Albany, Albany, New York 12203.**

BIOMETRICIAN

Individual with background in biological science and Ph.D. to provide biometrical and biostatistical competence in a multi-disciplinary research program on the behavior and effects of inhaled radionuclides. The opportunity exists for both collaborative and independent research. Burroughs 5500 Computer and programming services available. **The Lovelace Foundation For Medical Education and Research, Attn: Personnel, 5200 Gibson Blvd., S.E., Albuquerque, New Mexico 87108.**

An Equal Opportunity Employer

IMMUNOLOGIST-BIOCHEMIST:—For research with antigens and antibodies.—Conduct studies on virus propagation, purification and characterization, and develop immunological methods for studying (exotic) diseases of domestic animals.—Entrance salary \$11,306 to \$14,717 depending on qualifications. Full U.S. Civil Service coverage. No written test required. Excellent research facilities at this unusual but attractive location off the northeastern tip of Long Island. Send resume to **Plum Island Animal Disease Laboratory, Box 848, Greenport, N.Y. 11944.** (An equal opportunity employer)

IMMUNOCHEMIST —PhD

New research position for PhD in immunology or immunochemistry with general experience in biochemistry and microbiology.

This position involves research into mechanisms of immune induction, with special interest in the cellular and information transfer processes.

Ortho is located in an attractive suburban area of New Jersey near Princeton. If interested please write including your salary requirements to
Mr. Richard Groban

ORTHO

PHARMACEUTICAL CORPORATION
RT 202 RARITAN, NJ 08869

An Equal Opportunity Employer

PHARMACOLOGIST

Challenging Senior Research position with leading pharmaceutical firm located in Suburban Philadelphia.

Ph.D. with keen interest in cardiovascular pharmacology or physiology is desired.

Consideration will be given to recent graduates and candidates with industrial or academic experience. Write giving educational background and experience, indicating salary requirements, to:

Personnel Department

WYETH

P.O. BOX 8299
Philadelphia, Pa. 19101

An Equal Opportunity Employer

A graduate physicist (or physical chemist) needed for a continuing long-term study of the lower atmosphere and of air-sea exchange processes. Salary \$11,000 to \$13,000. Send curriculum vitae to: **A. H. Woodcock, Hawaii Institute of Geophysics, University of Hawaii, Honolulu, Hawaii 96822.**

The Market Place

BOOKS • SERVICES • SUPPLIES • EQUIPMENT

BOOKS AND MAGAZINES

N.Y. PUBLISHER WANTS MANUSCRIPTS

\$1600 BEST BOOK CONTEST

Want your book beautifully published, promoted, distributed by a New York leader in the field? Over 1,000 authors on our list. Attractive subsidy basis for fiction, non-fiction, poetry, scholarly, scientific or controversial books. Send manuscript for free editorial report, free Brochure SX and rules of \$1600 Best Book Contest open to Pageant authors.

PAGEANT PRESS

101 Fifth Ave., N.Y., N.Y. 10003

PROFESSIONAL SERVICES

HISTOLOGY SERVICE

RAPID SERVICE Large Orders Quickly Processed! Quickly Shipped! Professional supervision of every order. Free estimates on special problems. Distant points serviced swiftly. Special stains and techniques available. Full protected shipments. **HISTOLOGY SERVICE, INC.** 4801 N. Broad St., Philadelphia, Pa. Zipcode 19141. (215) DAvenport 4-5800.

CUSTOM ANTISERUMS

Prepared to Your Antigen

Standard Antiserums in Stock

NORMAN CAPPEL LABORATORY

Box 156, Downingtown, Pa. 19335

215-269-0275

SUPPLIES AND EQUIPMENT


● HYPOPHYSECTOMIZED RATS

Shipped to all points via Air Express

For further information write

HORMONE ASSAY LABORATORIES, INC.
8159 South Spaulding Ave., Chicago 29, Ill.

Four Enzyme Assays with Temperature Measurements made Simultaneously

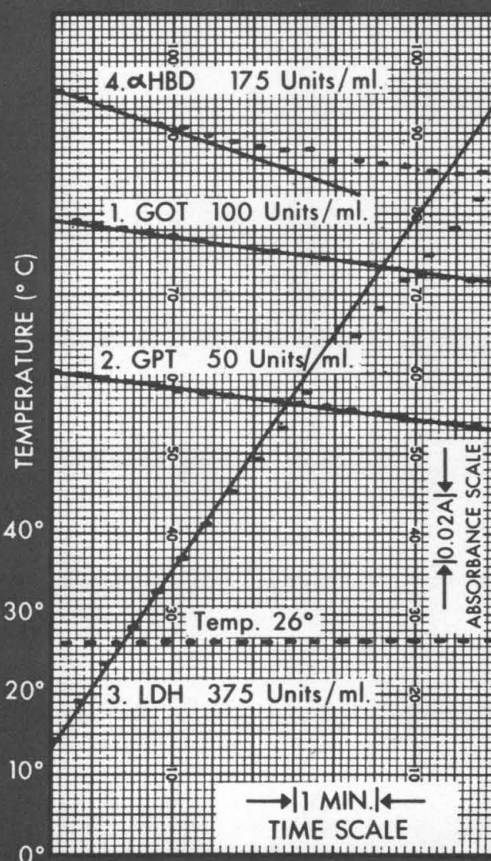

Enzyme Assays from Standardized Human Test Serum. Chart is from the Gilford Applications Laboratory, Oberlin, Ohio.

Scientists in hundreds of research laboratories throughout the world have come to depend on Gilford Automatic Spectrophotometers as the standard for a wide range of solution kinetics, including the enzyme reaction rates shown here.

Gilford Instruments have won acceptance because their accuracy is of a high order, and in addition they are extremely versatile. Gilford Spectrophotometers measure Absorbance directly — not percentage transmission converted to Absorbance. Thus, their accuracy is not limited to the small central portion of the scale, but has a fully usable range of 0 to 3 A with high accuracy anywhere in this range.


Gilford Spectrophotometers provide a digital display, reflecting their high sensitivity and resolution — direct readings to 0.001 A. Full scale recording is easily established anywhere in the 0 to 3 A range. The Gilford Photometric System is extremely stable; drift is less than 0.005 A per hour. Fewer "returns to reference" are needed.


The typical group of serum assays shown at left includes Glutamic Oxalacetic Transaminase (SGOT), Glutamic Pyruvic Transaminase (SGPT), Lactic Dehydrogenase (LDH) and α -Hydroxybutyric Dehydrogenase (α -HBD) — with a fifth trace for temperature. With the Gilford Offset Control, it is possible readily to separate the four recording traces, thus assuring clear, error-free recordings. True linear slopes can be determined from one-minute intervals, avoiding the need for averaging rates over long fixed time intervals.

In selecting a Gilford Automatic Spectrophotometer, you will find a wide range of "building blocks" available. These include a number of sample handling systems, including flow-through cells, temperature control and sensing units, dual wavelength mechanisms and others. With Gilford equipment, you get what you need to do today's jobs, and it will have the inherent adaptability so important in meeting your spectrophotometric assay problems of tomorrow.


Write for full information on Gilford Spectrophotometers.
Gilford Instrument Laboratories, Inc. • Oberlin, Ohio 44074

gilford®

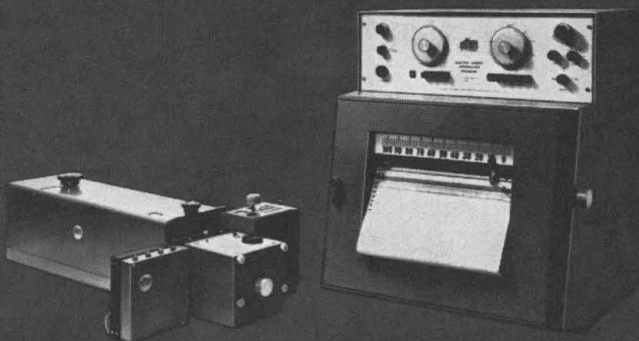

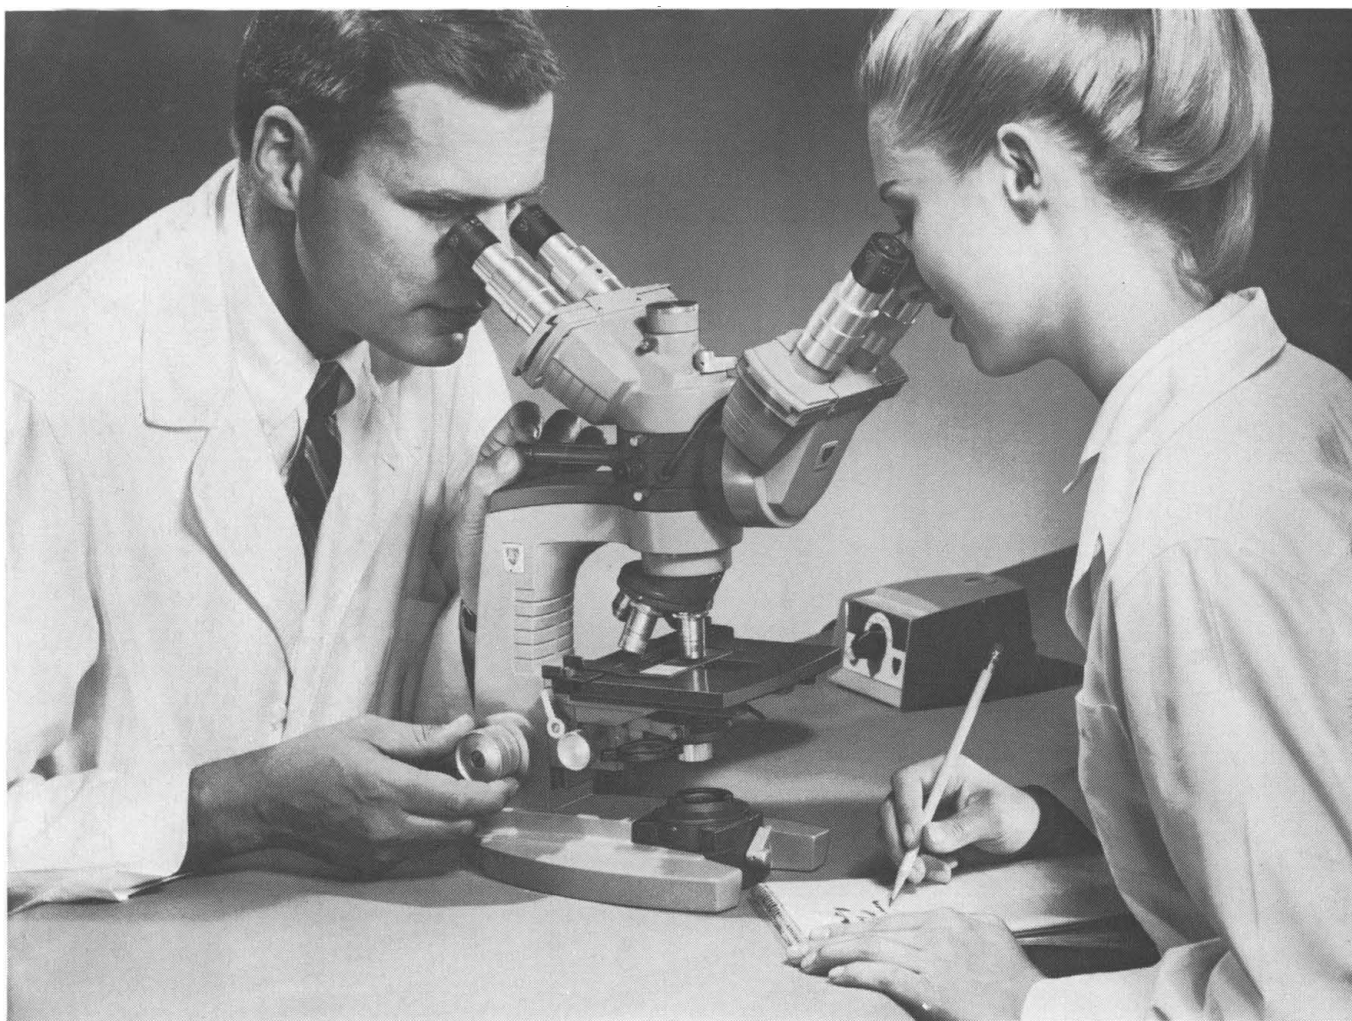

AO Dual Viewing Microstar® for more effective communication

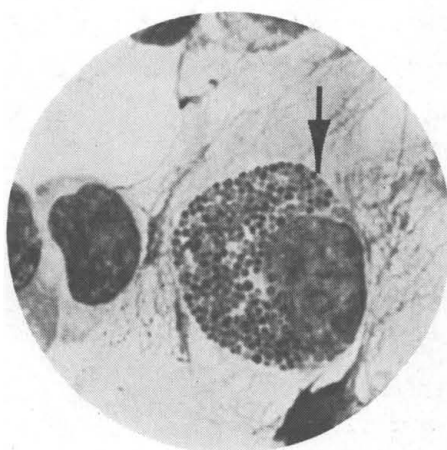

Two people can see the same image simultaneously without sacrificing image quality, adjustment time or superb operating convenience.

Each viewer enjoys the same sharp image over the entire field. The Microstar Microscope's unique infinity-corrected optical system eliminates blurred and fuzzy edges.

For cross-reference, an illuminated, transparent pointer is superimposed on the field. It can be positioned instantaneously to pinpoint specific slide areas or minute details of the specimen.

The Autofocus stop saves every-

® Registered Trademark American Optical Company

body's time . . . eliminates wasted motion. It simplifies coarse adjustment so that perfect focus is merely a matter of touching up the fine adjustment. And, since the nosepiece is gravity-loaded, it's practically impossible for you to break slides or to damage the objective.

Applications are unlimited—for a second opinion, immediate verification, continuous observation or routine lab training. Whenever accurate communication is essential, consider the AO Dual Viewing Microstar.

For more information, call your AO Sales Representative or write.



AMERICAN OPTICAL COMPANY
INSTRUMENT DIVISION • BUFFALO, NEW YORK 14215