

The Rabbit. A Practical Guide. T. A. G. Wells. Dover, New York, 1968. x + 74 pp., illus. Paper, \$1.35. Reprint of the 1964 edition.

Raspail. Scientist and Reformer. Dora B. Weiner, with a chapter by Simone Raspail. Columbia University Press, New York, 1968. xvi + 336 pp., illus. \$11.

The Rat. A Practical Guide. T. A. G. Wells. Dover, New York, 1968. viii + 77 pp., illus. Paper, \$1.35. Reprint of the 1964 edition.

Reactivity of the Photoexcited Organic Molecule. Proceedings of the 13th conference on chemistry, Brussels, October 1965. Solvay Institute of Chemistry. Interscience (Wiley), New York, 1967. x + 350 pp., illus. \$15.

Reagent Grade Water: How, When and Why? Martha Winstead. American Society of Medical Technologists, 1967. x + 142 pp., illus.

Recent Advances in Biological Psychiatry. Vol. 10. Proceedings of the 22nd Annual Convention and Scientific Program of the Society of Biological Psychiatry, Detroit, Mich., May 1967. Joseph Wortis, Ed. Plenum, New York, 1968. xvi + 328 pp., illus. \$19.50.

Sixth Turkish Ophthalmological Congress. Ankara, Oct. 1966. Kardes Matbaasi, Ankara, 1967. 489 pp., illus.

Soil and America's Future. Proceedings of the 22nd annual meeting of the Soil Conservation Society of America, Des Moines, Iowa, Aug. 1967. Soil Conservation Society of America, Ankeny, Iowa, 1967. Paper, \$5.

Source Book in Chemistry 1900-1950. Henry M. Leicester, Ed. Harvard University Press, Cambridge, Mass., 1968. xx + 408 pp., illus. \$11.95.

South of Yosemite. Selected writings by John Muir. Frederic R. Gunsby, Ed. Photographs by Philip Hyde. Sketches by John Muir. Published for the American Museum of Natural History by the Natural History Press, Garden City, N.Y., 1968. xviii + 269 pp. \$7.50.

The Speech Writing Guide. Professional Techniques for Regular and Occasional Speakers. James J. Welsh. Wiley, New York, 1968. xiv + 128 pp. \$5.95.


Uniformity and Simplicity. A Symposium on the Principle of the Uniformity of Nature, Nov. 1963. Claude C. Albritton, Jr., Ed. Geological Society of America, New York, 1967. x + 99 pp., illus. Paper, \$4.50.

Vector and Tensor Analysis with Applications. A. I. Borisenko and I. E. Tarapov. Revised and translated from the third Russian edition (Moscow, 1966) by Richard A. Silverman. Prentice-Hall, Englewood Cliffs, N.J., 1968. xii + 257 pp., illus.

Weatherability of Plastic Materials. Proceedings of a symposium, Gaithersburg, Md., Feb. 1967. Musa R. Kamal, Ed. Interscience (Wiley), New York, 1967. viii + 306 pp., illus. Paper, \$7.95.

Work-a-Text in Earth Science. Robert L. Stanger. Jack Robbins, Ed. Cambridge Book Co. (Cowles Communications), Bronxville, N.Y., 1967. viii + 247 pp., illus. Paper, \$1.35.

Work-a-Text in Life Science. Robert L. Stanger. Jack Robbins, Ed. Cambridge Book Co. (Cowles Communications), Bronxville, N.Y., 1967. xvi + 234 pp., illus. Paper, \$1.35.

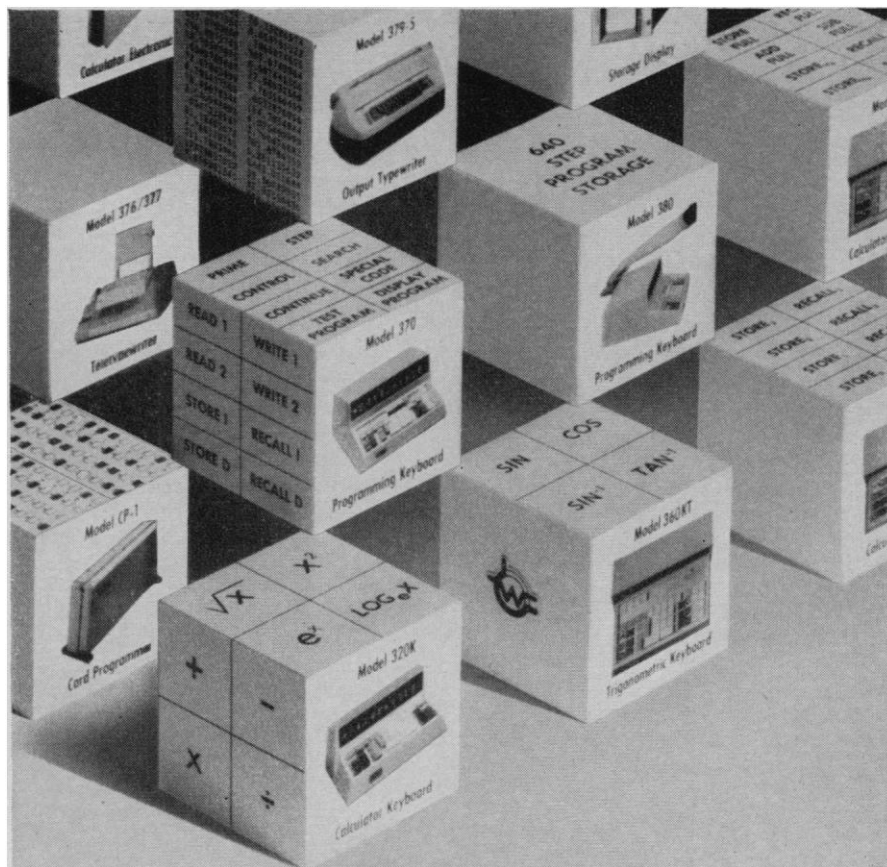

WANG'S versatile, expandable calculator/computing systems

A unique building-block approach.

You can specify the exact amount of power and versatility you need from a wide range of optional capabilities. (Wang offers more than all other electronic calculator manufacturers combined.)

Obsolescence-proof problem solving.

Begin as simply as budget and requirements dictate. Add-on compatibility ensures that your initial purchase is never obsolete. Simply add modular capabilities to match your needs.

You can standardize on 300 Series.

A growing number of companies use them to solve everything from basic arithmetic computations to complex equations and program-

med calculations. Models 370 and 380 Programming Keyboards branch, loop, do sub-routines, make decisions and manipulate arrays to put true desk top computing power at your fingertips. Each is furnished with the most comprehensive program library available.

No waiting for computer time.

Direct accessibility and immediate results on Wang 300 Series enable you to proceed directly to the important areas of analyzing and applying the information generated. Complete Wang systems can be purchased at less cost than renting a larger, less versatile system for 1 year. For application assistance or an immediate demonstration, call your nearest Wang office.




Dept. 6Q, 836 North St., Tewksbury, Massachusetts 01876 • Tel. 617 851-7311

In Major Cities, Tel:

(201) 241-0250	(215) 642-4321	(313) 278-4744	(412) 366-1906	(514) 482-0737	(702) 735-5802
(203) 666-9433	(216) 333-6611	(314) 727-0256	(415) 454-4140	(518) 463-8877	(713) 668-0275
(205) 245-6057	(301) 588-3711	(317) 631-0909	(416) 364-0327	(601) 234-7631	(714) 234-5651
(206) 622-2466	(301) 821-8212	(319) 365-2966	(504) 729-6858	(612) 881-5324	(716) 381-5440
(212) 682-5921	(303) 364-7361	(402) 341-6463	(505) 255-9042	(614) 488-9753	(717) 397-3212
(213) 278-3232	(305) 841-3691	(404) 457-6441	(512) 454-4324	(617) 851-7311	(816) 421-0890
(214) 361-4351	(312) 456-1542	(405) 842-7882	(513) 531-2729	(702) 322-4692	(817) 834-1433
					(919) 288-1695


NEW! BUCHLER UNIVERSAL DENSITY GRADIENT MIXER PERMITS GRADIENTS FROM 5 to 50 ml WITHIN THE SAME MIXER

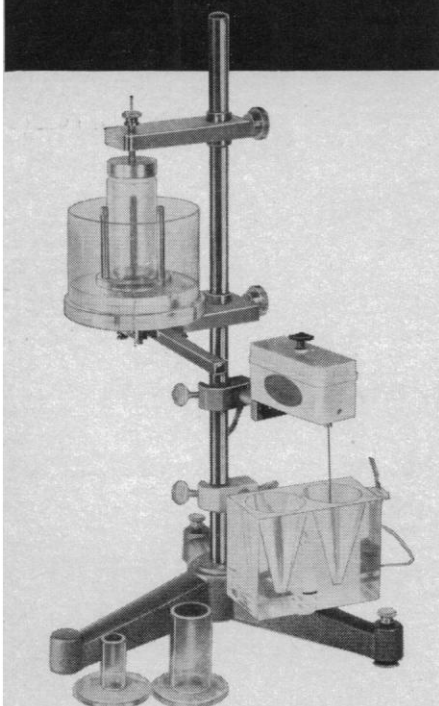

A GRADIENT SEDIMENTATION SYSTEM FOR THOSE WHO MUST VARY VOLUME FREQUENTLY!

● Prepare 5, 30 or 50 ml gradients with a single unit. ● Chambers available for single or triple gradient mixing. ● Piercing unit—with adapters to hold all commercially available centrifuge tubes. ● Precision bore conical chambers with interconnecting stopcock. ● Vibration type stirrer with adjustable speed. ● Pumps, UV monitors and fraction collectors to form complete system.

Request Buchler Bulletin S2-5100.

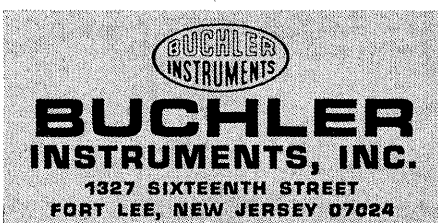

Index of Advertisers

21 June 1968

Ames Co.	1283
Beckman Instruments, Inc.	1273
Bio-Rad Laboratories	1378
Blackstone Ultrasonics, Inc.	1373
Blickman, S., Inc.	1370
Buchler Instruments, Inc.	1386
Clevite Corp., Brush Instruments Div.	1369
Coors Porcelain Co.	1376
Fisher Scientific Co.	1272
Gilson Medical Electronics	1292
Heat Systems-Ultrasonics, Inc.	1372, 1382
Honeywell, Test Instruments Div.	1277
Infotronics Corp.	1371
Instrumentation Associates, Inc.	1383
Instrumentation Laboratory, Inc.	1281
Instrumentation Specialties Co., Inc.	1376
Interscience Publishers, Div. of John Wiley & Sons, Inc.	1384
Intertechnique Instruments Inc.	1284
Klett Manufacturing Co., Inc.	1379
Labconco Corp.	1383
Labindustries	1288
LaPine Scientific Co.	1374, 1383
LKB Instruments Inc.	1286
Maryland Plastics, Inc.	1276
Materials Analysis Co.	1280
Matheson Co.	1278
Mercer Glass Works, Inc.	1373
Millipore Corp.	1374
Nalge	1381
Nuclear-Chicago Corp.	1288
New Brunswick Scientific Co.	1379, 1387
Ohaus Scale Corp.	1374
Orion Research Inc.	1289
Packard Instrument Co., Inc.	1294
Paillard Inc.	1279
Parr Instrument Co.	1374
Percival Refrigeration & Mfg. Co., Inc.	1379
Pharmacia Fine Chemicals, Inc.	1291
Professional Tape Co., Inc.	1383
Schleicher & Schuell Co.	1380
Scientific Glass Apparatus Co., Inc.	1377
Shandon Scientific Co., Inc.	1370
Technical Instruments, Inc.	1389
Technicon Corp.	1282
Thomas, Arthur H., Co.	1390
Tracerlab	1384
Wang Laboratories, Inc.	1385
Whittaker Corp.	1378
Wilkens-Anderson Co.	1386
Worthington Biochemical Corp.	1375
Yellow Springs Instrument Co.	1380
Zeiss, Carl, Inc.	1285




No other power stirrer made will give you as much service per dollar. And that's continuous 24 hour service, 7 days a week for months at a time! The Waco motor is not a stock item converted to a stirrer, but a sparkless — induction type motor specifically designed for laboratories where long, continuous use is required. A built-in cooling fan eliminates overheating or burning out.

86100—WACO Power Stirrer, with tubular brass mounting rod and 6 foot cord ... only **\$33.70**
Stirrer chucks, \$2.25 ea., set of three stirring rods (small, medium, large), \$9.30.

Order direct or write for descriptive folder.

Laboratory Supplies and Equipment
wilkens-anderson co.
4525 W. Division St., Chicago, Ill. 60651

Count Colonies Automatically!

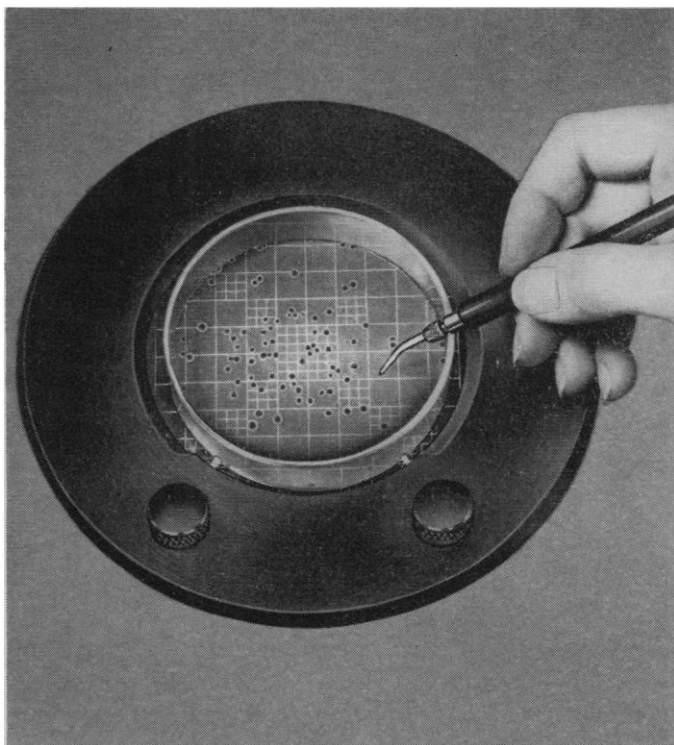

Bacterial colonies can be recorded quickly and accurately in a *single* probing action with the Bactronic Colony Counter, which marks as it counts automatically in open and closed petri dishes. An electronic probe picks up radio impulses on contact with *any* agar medium, actuates the counting mechanism, and leaves an identifying puncture in the agar. If puncturing is undesirable, a plug-in marking pen or grease pencil can be used to mark the back of the plate as it counts. A special system of illumination floods the plate with uniform, glare-free light that accentuates colonies in bold relief. Even pin-point colonies are clearly discerned. This transistorized instrument is equipped with a Sterilizing Probe Well, automatic numerical reset to zero and magnifying lens.



Send for Catalogue C110S/6218



NBS New Brunswick Scientific Co., Inc.
1130 Somerset Street, New Brunswick, New Jersey 08903

Personnel Placement

POSITIONS WANTED

Biomedical Instrumentation: Research Director, Ph.D. Biochemist. Dynamic, young technical executive seeks challenging and responsible position with good growth potential. Broad industrial research experience including drug metabolism, enzymology, clinical chemistry, analytical automation, data processing. Publications and proven performance record. Prefers metropolitan area in Northeast, Florida, or California. Box 234, SCIENCE. 6/21

Ph.D. Analytic Biochemist. Training in clinical biochemistry and cancer research. Desires responsible senior staff position, fundamental and applied with university, institute, or industrial complex. College teaching and industrial experience; Publications. Box 235, SCIENCE. X

Business Administrator, medical college, business and government experience. Minimum \$15,000. Box 236, SCIENCE. X

Biological Chemist, M.S., male, age 28, 5 years of research experience, diversified background. Wants to relocate, West Coast preferred. Box 237, SCIENCE. X

D.M.D. 2 years of postdoctoral study—research, developmental biology. Desires position, teaching, research or industrial affiliation. Box 238, SCIENCE. 6/28

Literature Scientist and Administrator. Doctorate, publications; 15 years' experience as laboratory director, researcher, editor, abstracter; biology, chemistry, clinical laboratory, and related health sciences. Northeastern United States. \$20,000–\$25,000. Box 239, SCIENCE. X

Physics-Mathematics. Ph.D. Publications. Seeks teaching/research position with opportunity to pursue own research interests. Box 242, SCIENCE. 6/28

POSITIONS WANTED

Pharmacology Ph.D. Veteran. Teaching experience medical and undergraduate school, publications, seeks teaching/research/administrative position pharmacology/physiology/biology. Available September. Box 241, SCIENCE. 6/28

Senior Research Biochemical Pharmacologist, Ph.D.; 11 years' postdoctoral experience in drug enzymology, biochemical pharmacology, toxicology, biochemistry, site and mode of action of drugs and toxic agents in central nervous system and other tissues. Industrial, governmental, university, and supervisory experience. Seeks mutually rewarding position in research or research administration. Box 240, SCIENCE. X

Ph.D. Broad investigative career in microbiology, biochemistry, oncology, and cell biology, seeks nonindustrial appointment in research, teaching, or administration. Washington, D.C., area preferred, but not obligatory. Will travel. Box 243, SCIENCE. X

Gross Anatomist (M.D. 1944; D.D.S. 1960), 17 years' experience of teaching human anatomy to medical, dental, and graduate students (emphasis on gross anatomy). Main research interest in quantitative morphology, especially at macroscopic level. Publications and monographs. Seeks senior faculty position, preferably in the East. Available early 1969. In replying refer to Box 244, SCIENCE. X

POSITIONS OPEN

Clinical Audiologist: Washington, D.C. area: \$9657–\$12,555. Retirement, sick and annual leave, group life insurance, hospital and medical plans are some of the many U.S. Civil Service Commission fringe benefits available; duties include complete audiological evaluations with all ages, hearing aid evaluations and fitting, auditory training, speech and/or language rehabilitation, some supervision of graduate intern program, lip reading classes for all ages and auditory training; work mainly with geriatric adults using comprehensive audiometric equipment.

Qualifications and Experience: MS; two years clinical experience; CCC Aud.; prior supervision in research. Available immediately. Send application to: Recruiting Officer, D.C. Department of Public Health, Personnel Office, STOP 40, 801 North Capitol Street, N.E., Washington, D.C. 20001

POSITIONS OPEN

M.S. Bacteriologist. Diagnostic microbiology for progressive hospital, 1500-bed capacity, with new laboratories and school of Medical Technology, located in medical center complex. Experience preferred, but not required. Relocation expenses provided. Reply to Personnel Director, Baptist Memorial Hospital, Memphis, Tennessee.

BIOPHYSICIST—To assist a physiatrist, head of a department of PM&R, also cooperating with the University of Pa. Medical School, in a medical research program. Duties include active assistance in medical research projects and in development of new medical instrumentation. Starting salary \$10,623 or higher based on qualifications. Exceptional fringe benefits. Located in large federal government hospital near Hershey, Pa., 1½ hours from Phila. by turnpike. Non-discriminatory employer. Contact **Personnel Office, VA Hospital, Lebanon, Pa. 17042.**

CLINICAL/ANALYTICAL BIOCHEMIST, Ph.D.

Recent Ph.D. in bio or analytical chemistry desired for varied professional work including clinical chemistry, toxicology, method development, residue studies. Send résumé to **L. E. Loveless, Ph.D., Clinical Laboratories, 100 N. Euclid, St. Louis, Missouri 63108.**

MARINE SCIENTISTS

Active center for research and education in Marine Science seeks scientists qualified at doctoral and magisterial levels to fill newly created research and graduate teaching positions. Areas of special interest are marsh ecology, shellfish biology, marine microbiology, productivity of coastal and estuarine waters, marine parasitology, pollution biology, sanitary engineering and coastal engineering. Location, mid-Atlantic state near large centers of population. Salaries and fringe benefits competitive. Address letters and résumés to: Box 229, SCIENCE.

POSITIONS OPEN

PHARMACOLOGIST/PHYSIOLOGIST

• Reproductive Studies •

Our expanding research program has created need for Ph.D. level scientist to head section with responsibilities for teratological investigations in rats & rabbits as well as routine toxicity studies. Prefer candidate with some experience.

Excellent environment for interdisciplinary exchange provided. Creative thinking & exploratory experimentation encouraged.

In confidence kindly send curriculum vitae to Personnel Manager, Research

Schering

SCHERING CORPORATION

Bloomfield, New Jersey 07003

A Plans for Progress Company

Biochemist, Ph.D. Canadian Dental Faculty invites applications for a position, the principle duty of which would be to assist in the teaching of biochemistry and applied pharmacology to dental students. The appointment is open on July 1st, 1968, at the Associate Professor level with a yearly salary between \$13,000 and \$17,500. Adequate research facilities in an established laboratory are available. A dental degree is not necessary. Inquiries should be addressed to: **Professor K. A. McMurchy, Head, Basic Science Department, Faculty of Dentistry, University of Alberta, Edmonton, Alberta, CANADA.**

CLINICAL RESEARCH

Ph.D. in biological sciences to participate in program of clinical evaluation of new drugs. Studies of efficacies, safety and mechanism of action, collaborate in experimental design, data analysis and final reports.

Excellent salary and benefits.

Submit your resume to:

Director of Clinical Pharmacology

SANDOZ, INC.

Route 10 Hanover, N.J.

An Equal Opportunity Employer

Wanted—experienced lab worker for research position in red blood cell metabolism. Bachelor's degree, biochemistry and references are essential. Contact **Dr. Joel Schwartz, Coney Island Hospital, Ocean and Shore Parkways, Brooklyn, New York 11235. SH 3-4100, extension 249.**

Program of Interdisciplinary research into the activity patterns of children in the free range needs a **Life Scientist** as a member of the team. Recruit would work in Children's Research Center, a division of the Graduate College of the University of Illinois, and would be expected to work without supervision. Ph.D. preferred, however, candidates for the Ph.D. will be considered. Write: **M. J. Ellis, Assistant Director, Motor Performance Laboratory, Children's Research Center, Champaign, Illinois 61820.**

ACADEMIC PATHOLOGIST

Position involves chiefly teaching and research, with limited service responsibility. Opportunities for independent or collaborative investigation. Rank according to qualifications. Attractive salary and fringe benefits. Contact **Doctor Joseph A. Sisson, Chairman, Department of Pathology, Creighton University School of Pathology, Creighton University School of Medicine, 2500 California Street, Omaha, Nebraska 68131.**

POSITIONS OPEN

PHARMACOLOGIST

Research position available in our Reproductive Research Section. This position will involve the design and performance of biochemical experiment on the regulation of reproduction and embryonic development. Candidates should have a M.S. or B.S. in Chemistry or Biology with some instrumentation experience.

If interested send resume in confidence to Mr. Richard Groben

ORTHO

PHARMACEUTICAL CORP.

Route 202 Raritan, NJ 08869

An Equal Opportunity Employer

A position as a **Radiobiologist** for the Division of Radiation Therapy is open at John Sealy Hospital, University of Texas Medical Branch, Galveston, Texas. This division is brand new with a fairly well-equipped radiobiology laboratory. This position will require a Ph.D. in Biophysics or in Physical Chemistry. Work will be centered around radiobiology research and teaching on our campus. The position will hold academic rank and full-time faculty membership. Approximately two-thirds of the work will be research and one-third will be teaching. The work will be mainly experimental in connection with cancer research applied to Radiation Therapy. Salary will be \$15,000-20,000 per year, depending upon experience.

WRITER-EDITOR for a top magazine for family doctors. Contact own sources, do own research, follow up. \$12-15,000. Some travel. Send resume, samples to **Bernard Weiss, Managing Editor, Patient Care, 1 Bank Street, Stamford, Connecticut 06901.**

POSITIONS OPEN

PLASTICS PRODUCTION MANAGER

A New York area firm specializing in plastic reproductions of fossil osteological material is seeking a production manager. The ideal candidate would have experience and competence in plastic production methods as well as the ability with an open and active mind to approach specialized quality control problems inherent in the large-scale reproduction of complex shapes and surfaces. Intelligence and enthusiasm, especially if coupled with a degree in mechanical or industrial engineering, could be substitutes for experience. Salary open. All replies held in strictest confidence. Please submit resume to:

Box 228, SCIENCE

NIH Traineeship in Developmental Immunology offered to M.D.'s and Ph.D.'s interested in developing a career of independent research and academic medicine. Laboratory part of medical center in prime educational area. Degree program possible. Stipend commensurate with level of training. Contact: **Joseph A. Bellanti, M.D., Department of Pediatrics, Georgetown University Medical Center, Washington, D.C. 20007.**

PROTEIN STRUCTURE RESEARCH

Several positions open at postdoctoral level for work in protein separations, characterization, and sequence analysis. New program. Development of techniques emphasized. Resume to: **J. E. Sergeant—Oak Ridge National Laboratory Union Carbide Corporation—Nuclear Division P. O. Box X Oak Ridge, Tennessee 37830**

The Market Place

BOOKS • SERVICES • SUPPLIES • EQUIPMENT

WRITERS

N. Y. publisher wants books on all subjects, fiction, nonfiction. No fee for professional opinion. FREE: Brochures that show how your book can be published, publicized, sold; contracts. Write Dept. 75 F

EXPOSITION PRESS INC.
386 Park Ave. So., New York, N. Y. 10016

EXPOSITION PRESS INC.
9172 Sunset Blvd., Los Angeles, Cal. 90069



HISTOLOGY SERVICE joined **LAWDALE LABORATORY** to provide Reliable, Accurate & Fast Service with Quality Control at LOW UNIT COST for:

- * Full Range Histology Studies.
- * Chemical Analysis for Toxicology Studies.
- * Biochemical Profile Studies.
- * Specialized & Routine Chemistry Tests.

6190 RISING SUN AVE., PHILA., PA. 19111
Phone (215) RA 5-5103


SPRAGUE-DAWLEY, INC.

Pioneers in the development of the **STANDARD LABORATORY RAT.**

P.O. Box 4220

Madison, Wisconsin

CE 3-5318



SPECIAL NUCLEAR SHIELDING

CHEMTREE CORPORATION
Central Valley, N.Y.
914-928-2293

ON-LINE, ON-LINE, ON-LINE ANALYSIS

**Mnemotron CAT systems
from TECHNICAL INSTRUMENTS, INC.**

Whatever your application — we have the building blocks

CAT® — 1000 COMPUTER of AVERAGE TRANSIENTS

For on-line data reduction . . . offers increased resolution for signal averaging and histogram applications . . . 1024 address memory provides significant increase in resolution . . . permits accurate analysis of transients having long durations and continuing high frequency components.

CAT® 400C

CAT® 400C for on-line isolation of specific signal responses masked by background noise . . . histogram and correlation capabilities . . . external add/subtract . . . readout capability to plotters and various types of digital devices.

CORRELATION COMPUTERS MODELS 257 and 258

Employs both analog and digital techniques to determine the auto-correlation and cross-correlation function of electrical signals . . . computes up to 256 points of correlation function simultaneously . . . correlator system contains provisions for statistical analysis in both the amplitude and frequency domains.

HISTOGRAM ACCESSORIES

For on-line analysis of interval, dwell time, latency, amplitude distribution and the amplitudes frequency. The models 605, 606, 607, 610 and 646 enables the user to select this type of analysis sequentially and non-sequentially.

SWEEP ACCESSORIES

Model 646 permits the user to dial in the number of sweeps to be averaged. This versatile accessory indicates visually as the number is running down.

Model 609 sampling unit provides more than 3,000% increase in maximum effective sweep speed of CAT 1000 computer . . . reduces effective dwell time of CAT system to one microsecond per data point . . .

READOUT CONTROL MODEL 520B

Engineered for use with the CAT to provide maximum readout flexibility in average, histogram, and correlation modes — Model 520B Type-punch-read control unit contains parallel-to-serial conversion circuits for transferring information stored in the CAT memory into format suitable for input to a tape punch or typewriter.

RESOLVER/INTEGRATOR MODEL 522A

Multi-purpose data processing unit for expanding application capabilities of the CAT computers . . . can be as a selective readout control unit, resolver or digital integrator . . . resolver mode allows selected memory quarters or halves to be subtracted from (or added to) data stored in any band of memory addresses, in either normal or sub-total integrate mode.

PRINTER MODEL 500A

Is a parallel readout device to operate with the CAT 400 or 1000. By pressing the readout button the printer will record the contents of the memory. Each line of information prints the address and six digits of arithmetic data.



TECHNICAL INSTRUMENTS, INC


A Simkins Industry

For complete information, write Technical Instruments, Inc., 441 Washington Avenue, North Haven, Connecticut.


Thomas

SPECTROPHOTOMETER ACCESSORIES

... reduce analysis time, minimize error

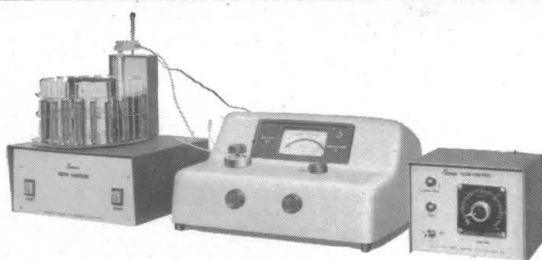

Automatic Sampling Assembly consisting of Thomas 20-tube Roto-Sampler with Suction Pump and Flow Control Timer; for completely automatic transfer of samples to Spectronic 20 Spectrophotometer

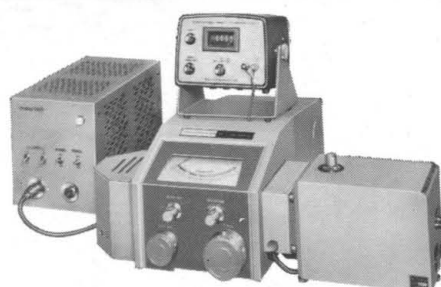

Complete Assembly of Hitachi Perkin-Elmer 139 Spectrophotometer and Thomas Absorbance/Transmittance Readout



Thomas Digital Converter (Printout), for use with Thomas Absorbance/Transmittance or Peak Detector-Concentration Readout



Thomas Flow Cell Adapter for Coleman 101 Spectrophotometer



Thomas Flow Cell Adapter for B. & L. Spectronic 20



Thomas Model 4 Peak Detector-Concentration Readout; reads positive or negative peaks in transmittance, absorbance or concentration units.

Since the appearance of the Hilger Wavelength Spectrometer with Photometer Attachment in the 1914 edition of our general catalog, our Company has been active in the promotion of spectrophotometric instrumentation. We have devised a number of time-saving, mistake-avoiding accessories for many spectrophotometers now in general use. Current models of these accessories are listed in our new Bulletin 153.

All of the Thomas devices, whether simple or sophisticated, are intended to implement existing analytical methods. They can be used with most of the standard spectrophotometers, with the same sample treatment, and with standard 10 mm light path cells. The modular

accessories are directly adaptable to currently employed methods. They can save time and reduce error in data compilation and repetitive manipulations which are capable of being automated. Modular designs offer simplicity, economy and flexibility.

Thomas digital accessories are intended for use with Coleman Model 101 and Hitachi Perkin-Elmer Model 139 Spectrophotometers which have been modified by us for direct hookup to our equipment. A coupler is offered for adapting the electronic regulated Spectronic 20 to our digital equipment. A coupler adapter is also available for Coleman Model 124 Spectrophotometer; Coleman Model 111 does not require any adapter.

Copy of detailed Bulletin 153 sent upon request.
See also Thomas 1968 catalog, pp. 958-993.



ARTHUR H. THOMAS COMPANY

Scientific Apparatus and Reagents

VINE STREET AT 3RD • P.O. BOX 779 • PHILADELPHIA, PA. 19105, U.S.A.